

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101222\
 Data File : PD072377.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 12:15
 Operator : AR\AJ
 Sample : N4950-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB8S0

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/14/2022
 Supervised By : Ankita Jodhani 10/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 00:34:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 06:06:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.710	3.470	22448552	240.7E6	9.197	10.065
27)	SA Decachlor...	7.847	8.928	27530253	113.4E6	14.094	22.441 #
Target Compounds							
10)	B trans-Chl...	4.913	5.870	9608355	90451274	3.163	8.170m#
11)	B cis-Chlor...	4.974	5.935	7861372	58412017	2.675m	5.534m#
12)	B 4,4'-DDE	5.162	6.107	2610114	12965080	0.905m	1.379m#
13)	MA Dieldrin	5.302	6.270	39058139	51100452	13.613	5.360 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101222\
Data File : PD072377.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 12:15
Operator : AR\AJ
Sample : N4950-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 00:34:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 06:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

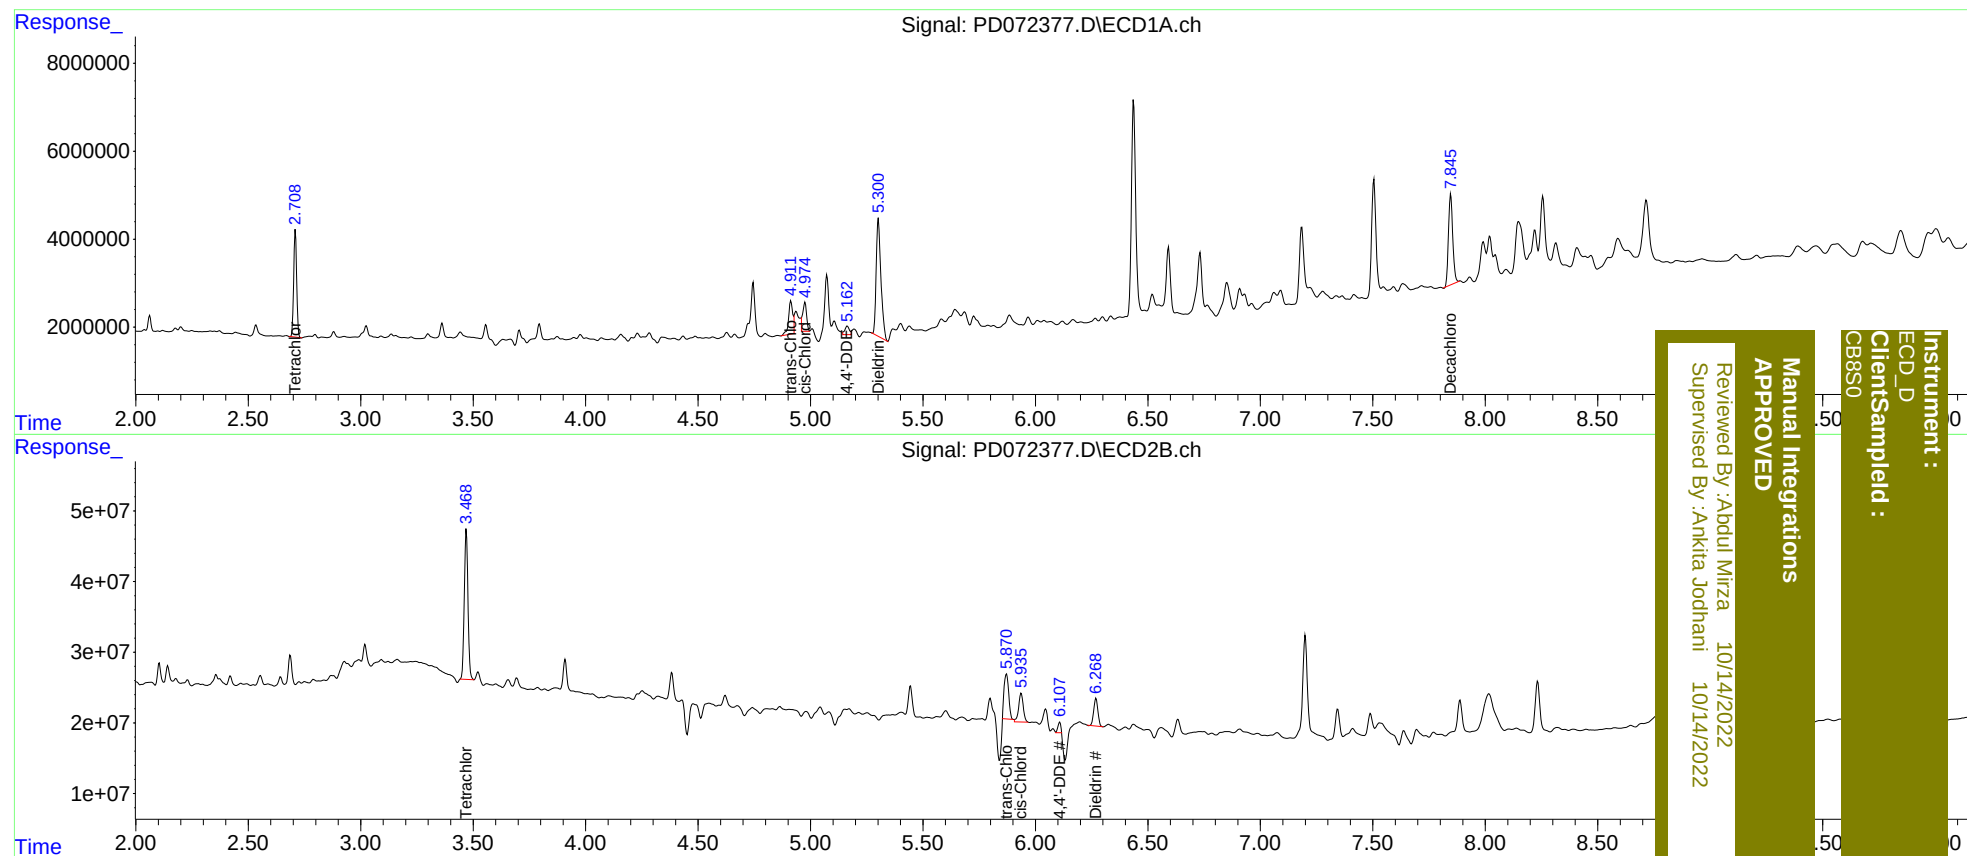

Reviewed By: Abdul Mirza 10/14/2022
Supervised By: Ankita Jodhani 10/14/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
CB8S0