

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101222\
 Data File : PD072378.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 12:29
 Operator : AR\AJ
 Sample : N4950-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB8T0

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/13/2022
 Supervised By : Ankita Jodhani 10/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 00:35:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 06:06:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.710	3.470	32168063	317.7E6	13.179	13.286
2)	SA Decachlor...	7.847	8.927	28906531	659.5E6	14.798	130.569m#
Target Compounds							
3)	MA gamma-BHC...	3.556	4.251	127.5E6	524.3E6	43.092	20.159 #
10)	B trans-Chl...	4.913	5.875	19989474	1977.4E6	6.579	178.615 #
11)	B cis-Chlor...	4.974	5.935	17995125	111.3E6	6.123	10.540m#
13)	MA Dieldrin	5.301	6.270	552.2E6	35633001	192.448	3.738m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101222\
Data File : PD072378.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 12:29
Operator : AR\AJ
Sample : N4950-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 00:35:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 06:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

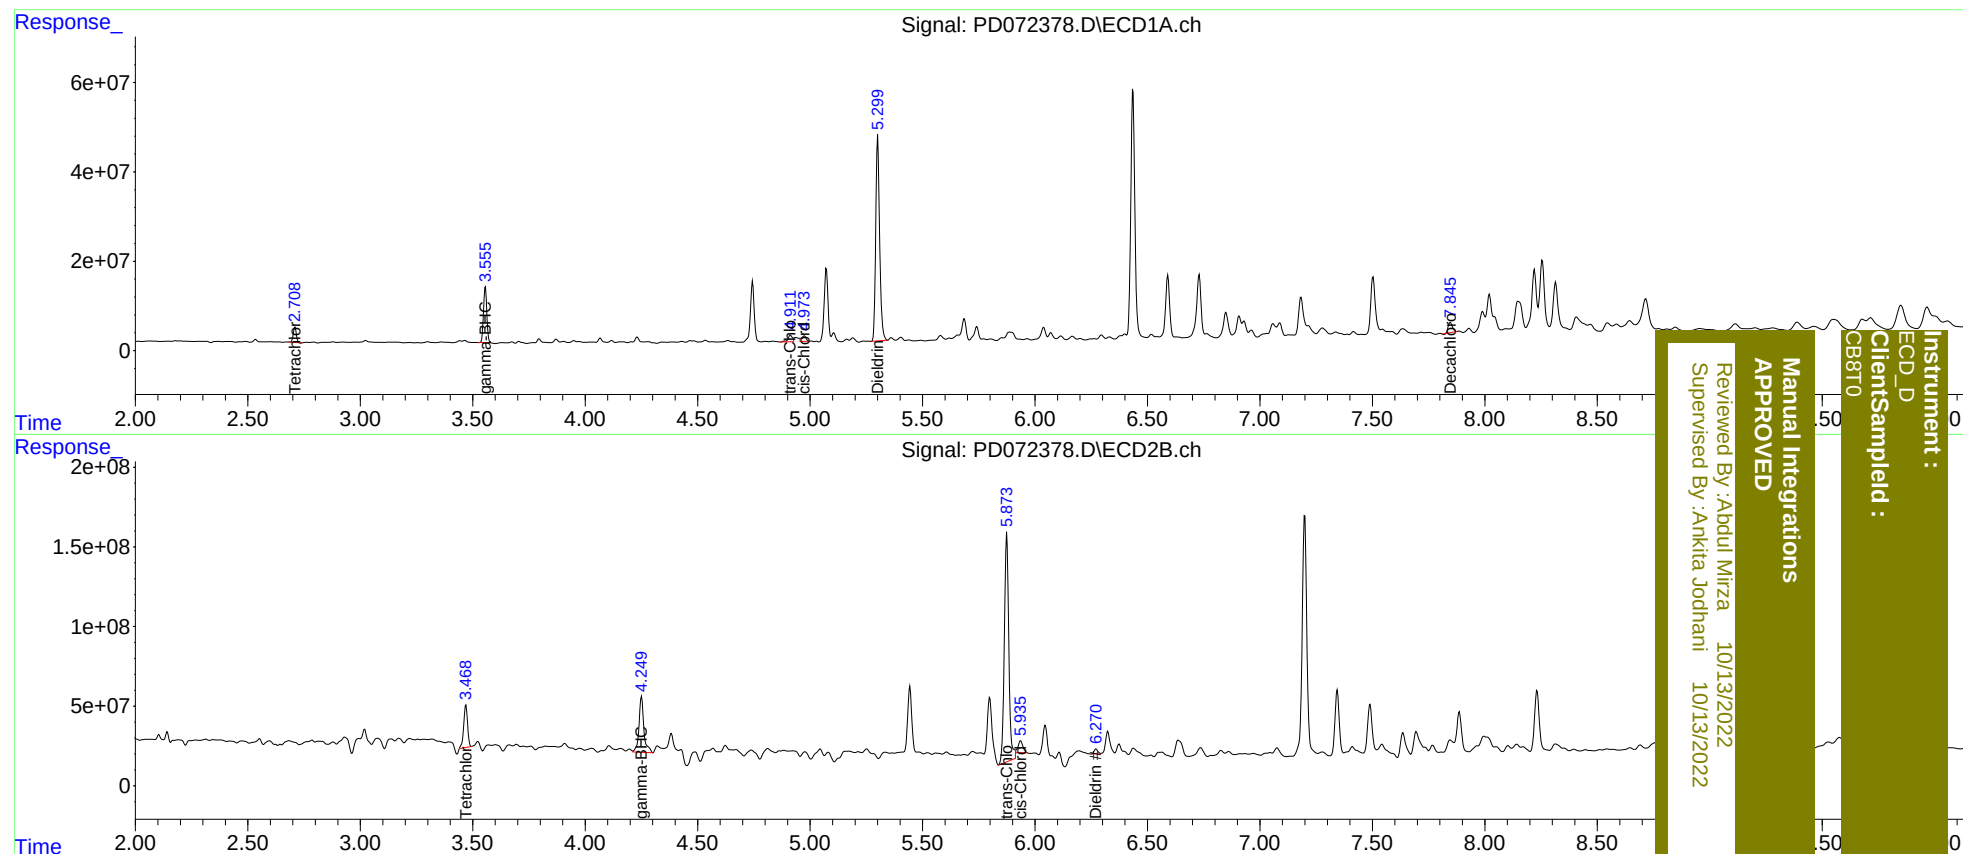

Reviewed By: Abdul Mirza 10/13/2022
Supervised By: Ankita Jodhani 10/13/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
CB8T0