

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101222\
 Data File : PD072379.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 12:42
 Operator : AR\AJ
 Sample : N4950-04MS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB8TOMS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/13/2022
 Supervised By : Ankita Jodhani 10/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 00:36:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 06:06:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.731	3.472	31824207	362.4E6	13.038m	15.153
27)	SA Decachlor...	7.869	8.928	42216867	594.2E6	21.612m	117.646 #
Target Compounds							
2)	A alpha-BHC	3.238	3.936	174.8E6	1405.1E6	48.976	46.422
3)	MA gamma-BHC...	3.571f	4.269	286.5E6	1605.0E6	96.783m	61.707 #
4)	MA Heptachlor	3.870	4.836	68760702	861.0E6	20.986m	50.289 #
5)	MB Aldrin	4.180	5.175	171.6E6	848.8E6	52.177m	58.732
6)	B beta-BHC	3.871	4.485	41801501	568.0E6	27.719	56.292 #
7)	B delta-BHC	4.100	4.729	60285084	433.6E6	17.863m	22.865 #
8)	B Heptachlo...	4.687	5.608	152.7E6	551.4E6	51.412	48.862
9)	A Endosulfan I	5.055	5.991	94626093	483.1E6	36.434m	50.500m#
10)	B trans-Chl...	4.936	5.874	152.5E6	2169.5E6	50.183	195.964 #
11)	B cis-Chlor...	4.998	5.936	151.8E6	605.6E6	51.666m	57.374m
12)	B 4,4'-DDE	5.188	6.110	284.9E6	827.2E6	98.759	87.969
13)	MA Dieldrin	5.323	6.270	821.0E6	938.5E6	286.147m	98.449 #
14)	MA Endrin	5.598	6.501	279.6E6	874.1E6	112.118m	108.937
15)	B Endosulfa...	5.897	6.731	237.6E6	881.9E6	101.346m	122.107
16)	A 4,4'-DDD	5.746	6.635	237.1E6	879.9E6	105.622m	123.544
17)	MA 4,4'-DDT	5.994	6.943	214.6E6	744.5E6	99.505m	110.439
18)	B Endrin al...	6.079	6.863	242.2E6	622.7E6	120.449m	100.965
19)	B Endosulfa...	6.303	7.095	192.4E6	644.2E6	81.218m	94.314
20)	A Methoxychlor	6.578	7.420	581.3E6	2036.0E6	493.879m	634.315m#
21)	B Endrin ke...	6.812	7.585	237.7E6	805.7E6	85.370m	109.693 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101222\
Data File : PD072379.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 12:42
Operator : AR\AJ
Sample : N4950-04MS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 00:36:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 06:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

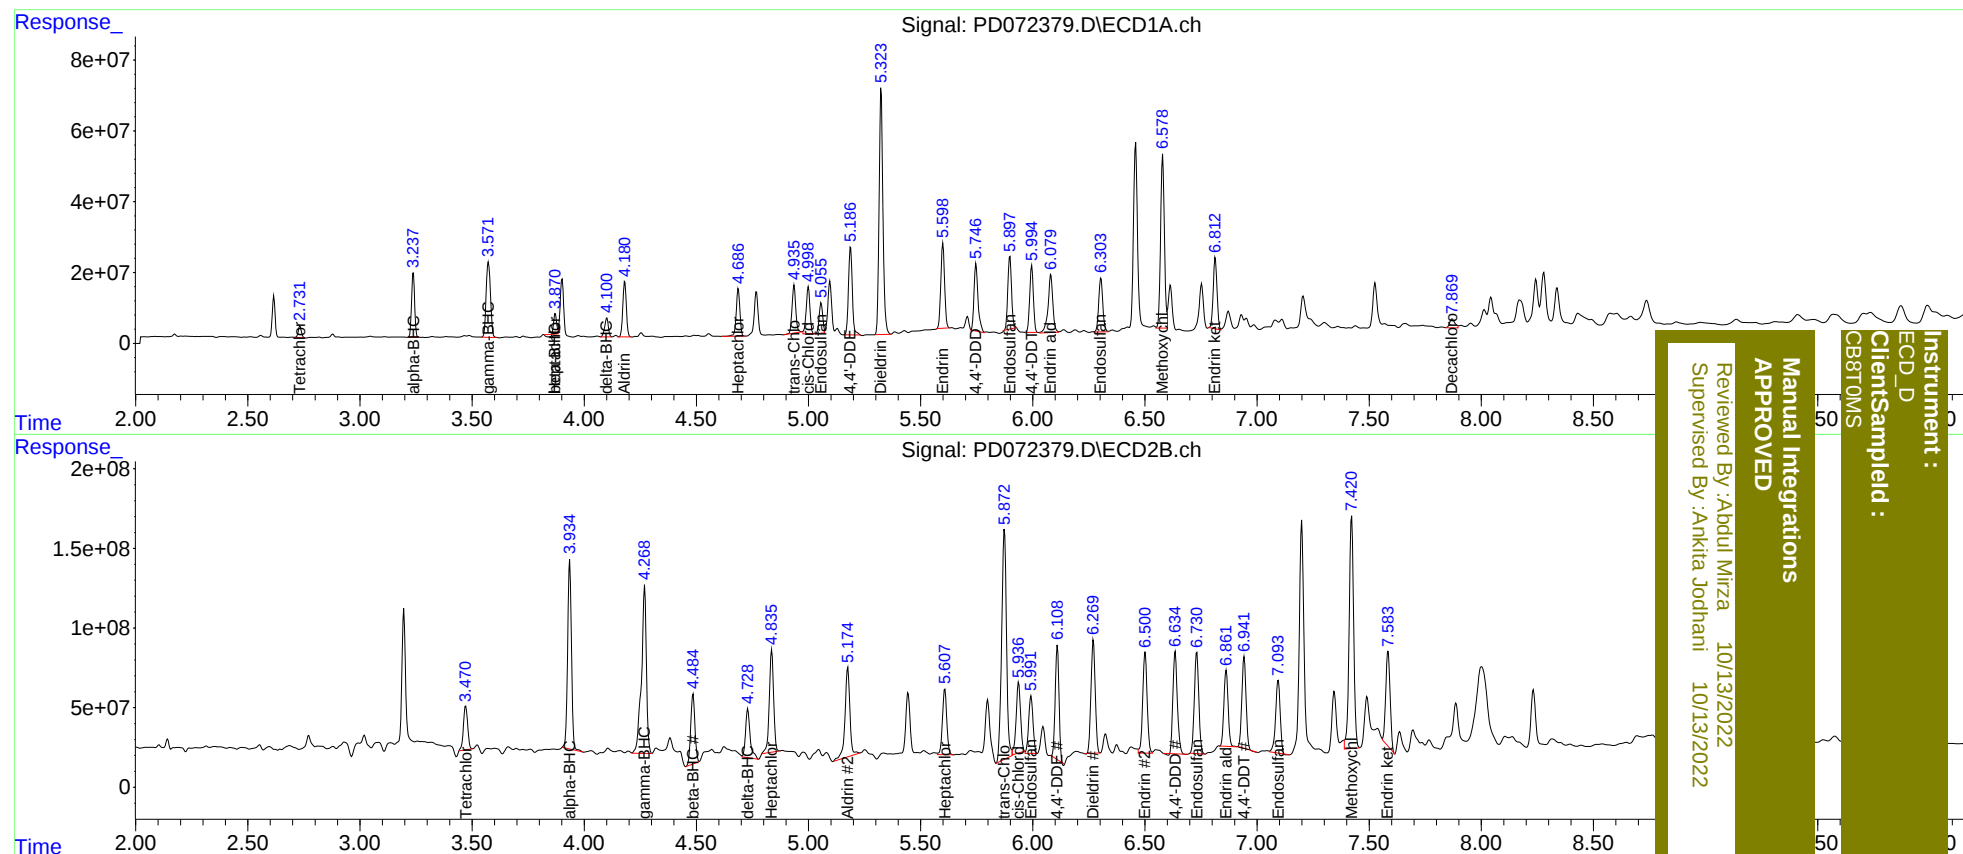

Reviewed By: Abdul Mirza 10/13/2022
Supervised By: Ankita Jodhani 10/13/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
CB8TOMS