

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101222\
 Data File : PD072380.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 12:55
 Operator : AR\AJ
 Sample : N4950-05MSD
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB8T0MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/13/2022
 Supervised By : Ankita Jodhani 10/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 00:36:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 06:06:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.710	3.472	30491786	369.9E6	12.492	15.466
27)	SA Decachlor...	7.846	8.929	30921243	606.6E6	15.830m	120.095 #
Target Compounds							
2)	A alpha-BHC	3.215	3.936	173.0E6	1387.7E6	48.476	45.846
3)	MA gamma-BHC...	3.550	4.270	280.2E6	1589.2E6	94.679	61.102 #
4)	MA Heptachlor	3.878	4.836	178.4E6	838.1E6	54.459	48.952
5)	MB Aldrin	4.158	5.175	172.2E6	824.5E6	52.360	57.056
6)	B beta-BHC	3.848	4.486	65479154	560.5E6	43.421	55.548 #
7)	B delta-BHC	4.078	4.729	62305478	430.3E6	18.462	22.688
8)	B Heptachlo...	4.663	5.608	149.6E6	538.1E6	50.379	47.686
9)	A Endosulfan I	5.033	5.993	96456976	433.6E6	37.139	45.325
10)	B trans-Chl...	4.912	5.874	166.6E6	2153.1E6	54.838	194.483 #
11)	B cis-Chlor...	4.976	5.935	153.7E6	556.4E6	52.309	52.713m
12)	B 4,4'-DDE	5.164	6.110	294.4E6	810.7E6	102.023	86.218
13)	MA Dieldrin	5.301	6.270	811.6E6	909.6E6	282.867	95.418 #
14)	MA Endrin	5.576	6.502	272.0E6	825.9E6	109.101	102.934
15)	B Endosulfa...	5.875	6.731	269.0E6	863.1E6	114.735	119.498
16)	A 4,4'-DDD	5.723	6.635	233.2E6	863.2E6	103.868m	121.205
17)	MA 4,4'-DDT	5.972	6.943	209.4E6	722.7E6	97.076	107.201
18)	B Endrin al...	6.058	6.863	215.8E6	599.9E6	107.292	97.270
19)	B Endosulfa...	6.282	7.096	182.7E6	639.2E6	77.099	93.571
20)	A Methoxychlor	6.556	7.421	560.1E6	1966.1E6	475.877	612.535m#
21)	B Endrin ke...	6.790	7.585	230.4E6	803.3E6	82.741	109.375 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101222\
Data File : PD072380.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 12:55
Operator : AR\AJ
Sample : N4950-05MSD
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 00:36:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 06:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

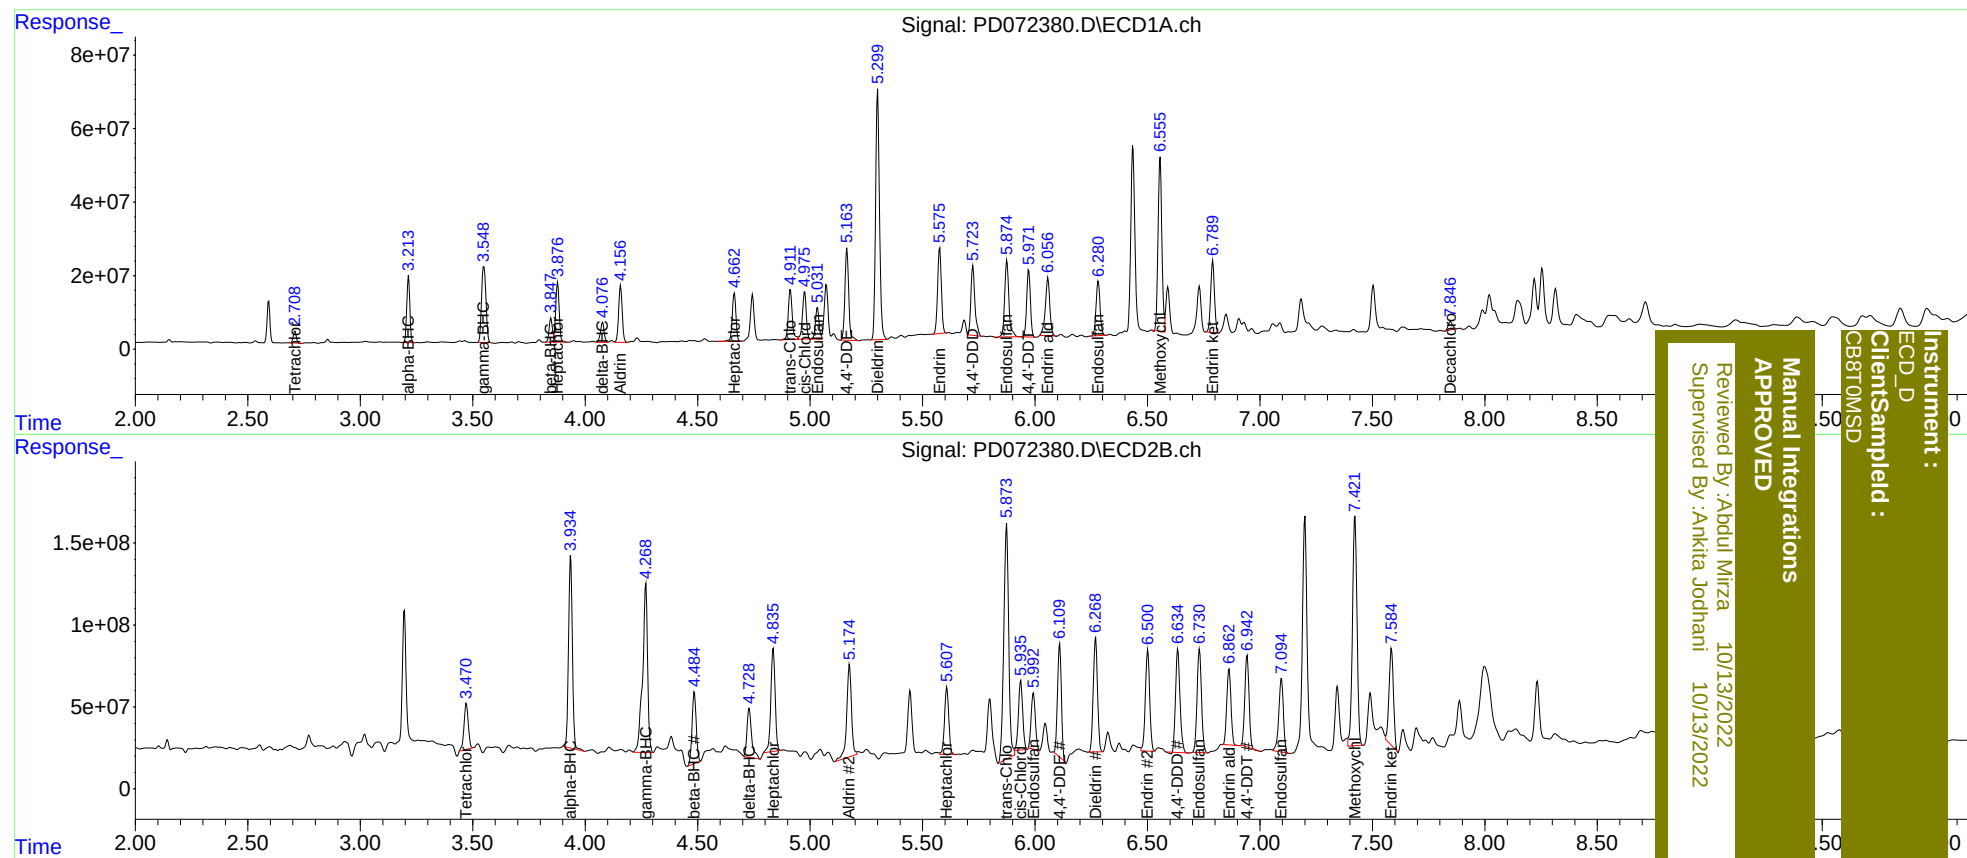

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/13/2022
Supervised By: Ankita Jodhani 10/13/2022

Instrument :
ECD_D
Client Sampled :
CB8TOMSD