
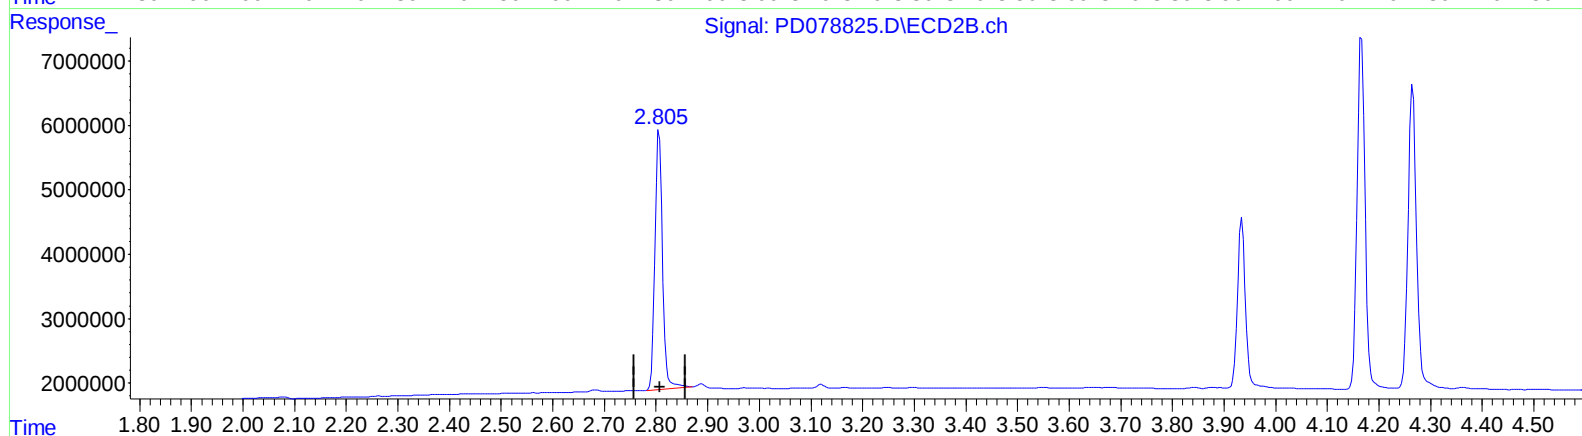


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101223\
Data File : PD078825.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2023 12:33
Operator : AR\AJ
Sample : INDB002
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 22:18:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 05:55:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

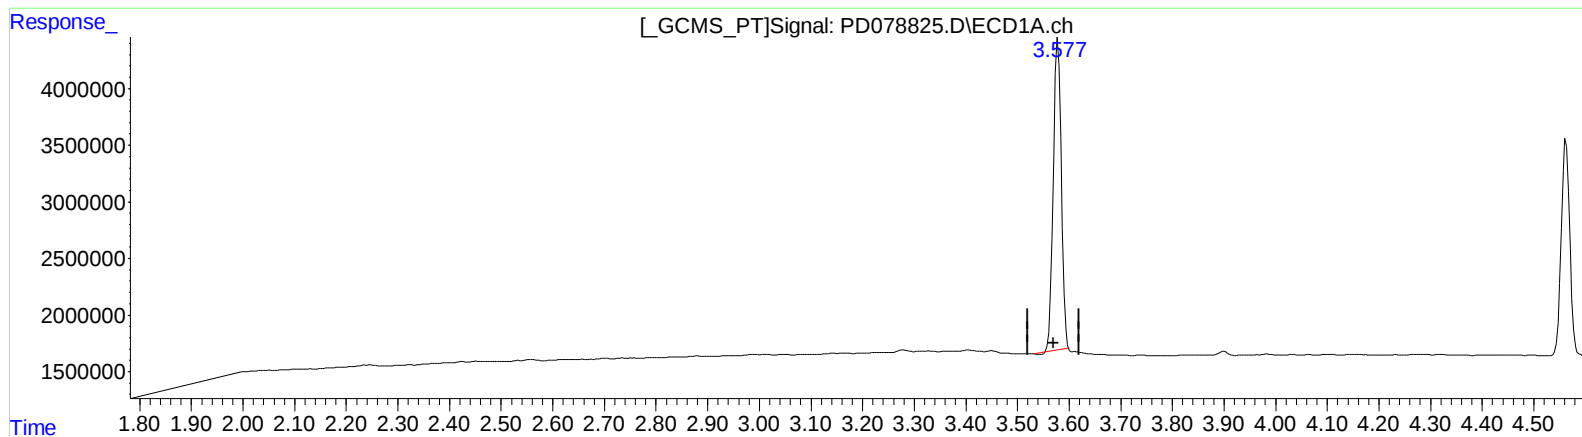

QEdit

(1) Tetrachloro-m-xylene (SA)

3.578min 19.330 ng/ml

response 29279020

(1) Tetrachloro-m-xylene #2 (SA)



2.806min 21.221 ng/ml

response 41410142

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101223\
Data File : PD078825.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2023 12:33
Operator : AR\AJ
Sample : INDB002
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 22:18:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 05:55:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

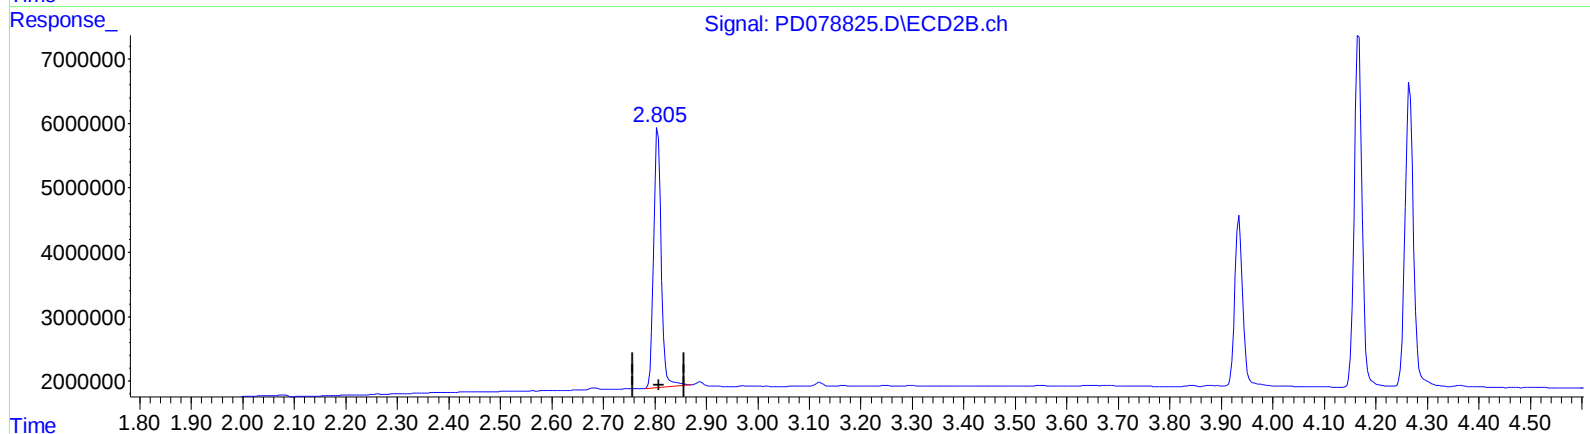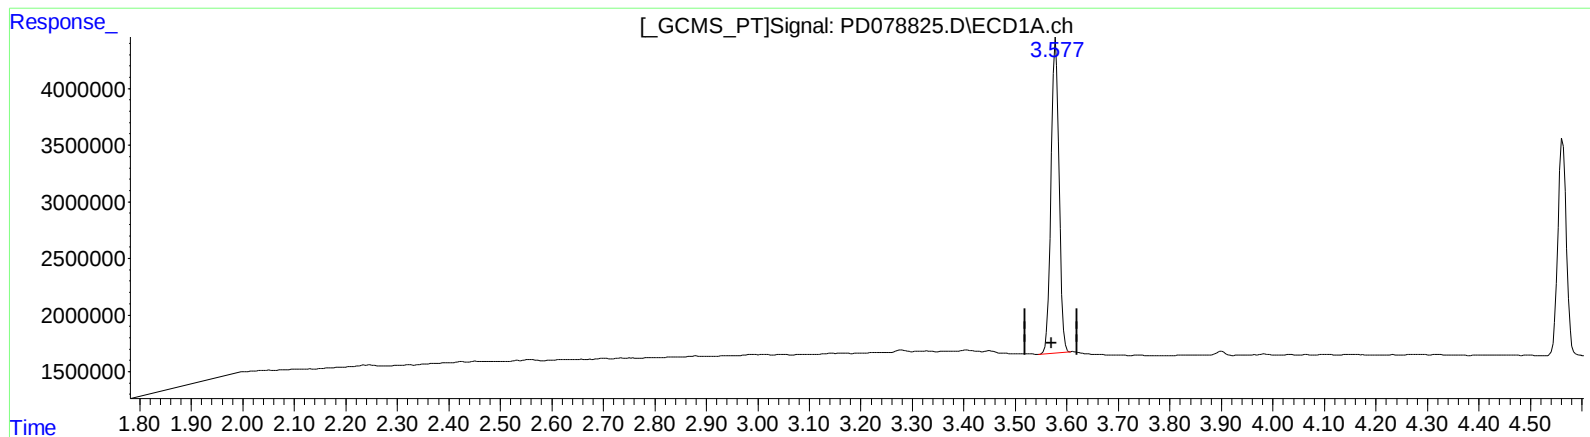

QEdit

(1) Tetrachloro-m-xylene (SA)

3.577min 19.957 ng/ml m

response 30228399

(1) Tetrachloro-m-xylene #2 (SA)

2.806min 21.221 ng/ml

response 41410142

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101223\
 Data File : PD078825.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2023 12:33
 Operator : AR\AJ
 Sample : INDB002
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 22:18:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 11 05:55:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.577	2.806	30228399	41410142	19.957m	21.221
27)	SA Decachlor...	9.131	7.961	73297064	62562826	42.943	46.272
Target Compounds							
5)	MB Aldrin	5.307	4.266	47211146	53686090	18.814	21.055
6)	B beta-BHC	4.563	3.935	21540998	28161367	19.090	22.615
7)	B delta-BHC	4.812	4.167	50247742	58300410	18.497	21.132
8)	B Heptachlo...	5.734	4.768	44107027	48817226	18.915	20.614
10)	B trans-Chl...	5.989	5.019	42709675	45051788	18.994	20.123
11)	B cis-Chlor...	6.069	5.083	43596247	46367221	19.131	20.121
12)	B 4,4'-DDE	6.240	5.273	80060397	80329858	37.965	40.149
15)	B Endosulfa...	6.843	5.971	75608078	69752119	38.778m	41.480
18)	B Endrin al...	6.974	6.151	58882199	55167150	40.503	44.209
19)	B Endosulfa...	7.208	6.374	73880787	66579980	38.797	43.273
21)	B Endrin ke...	7.695	6.881	80003118	75953689	38.969	43.028

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101223\
Data File : PD078825.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2023 12:33
Operator : AR\AJ
Sample : INDB002
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 22:18:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 05:55:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

