

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101223\
 Data File : PD078820.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2023 10:21
 Operator : AR\AJ
 Sample : 04360-03MS 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JLDA7MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/12/2023
 Supervised By : Ankita Jodhani 10/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 22:15:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 11 05:55:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.578	2.808	31911658	41549897	21.068	21.293
27)	SA Decachlor...	9.130	7.963	36194701	30035068	21.205	22.214
Target Compounds							
2)	A alpha-BHC	4.036	3.312	131.0E6	154.8E6	49.890	55.126
3)	MA gamma-BHC...	4.368	3.643	119.1E6	134.2E6	48.180m	52.320
4)	MA Heptachlor	4.963	3.987	124.5E6	130.5E6	47.368	52.856
5)	MB Aldrin	5.307	4.268	121.3E6	125.2E6	48.330	49.086
6)	B beta-BHC	4.562	3.937	50976158	58611126	45.175	47.069
7)	B delta-BHC	4.812	4.169	90224058	94239224	33.212	34.158
8)	B Heptachlo...	5.733	4.771	109.5E6	107.0E6	46.948	45.202
9)	A Endosulfan I	6.119	5.142	103.9E6	91606611	50.016	46.424
10)	B trans-Chl...	5.988	5.021	108.5E6	98720836	48.265	44.096
11)	B cis-Chlor...	6.068	5.086	108.1E6	98640407	47.449	42.804
12)	B 4,4'-DDE	6.239	5.275	209.0E6	180.5E6	99.130	90.193
13)	MA Dieldrin	6.396	5.406	227.0E6	192.3E6	101.214	90.574
14)	MA Endrin	6.624	5.681	191.7E6	160.6E6	105.544m	92.377
15)	B Endosulfa...	6.841	5.973	191.4E6	150.8E6	98.174m	89.660
16)	A 4,4'-DDD	6.756	5.829	165.9E6	135.8E6	101.125	91.132
17)	MA 4,4'-DDT	7.071	6.081	184.0E6	135.6E6	105.813	94.313
18)	B Endrin al...	6.973	6.154	139.3E6	110.7E6	95.825	88.745
19)	B Endosulfa...	7.207	6.376	174.8E6	133.8E6	91.796	86.959
20)	A Methoxychlor	7.545	6.657	464.3E6	352.4E6	501.343	469.156
21)	B Endrin ke...	7.693	6.882	198.4E6	163.4E6	96.641m	92.557

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101223\
Data File : PD078820.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2023 10:21
Operator : AR\AJ
Sample : 04360-03MS 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 22:15:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 05:55:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

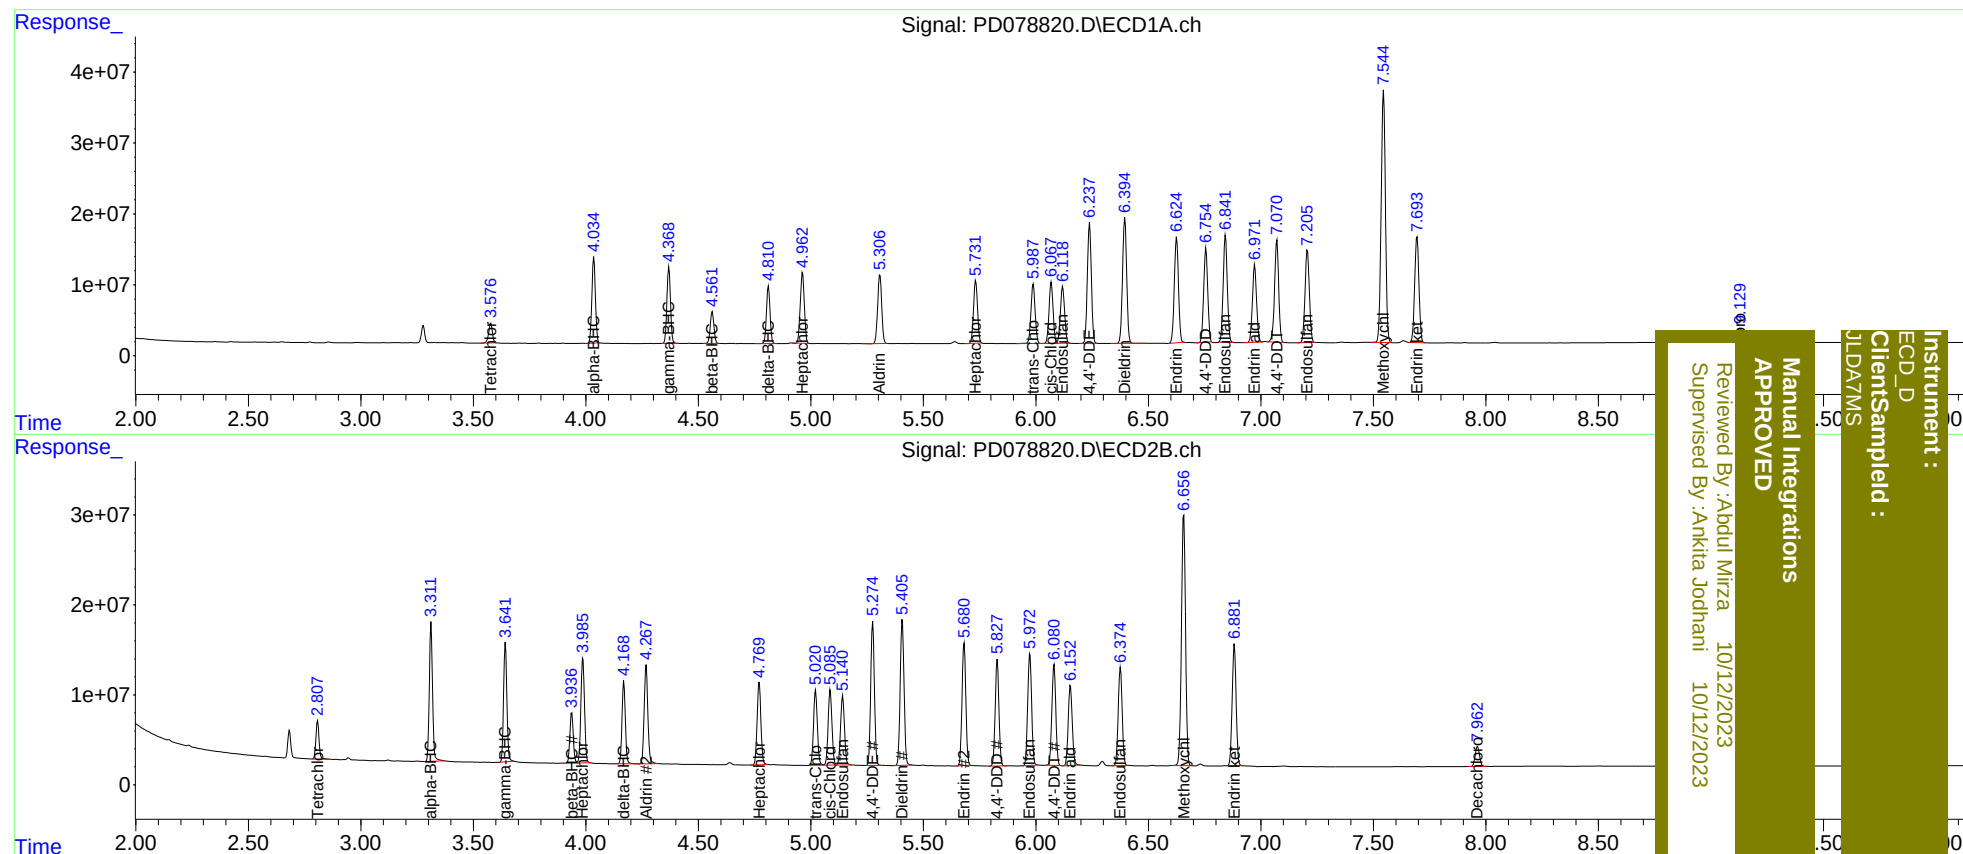

Instrument :
ECD_D
ClientSampled :
JLDA7MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 10/12/2023
Supervised By: Ankita Jodhani 10/12/2023