

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101320\
 Data File : PD059706.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2020 10:00
 Operator : DD\AJ
 Sample : L4184-16
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AP2

Manual Integrations
 APPROVED

Ankita
 10/16/2020 8:40:57 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:11:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 02 04:21:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.509	4.023	21429143	25271213	14.835	12.723m
27)	SA Decachlor...	8.311	9.110	72735180	74920946	67.883m	50.357m#
Target Compounds							
3)	MA gamma-BHC...	4.243	4.681	36979070	67297410	18.934	25.358 #
8)	B Heptachlo...	5.240	5.893	4513453	17316339	2.789	7.714 #
10)	B trans-Chl...	5.474	6.125	53891379	183.6E6	33.176m	82.269 #
11)	B cis-Chlor...	5.534	6.215	50724390	105.4E6	31.328	48.176 #
12)	B 4,4'-DDE	5.697	6.368	36427704	58271972	23.643m	27.863
13)	MA Dieldrin	5.833	6.522	146.2E6	124.5E6	89.163	55.840m#
14)	MA Endrin	6.092	6.730	18248035	6287237	15.447	4.058m#
16)	A 4,4'-DDD	6.219	6.858	104.0E6	187.9E6	79.562	108.563m#
17)	MA 4,4'-DDT	6.462	7.159	72076240	105.2E6	53.710	65.520

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101320\
Data File : PD059706.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2020 10:00
Operator : DD\AJ
Sample : L4184-16
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:11:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 02 04:21:20 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

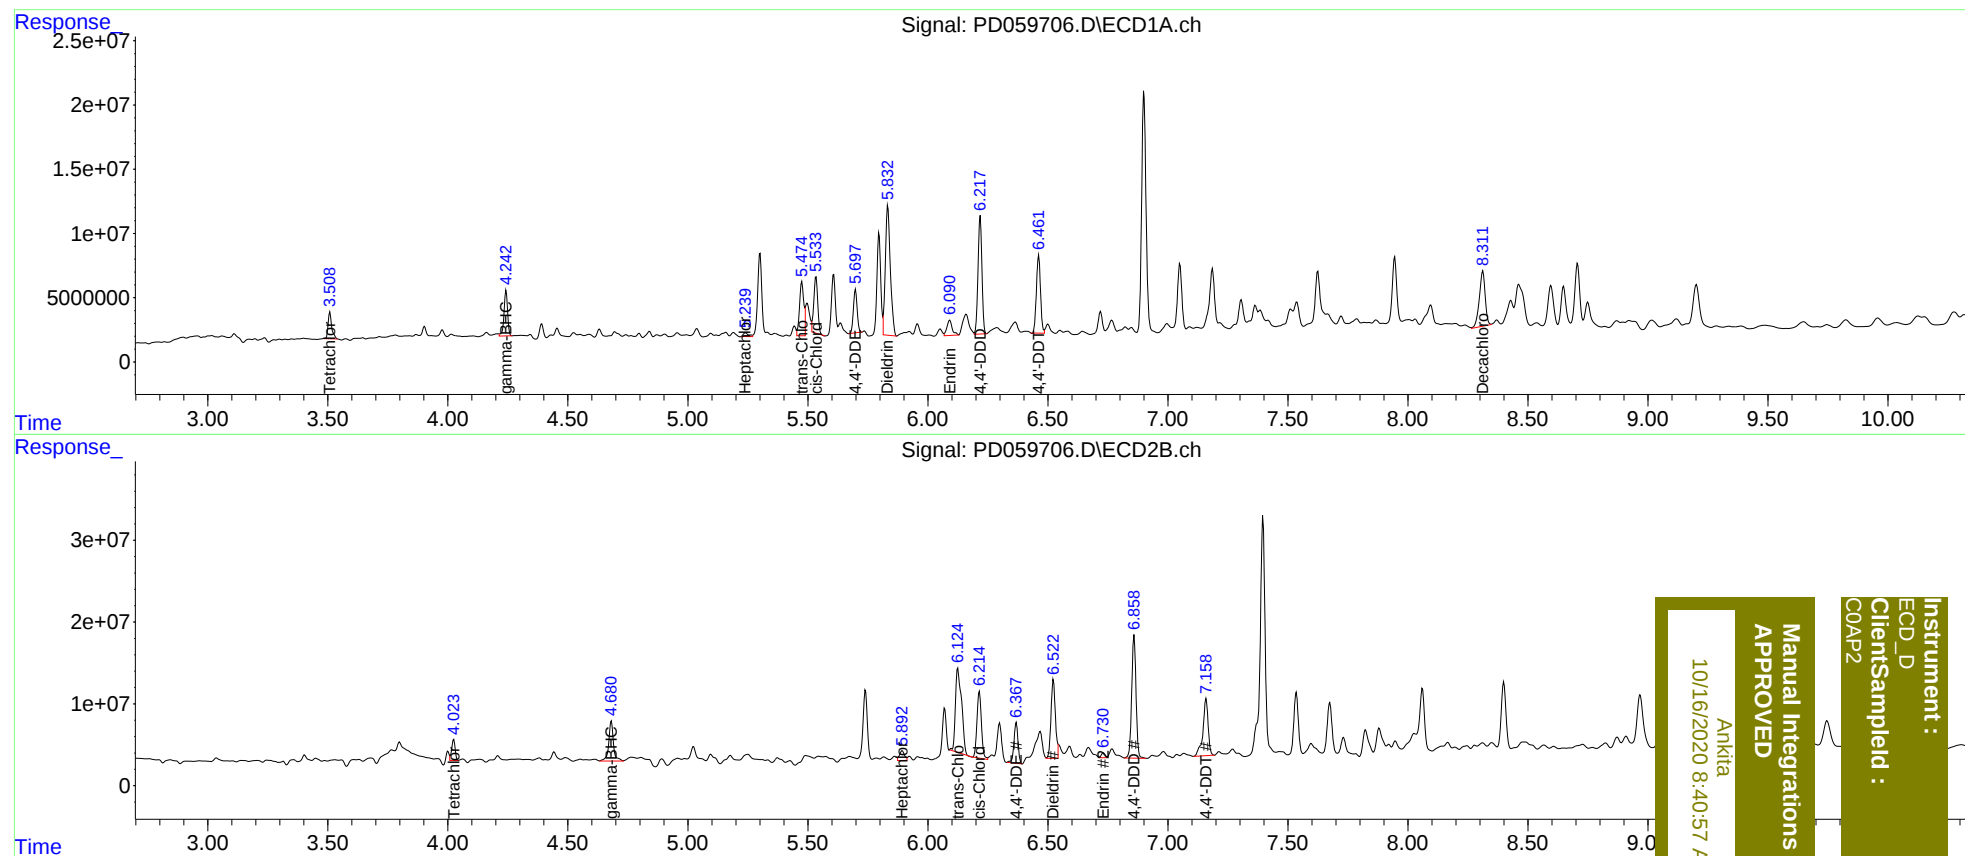

10/16/2020 8:40:57 AM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client Sampled :
COAP2