

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101321\
 Data File : PD066187.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2021 20:58
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 05:44:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101321CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 13 05:43:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	3.970	9908370	36405923	5.220	5.360
27)	SA Decachlor...	8.169	9.018	22553988	59730485	11.264	12.248
Target Compounds							
2)	A alpha-BHC	3.880	4.363	15576169	73195543	5.350	7.266 #
3)	MA gamma-BHC...	4.162	4.648	18322116	53692116	6.186	5.565
4)	MA Heptachlor	4.456	5.148	12737582	49313627	5.165	5.453
9)	A Endosulfan I	5.478	6.197	11037547	49743980	4.714	5.509
13)	MA Dieldrin	5.720	6.454	24686955	102.5E6	9.537	10.756
14)	MA Endrin	5.977	6.673	19866970	91960528	10.166	11.863
16)	A 4,4'-DDD	6.103	6.798	19033270	79957163	9.441	10.546
17)	MA 4,4'-DDT	6.341	7.094	16426961	103.4E6	9.252	13.646 #
20)	A Methoxychlor	6.888	7.555	55244600	228.9E6	53.721	67.063

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101321\
Data File : PD066187.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2021 20:58
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 05:44:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101321CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 13 05:43:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

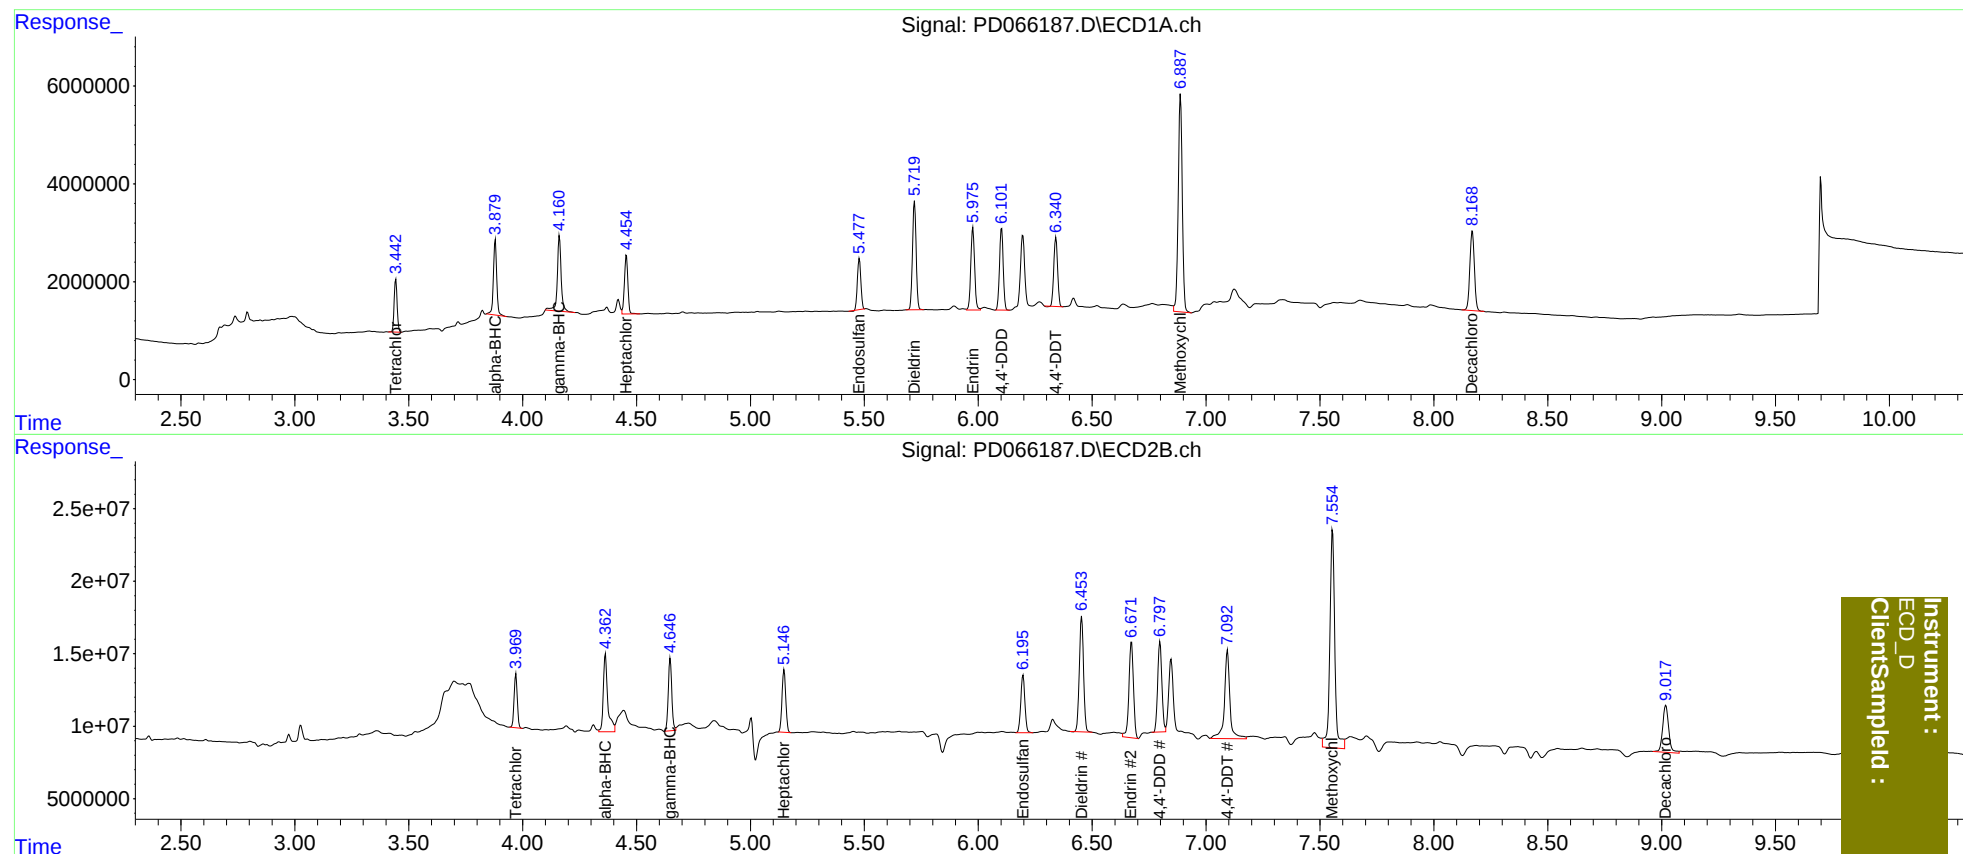


Instrument :
ECD_D
ClientSampled :

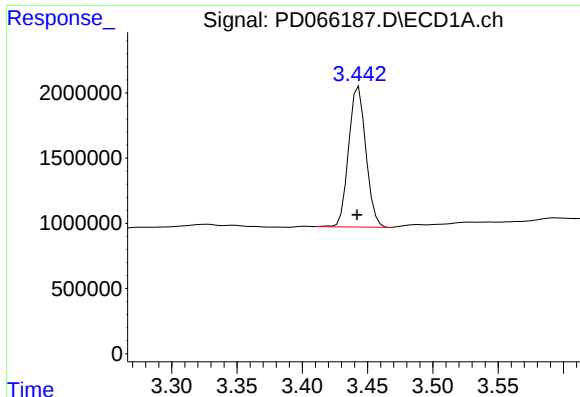

#1 Tetrachloro-m-xylene


R.T.: 3.443 min
Delta R.T.: 0.001 min
Response: 9908370
Conc: 5.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

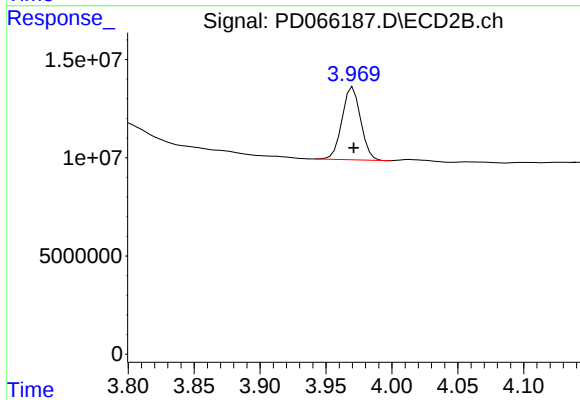


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 36405923
Conc: 5.36 ng/ml

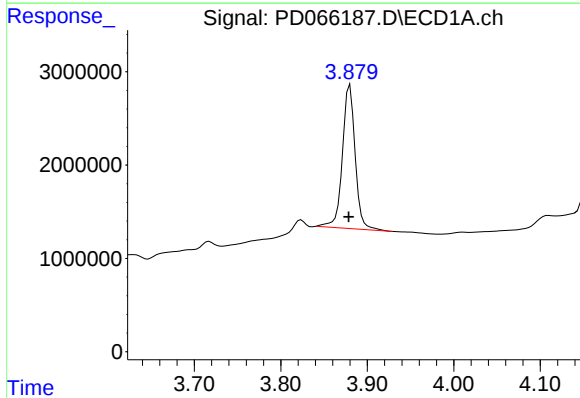


#2 alpha-BHC

R.T.: 3.880 min
Delta R.T.: 0.001 min
Response: 15576169
Conc: 5.35 ng/ml

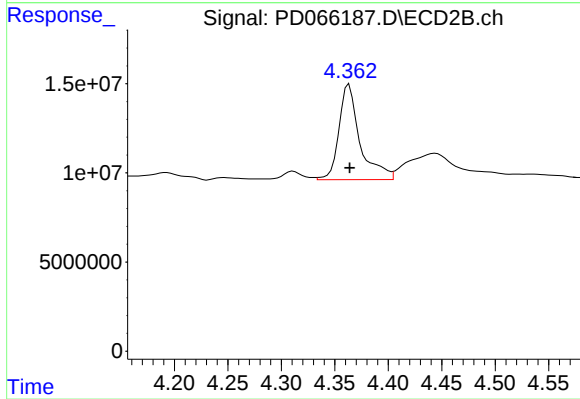

#2 alpha-BHC


R.T.: 4.363 min
Delta R.T.: 0.000 min
Response: 73195543
Conc: 7.27 ng/ml

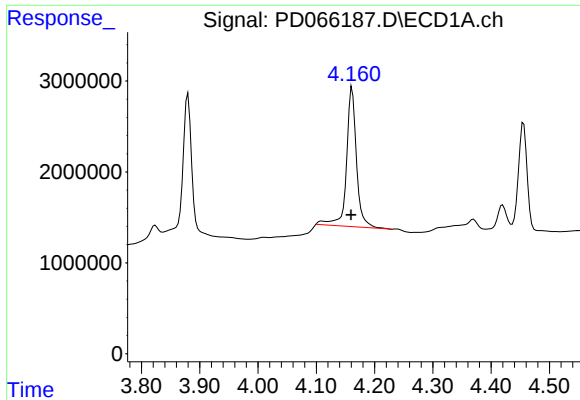

#3 gamma-BHC (Lindane)


R.T.: 4.162 min
Delta R.T.: 0.002 min
Response: 18322116
Conc: 6.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

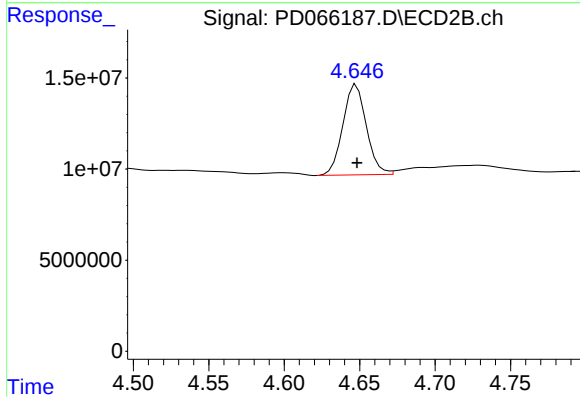


#3 gamma-BHC (Lindane)

R.T.: 4.648 min
Delta R.T.: 0.000 min
Response: 53692116
Conc: 5.57 ng/ml

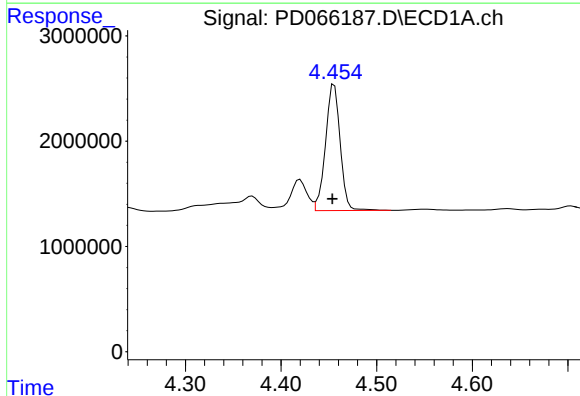


#4 Heptachlor

R.T.: 4.456 min
Delta R.T.: 0.002 min
Response: 12737582
Conc: 5.17 ng/ml

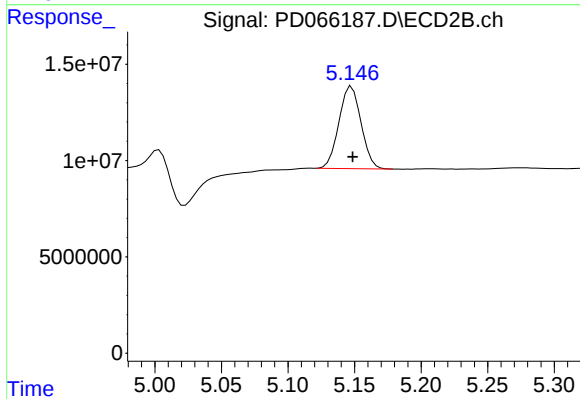

#4 Heptachlor


R.T.: 5.148 min
Delta R.T.: 0.000 min
Response: 49313627
Conc: 5.45 ng/ml

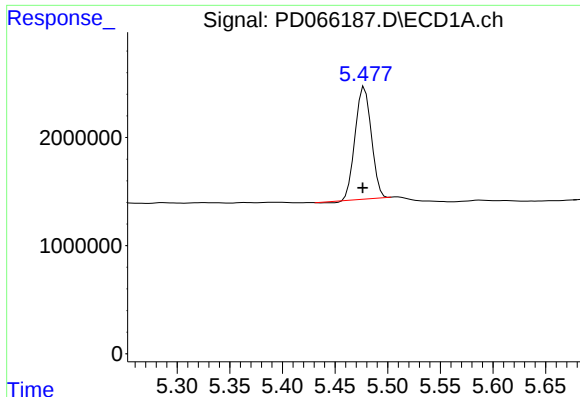

#9 Endosulfan I


R.T.: 5.478 min
Delta R.T.: 0.002 min
Response: 11037547
Conc: 4.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

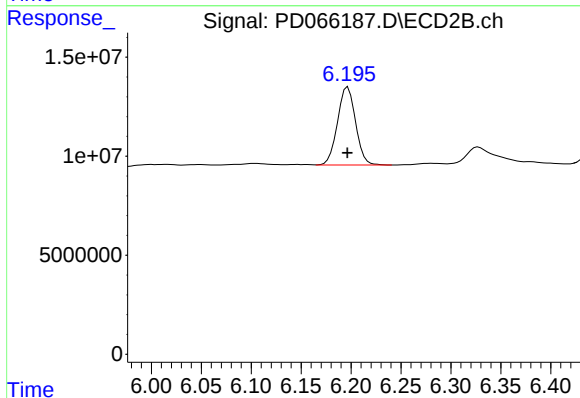


#9 Endosulfan I

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 49743980
Conc: 5.51 ng/ml

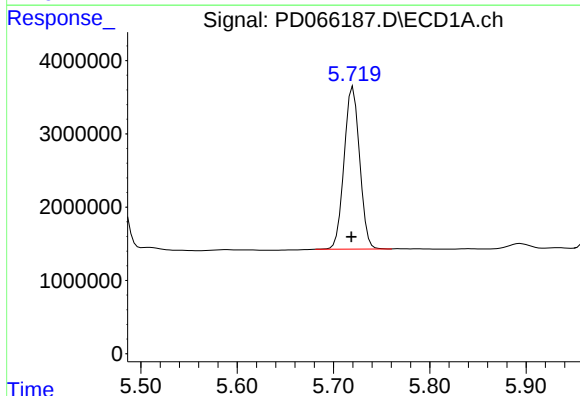


#13 Dieldrin

R.T.: 5.720 min
Delta R.T.: 0.002 min
Response: 24686955
Conc: 9.54 ng/ml

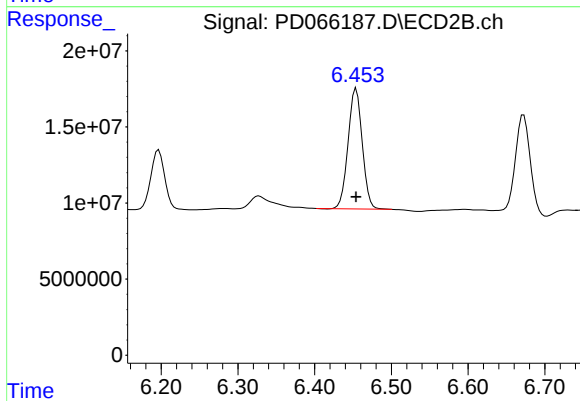

#13 Dieldrin


R.T.: 6.454 min
Delta R.T.: 0.000 min
Response: 102512471
Conc: 10.76 ng/ml

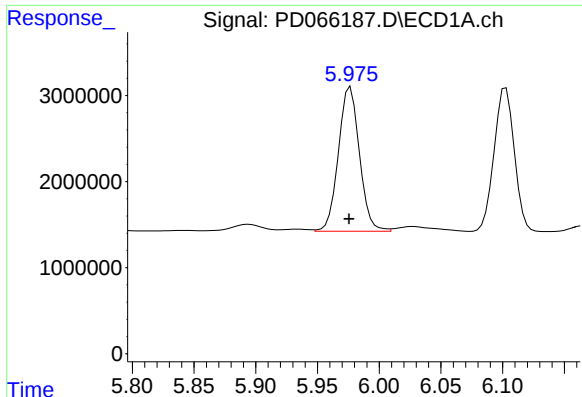

#14 Endrin


R.T.: 5.977 min
Delta R.T.: 0.001 min
Response: 19866970
Conc: 10.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

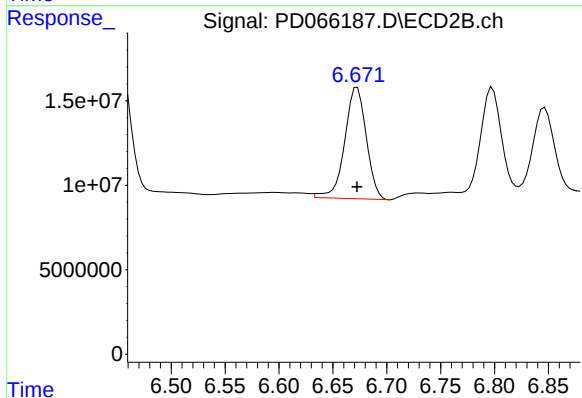


#14 Endrin

R.T.: 6.673 min
Delta R.T.: 0.000 min
Response: 91960528
Conc: 11.86 ng/ml

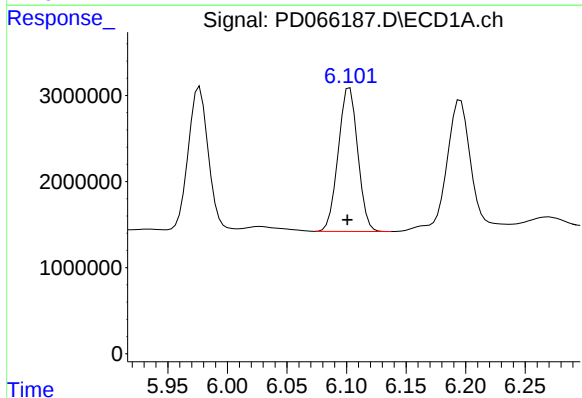


#16 4,4'-DDD

R.T.: 6.103 min
Delta R.T.: 0.002 min
Response: 19033270
Conc: 9.44 ng/ml

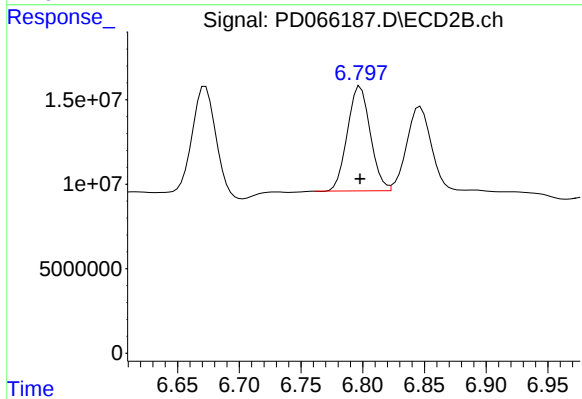

#16 4,4'-DDD


R.T.: 6.798 min
Delta R.T.: 0.000 min
Response: 79957163
Conc: 10.55 ng/ml

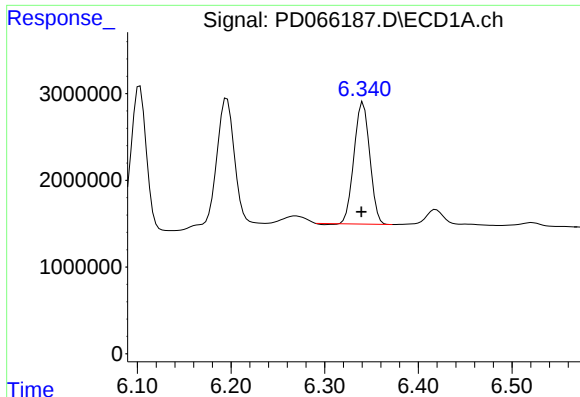

#17 4,4'-DDT


R.T.: 6.341 min
Delta R.T.: 0.002 min
Response: 16426961
Conc: 9.25 ng/ml

Instrument :
ECD_D
ClientSampleId :

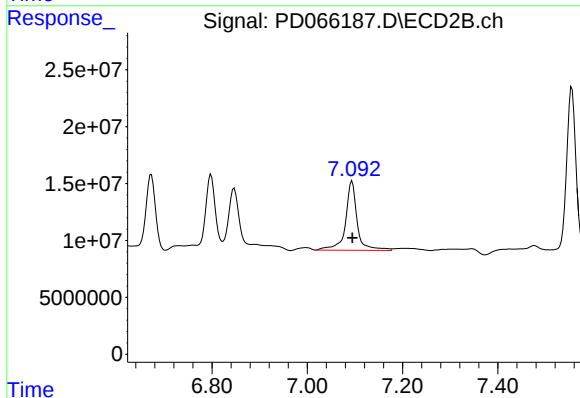


#17 4,4'-DDT

R.T.: 7.094 min
Delta R.T.: 0.000 min
Response: 103374833
Conc: 13.65 ng/ml

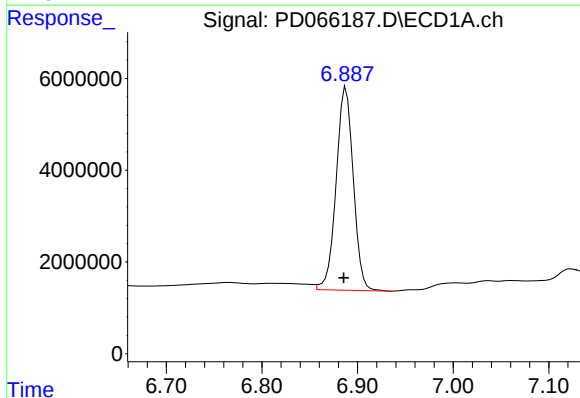


#20 Methoxychlor

R.T.: 6.888 min
Delta R.T.: 0.002 min
Response: 55244600
Conc: 53.72 ng/ml

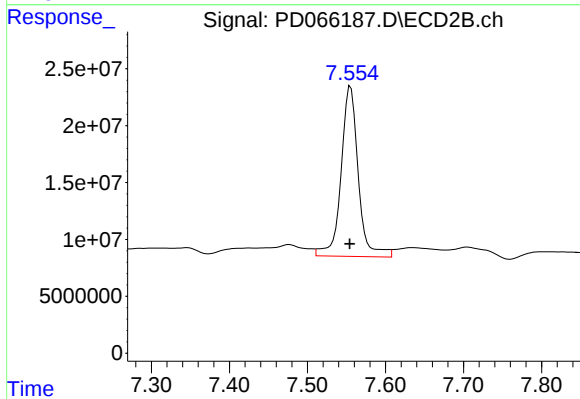

#20 Methoxychlor


R.T.: 7.555 min
Delta R.T.: 0.000 min
Response: 228905398
Conc: 67.06 ng/ml

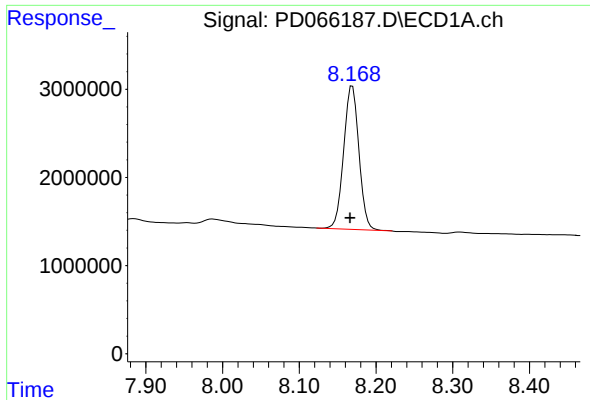

#27 Decachlorobiphenyl

R.T.: 8.169 min
Delta R.T.: 0.003 min
Response: 22553988
Conc: 11.26 ng/ml

Instrument :
ECD_D
ClientSampleId :

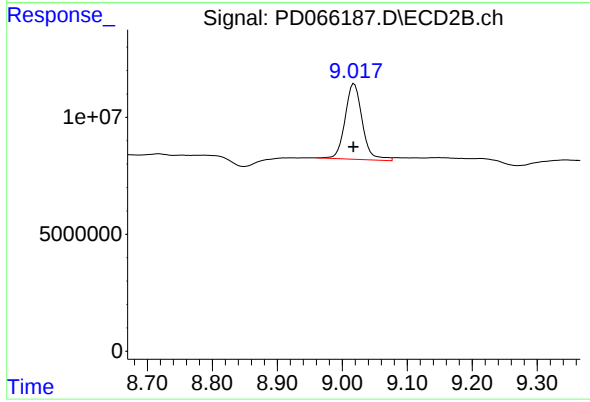

#27 Decachlorobiphenyl

R.T.: 9.018 min
Delta R.T.: 0.001 min
Response: 59730485
Conc: 12.25 ng/ml