

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101321\
 Data File : PD066189.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2021 21:26
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 05:45:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101321CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 13 05:43:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	3.971	19636020	72228300	10.345	10.633
27)	SA Decachlor...	8.167	9.017	42888076	103.5E6	21.419	21.229
Target Compounds							
2)	A alpha-BHC	3.878	4.363	29439698	108.9E6	10.111	10.808
3)	MA gamma-BHC...	4.160	4.648	32403090	102.5E6	10.940	10.623
4)	MA Heptachlor	4.454	5.148	25370619	96768266	10.289	10.700
9)	A Endosulfan I	5.476	6.196	23941846	96341955	10.225	10.670
13)	MA Dieldrin	5.718	6.454	51382841	199.0E6	19.851	20.880
14)	MA Endrin	5.975	6.672	39673952	168.2E6	20.301	21.703
16)	A 4,4'-DDD	6.101	6.797	40142913	158.0E6	19.913	20.839
17)	MA 4,4'-DDT	6.339	7.094	35039653	164.9E6	19.735	21.763
20)	A Methoxychlor	6.886	7.554	108.7E6	367.5E6	105.685	107.677

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101321\
Data File : PD066189.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2021 21:26
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 05:45:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101321CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 13 05:43:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

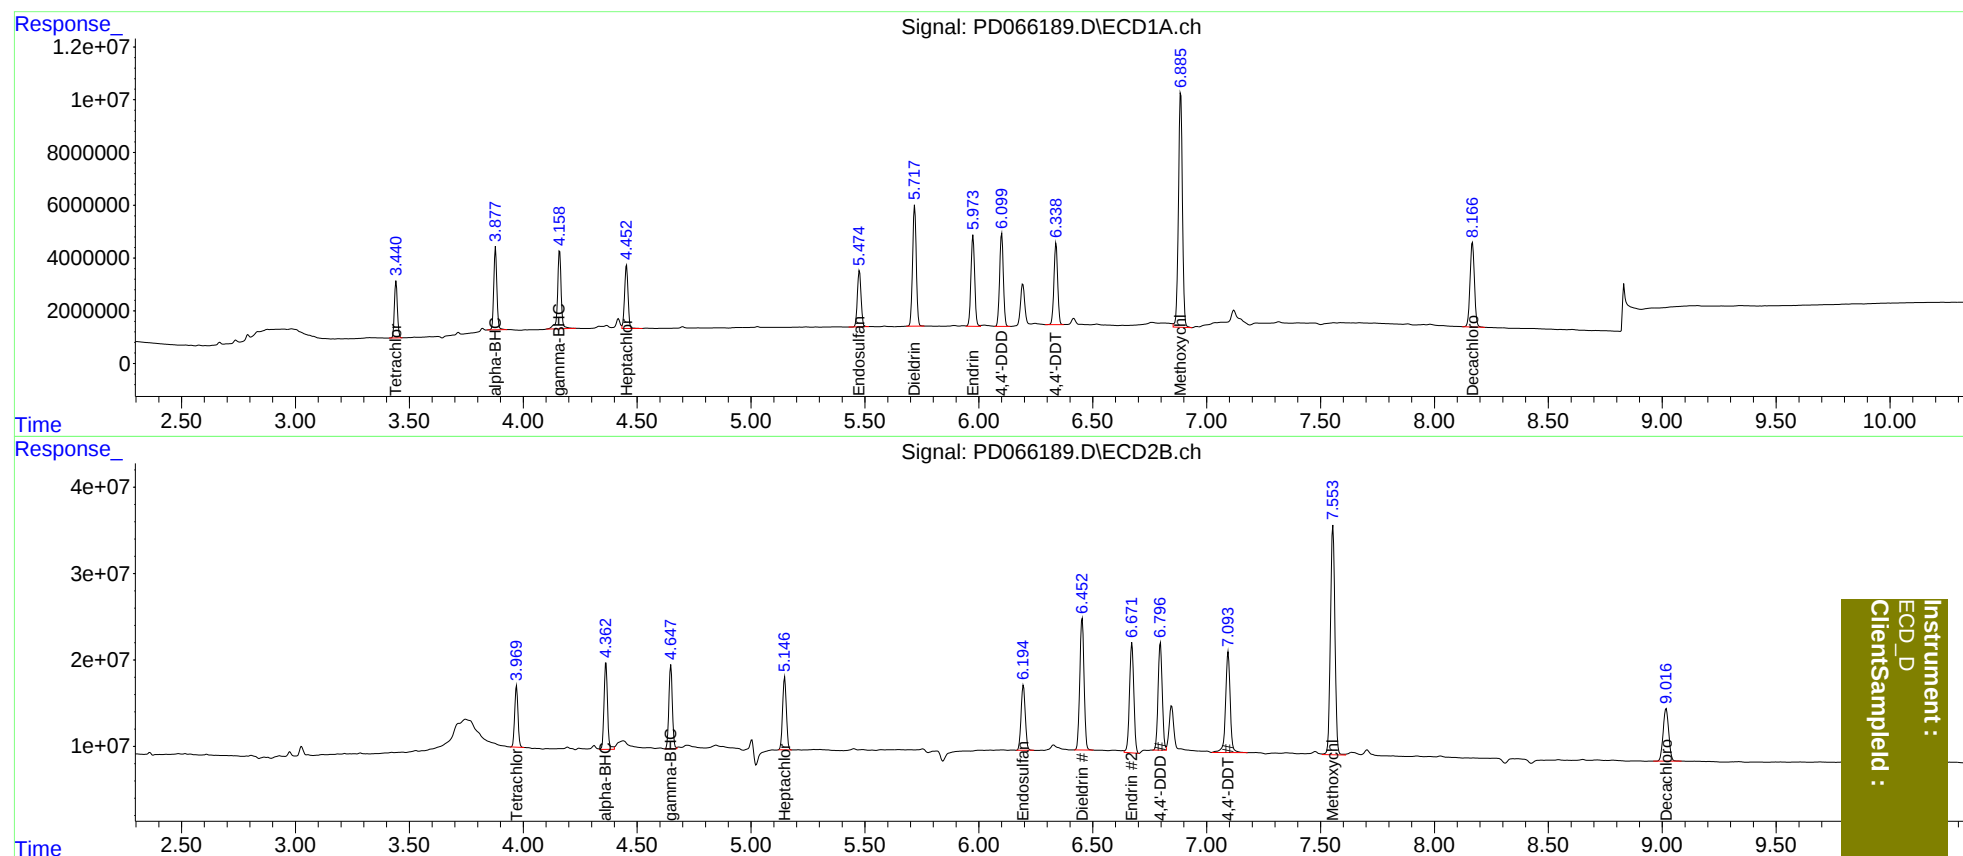


Instrument :
ECD_D
ClientSampled :

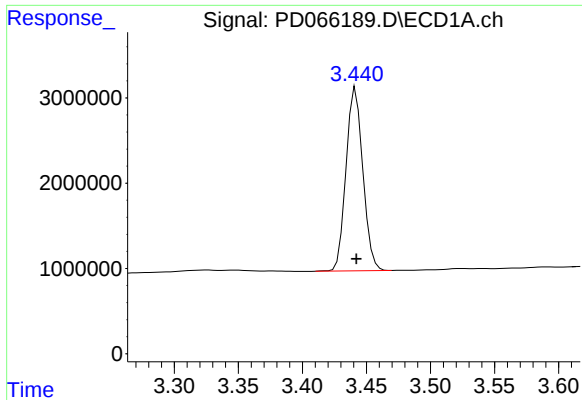

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 19636020
Conc: 10.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

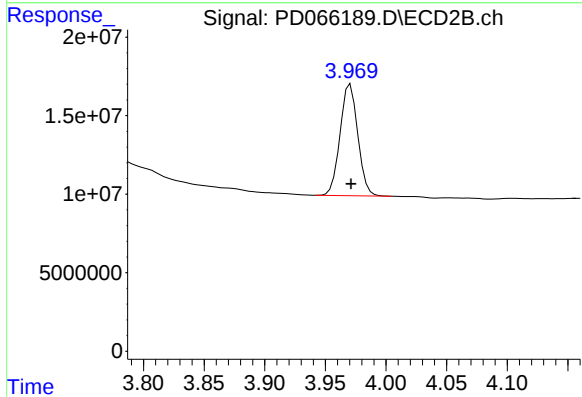


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 72228300
Conc: 10.63 ng/ml

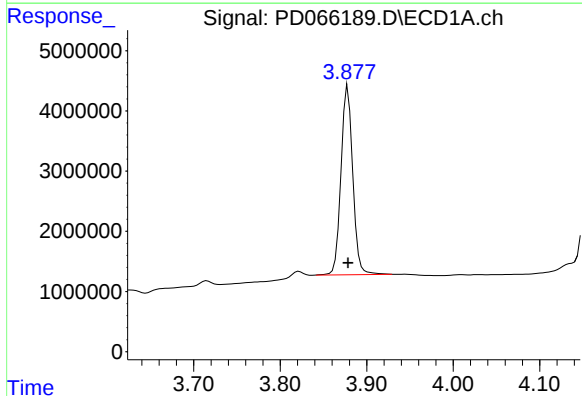


#2 alpha-BHC

R.T.: 3.878 min
Delta R.T.: 0.000 min
Response: 29439698
Conc: 10.11 ng/ml

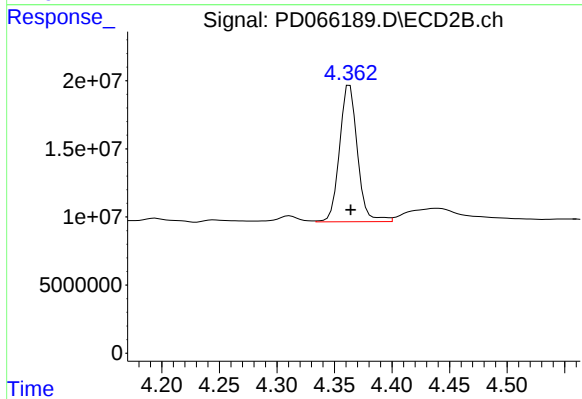

#2 alpha-BHC


R.T.: 4.363 min
Delta R.T.: 0.000 min
Response: 108881356
Conc: 10.81 ng/ml

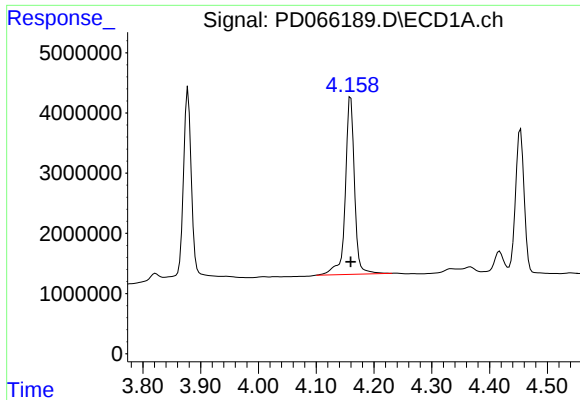

#3 gamma-BHC (Lindane)


R.T.: 4.160 min
Delta R.T.: 0.000 min
Response: 32403090
Conc: 10.94 ng/ml

Instrument :
ECD_D
ClientSampleId :

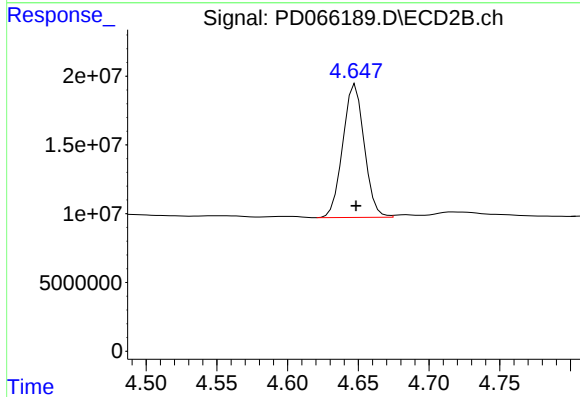


#3 gamma-BHC (Lindane)

R.T.: 4.648 min
Delta R.T.: 0.000 min
Response: 102487466
Conc: 10.62 ng/ml

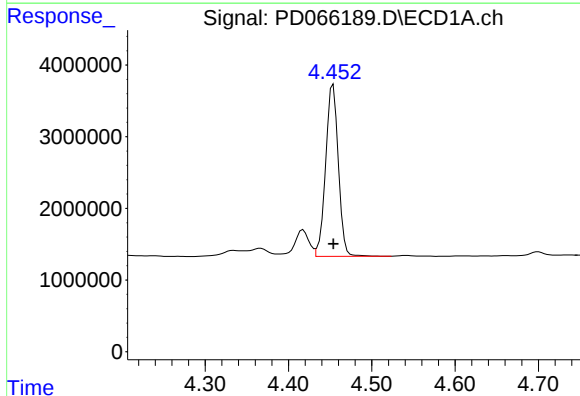


#4 Heptachlor

R.T.: 4.454 min
Delta R.T.: 0.000 min
Response: 25370619
Conc: 10.29 ng/ml

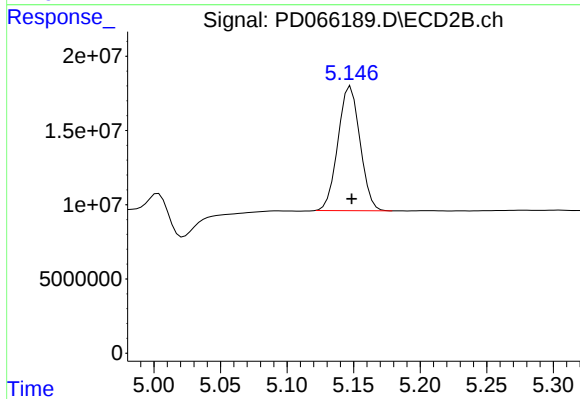

#4 Heptachlor


R.T.: 5.148 min
Delta R.T.: 0.000 min
Response: 96768266
Conc: 10.70 ng/ml

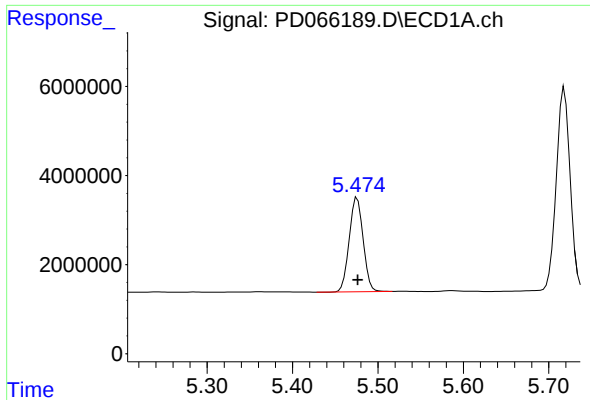

#9 Endosulfan I


R.T.: 5.476 min
Delta R.T.: 0.000 min
Response: 23941846
Conc: 10.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

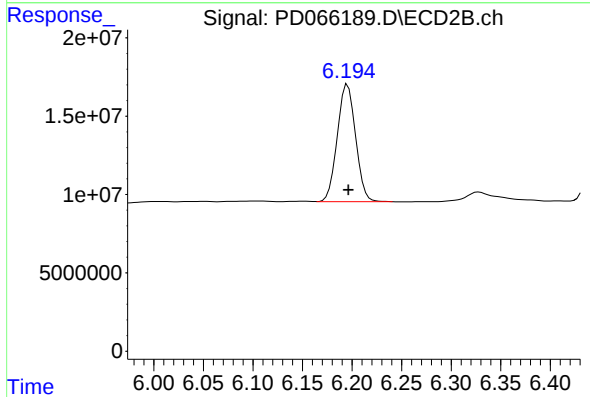


#9 Endosulfan I

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 96341955
Conc: 10.67 ng/ml

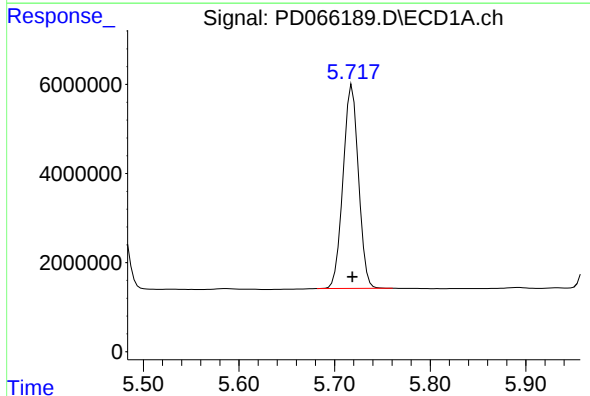


#13 Dieldrin

R.T.: 5.718 min
Delta R.T.: 0.000 min
Response: 51382841
Conc: 19.85 ng/ml

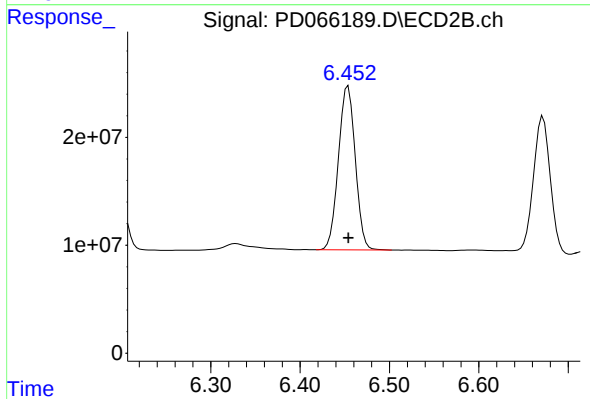

#13 Dieldrin


R.T.: 6.454 min
Delta R.T.: 0.000 min
Response: 198993062
Conc: 20.88 ng/ml

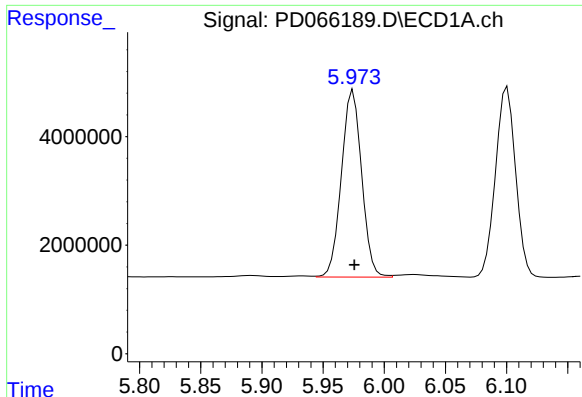

#14 Endrin


R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 39673952
Conc: 20.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

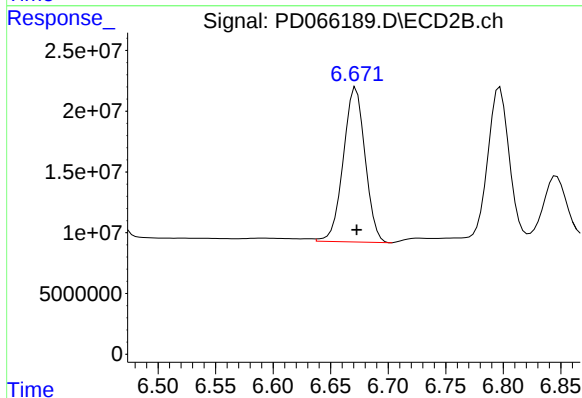


#14 Endrin

R.T.: 6.672 min
Delta R.T.: 0.000 min
Response: 168236696
Conc: 21.70 ng/ml

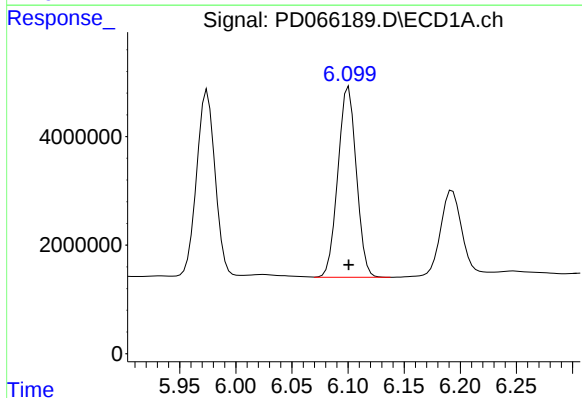


#16 4,4'-DDD

R.T.: 6.101 min
Delta R.T.: 0.000 min
Response: 40142913
Conc: 19.91 ng/ml

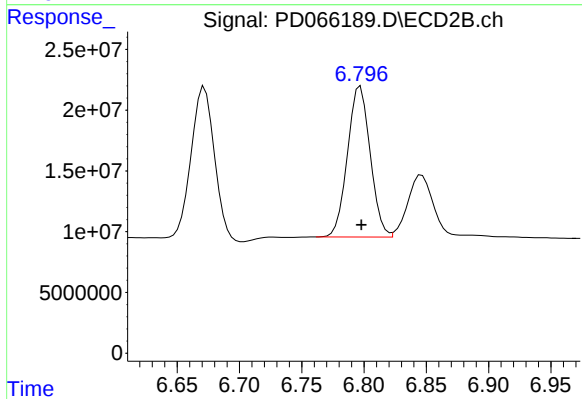

#16 4,4'-DDD


R.T.: 6.797 min
Delta R.T.: 0.000 min
Response: 157989785
Conc: 20.84 ng/ml

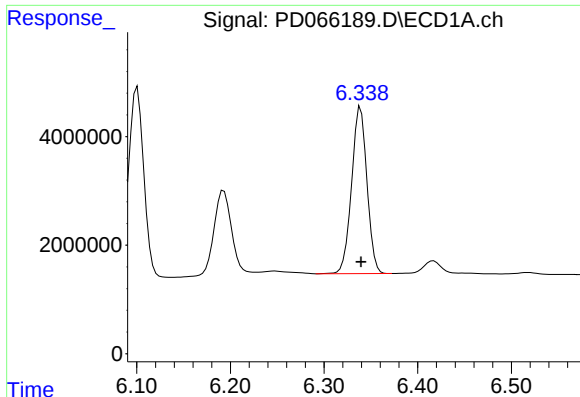

#17 4,4'-DDT


R.T.: 6.339 min
Delta R.T.: 0.000 min
Response: 35039653
Conc: 19.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

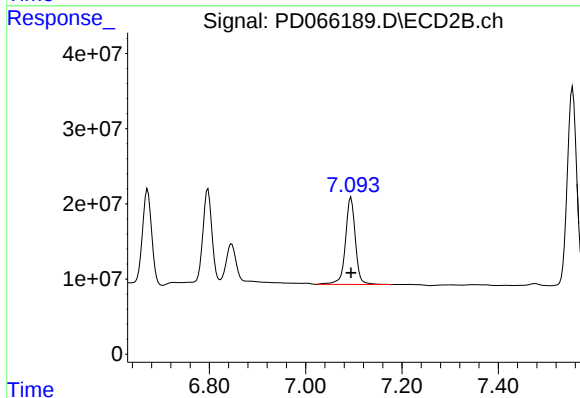


#17 4,4'-DDT

R.T.: 7.094 min
Delta R.T.: 0.000 min
Response: 164863305
Conc: 21.76 ng/ml

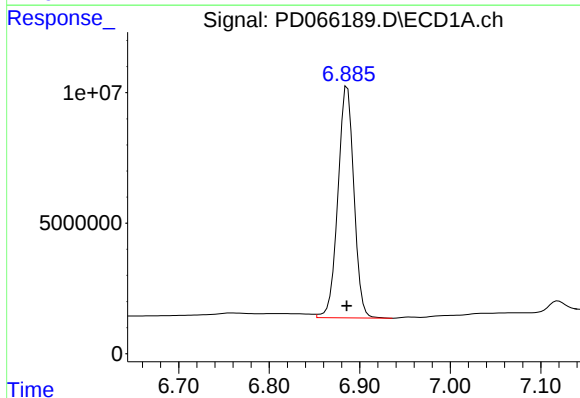


#20 Methoxychlor

R.T.: 6.886 min
Delta R.T.: 0.000 min
Response: 108682682
Conc: 105.69 ng/ml

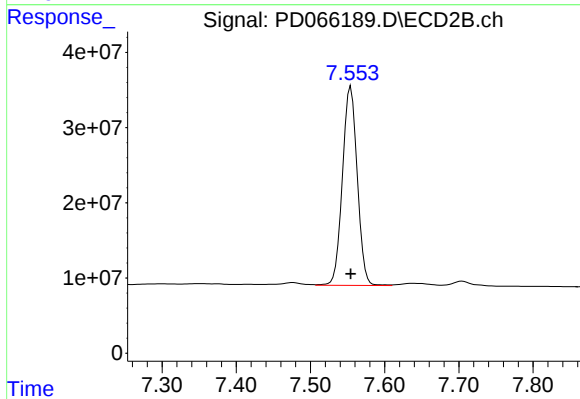

#20 Methoxychlor


R.T.: 7.554 min
Delta R.T.: 0.000 min
Response: 367534523
Conc: 107.68 ng/ml

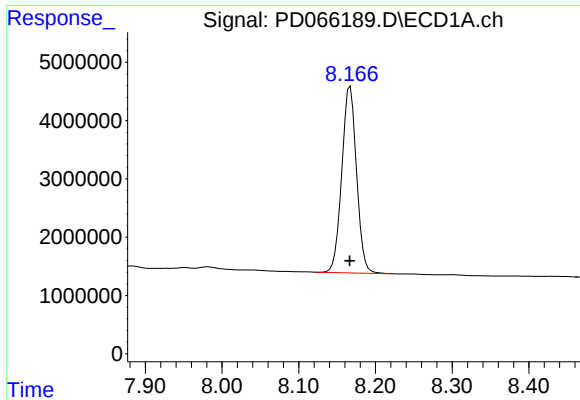

#27 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: 0.000 min
Response: 42888076
Conc: 21.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

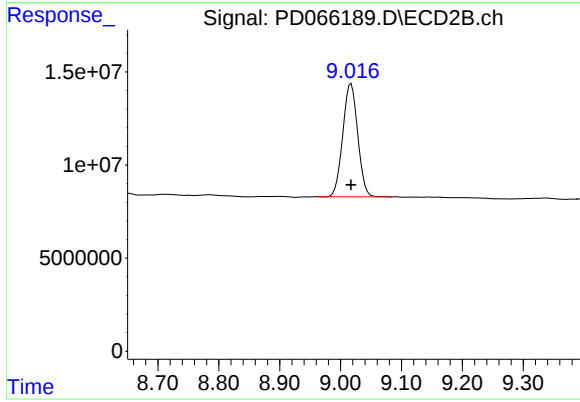

#27 Decachlorobiphenyl

R.T.: 9.017 min
Delta R.T.: 0.000 min
Response: 103534458
Conc: 21.23 ng/ml