

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101321\
 Data File : PD066191.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2021 21:53
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 05:45:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101321CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 13 05:43:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	3.971	37960805	135.9E6	20.000	20.000
27)	SA Decachlor...	8.166	9.017	80091919	195.1E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.878	4.364	58233250	201.5E6	20.000	20.000
3)	MA gamma-BHC...	4.160	4.648	59240225	193.0E6	20.000	20.000
4)	MA Heptachlor	4.454	5.148	49318134	180.9E6	20.000	20.000
9)	A Endosulfan I	5.476	6.196	46828446	180.6E6	20.000	20.000
13)	MA Dieldrin	5.718	6.454	103.5E6	381.2E6	40.000	40.000
14)	MA Endrin	5.976	6.673	78171009	310.1E6	40.000	40.000
16)	A 4,4'-DDD	6.101	6.798	80637995	303.3E6	40.000	40.000
17)	MA 4,4'-DDT	6.339	7.094	71018821	303.0E6	40.000	40.000
20)	A Methoxychlor	6.886	7.554	205.7E6	682.7E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101321\
Data File : PD066191.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2021 21:53
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 05:45:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101321CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 13 05:43:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

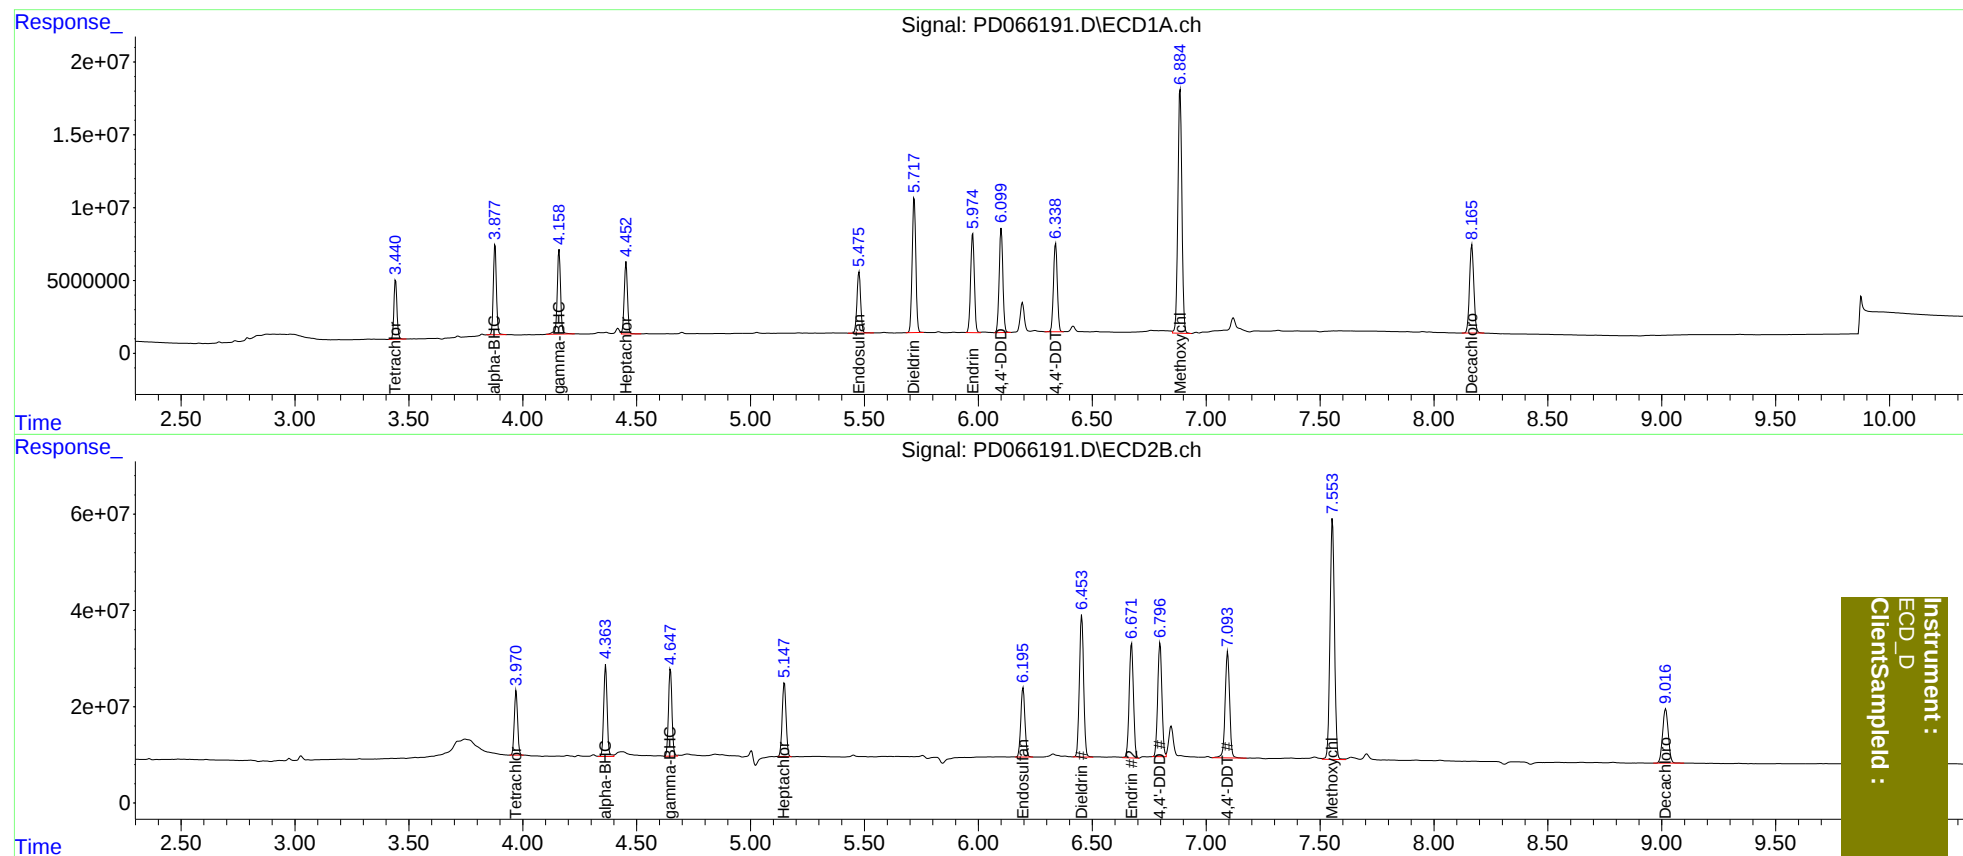


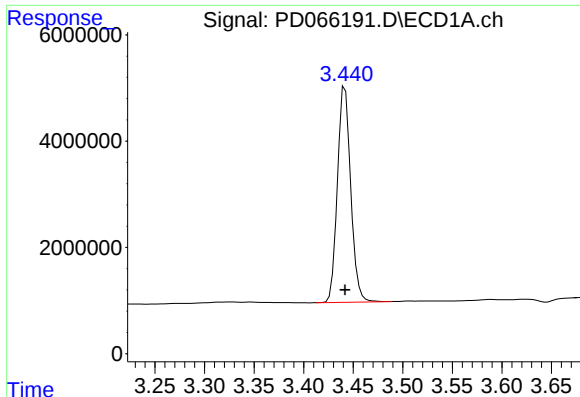

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 37960805
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

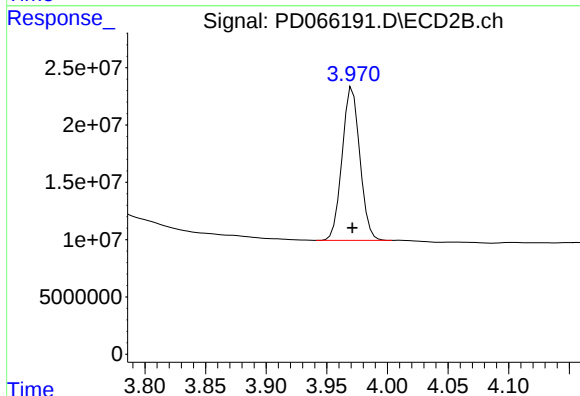


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 135851253
Conc: 20.00 ng/ml

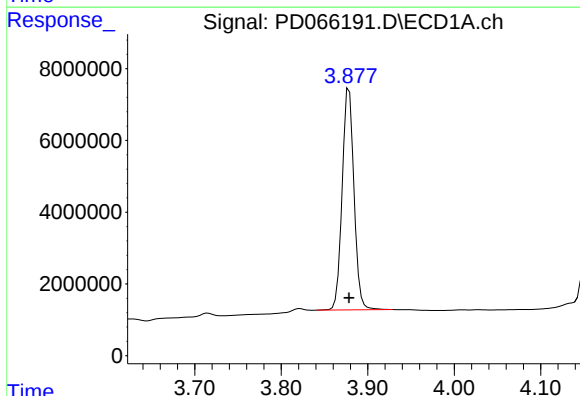


#2 alpha-BHC

R.T.: 3.878 min
Delta R.T.: 0.000 min
Response: 58233250
Conc: 20.00 ng/ml

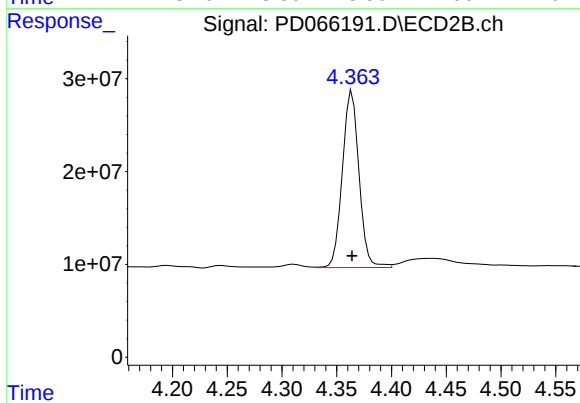

#2 alpha-BHC


R.T.: 4.364 min
Delta R.T.: 0.000 min
Response: 201487495
Conc: 20.00 ng/ml

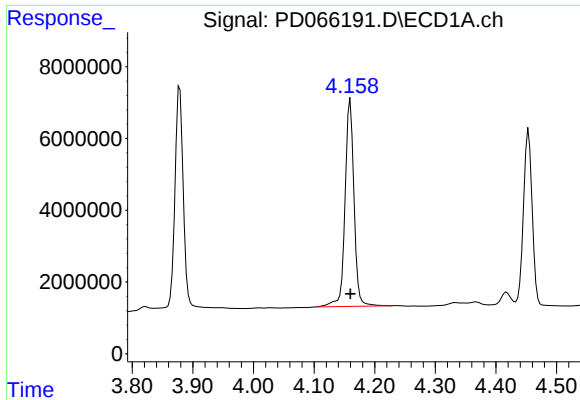

#3 gamma-BHC (Lindane)


R.T.: 4.160 min
Delta R.T.: 0.000 min
Response: 59240225
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

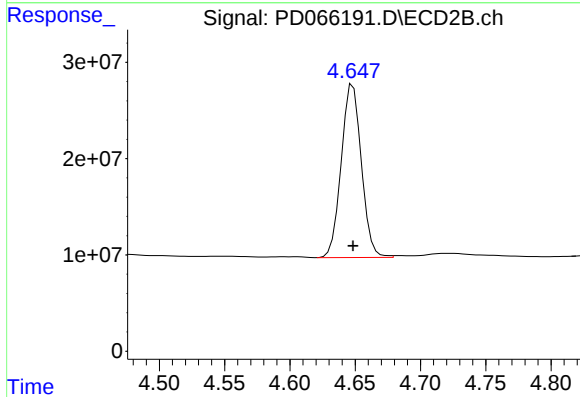


#3 gamma-BHC (Lindane)

R.T.: 4.648 min
Delta R.T.: 0.000 min
Response: 192956212
Conc: 20.00 ng/ml

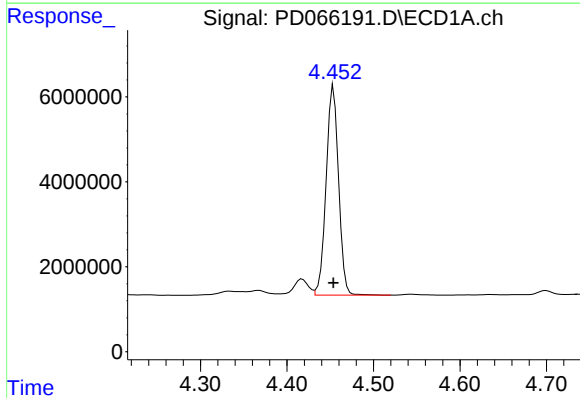


#4 Heptachlor

R.T.: 4.454 min
Delta R.T.: 0.000 min
Response: 49318134
Conc: 20.00 ng/ml

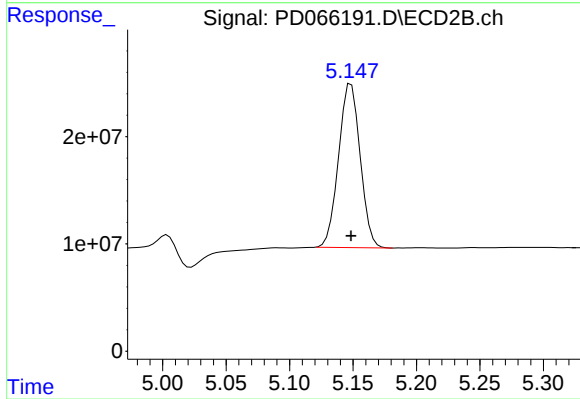

#4 Heptachlor


R.T.: 5.148 min
Delta R.T.: 0.000 min
Response: 180880815
Conc: 20.00 ng/ml

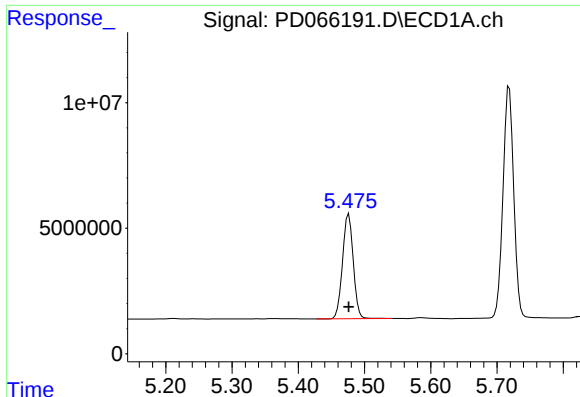

#9 Endosulfan I


R.T.: 5.476 min
Delta R.T.: 0.000 min
Response: 46828446
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

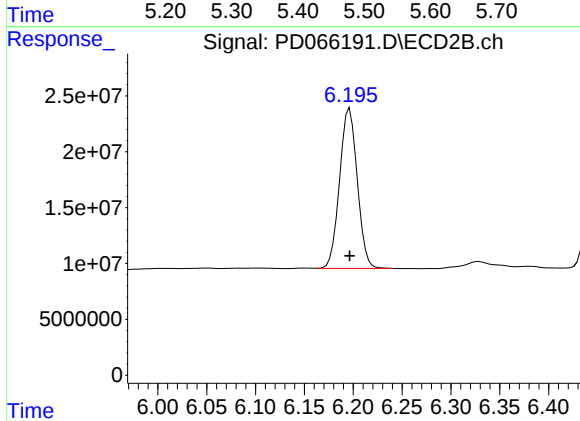


#9 Endosulfan I

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 180578458
Conc: 20.00 ng/ml

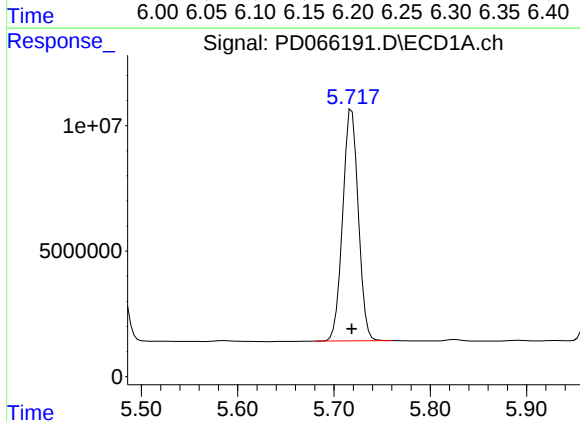


#13 Dieldrin

R.T.: 5.718 min
Delta R.T.: 0.000 min
Response: 103538480
Conc: 40.00 ng/ml

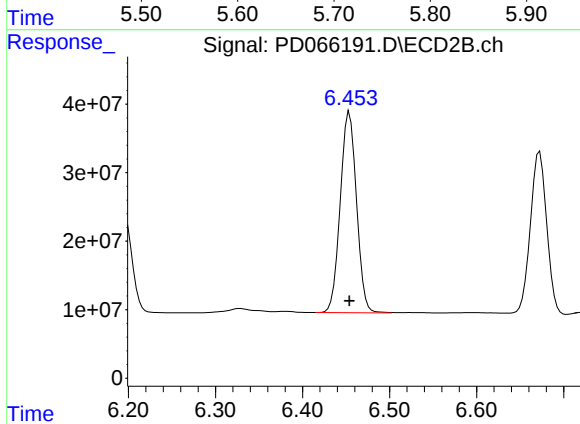

#13 Dieldrin


R.T.: 6.454 min
Delta R.T.: 0.000 min
Response: 381211259
Conc: 40.00 ng/ml

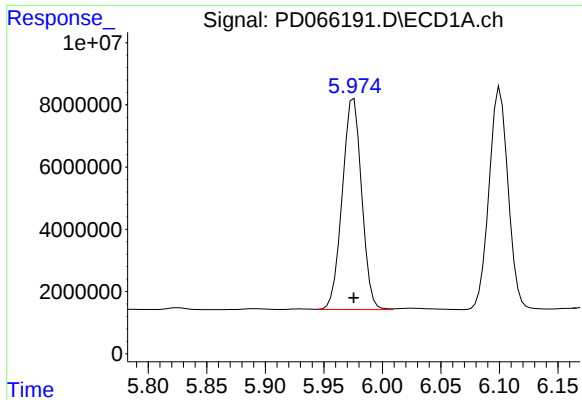

#14 Endrin


R.T.: 5.976 min
Delta R.T.: 0.000 min
Response: 78171009
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

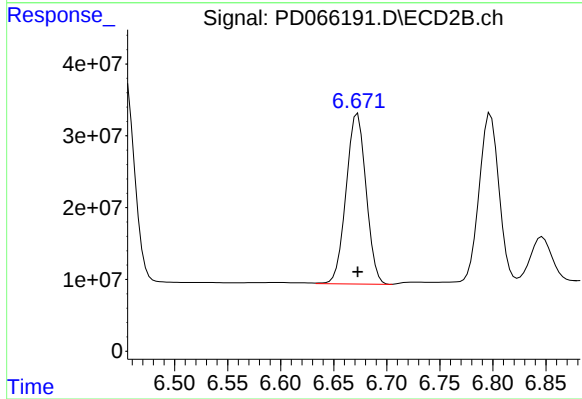


#14 Endrin

R.T.: 6.673 min
Delta R.T.: 0.000 min
Response: 310070853
Conc: 40.00 ng/ml

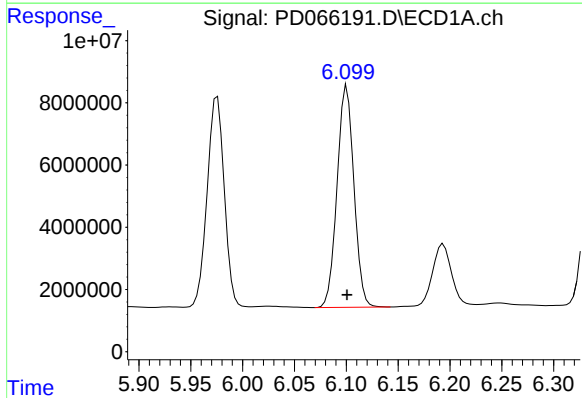


#16 4,4'-DDD

R.T.: 6.101 min
Delta R.T.: 0.000 min
Response: 80637995
Conc: 40.00 ng/ml

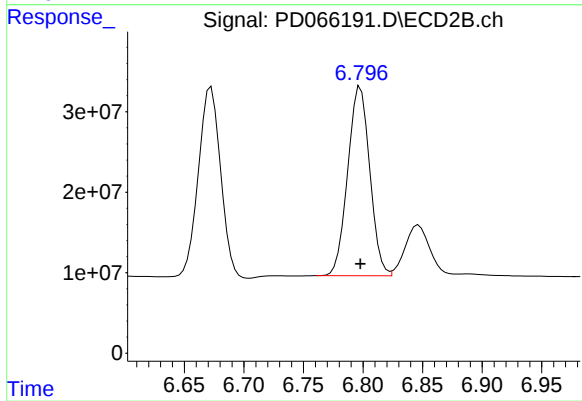

#16 4,4'-DDD


R.T.: 6.798 min
Delta R.T.: 0.000 min
Response: 303264346
Conc: 40.00 ng/ml

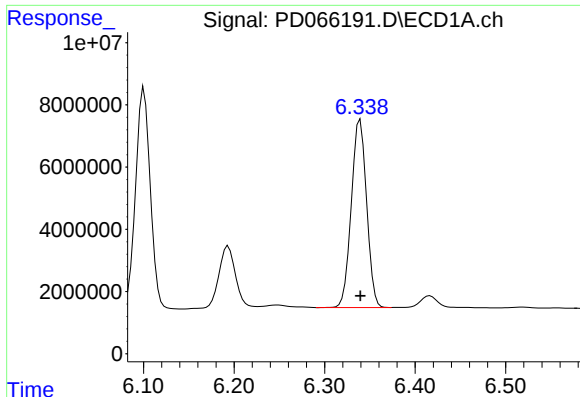

#17 4,4'-DDT


R.T.: 6.339 min
Delta R.T.: 0.000 min
Response: 71018821
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

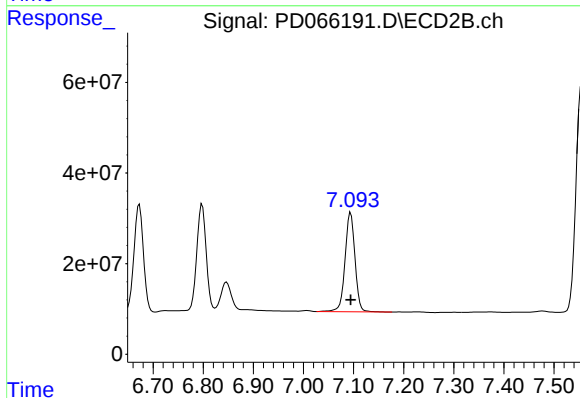


#17 4,4'-DDT

R.T.: 7.094 min
Delta R.T.: 0.000 min
Response: 303014106
Conc: 40.00 ng/ml

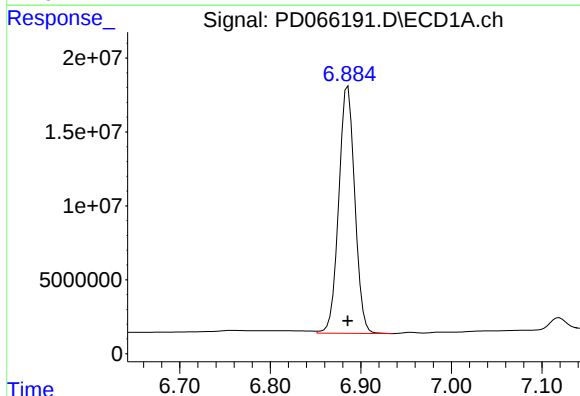


#20 Methoxychlor

R.T.: 6.886 min
Delta R.T.: 0.000 min
Response: 205672345
Conc: 200.00 ng/ml

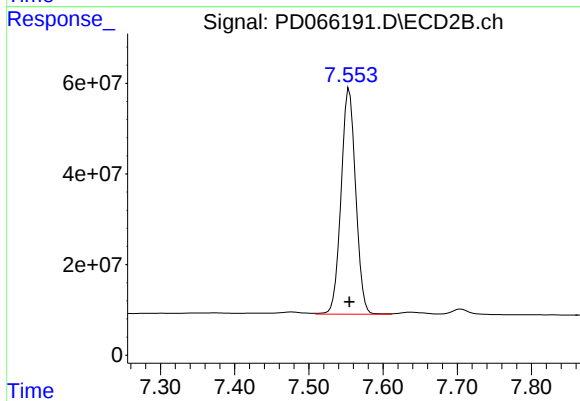

#20 Methoxychlor


R.T.: 7.554 min
Delta R.T.: 0.000 min
Response: 682659298
Conc: 200.00 ng/ml

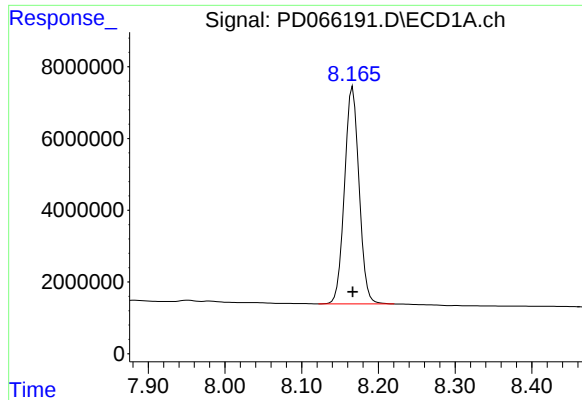

#27 Decachlorobiphenyl

R.T.: 8.166 min
Delta R.T.: 0.000 min
Response: 80091919
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

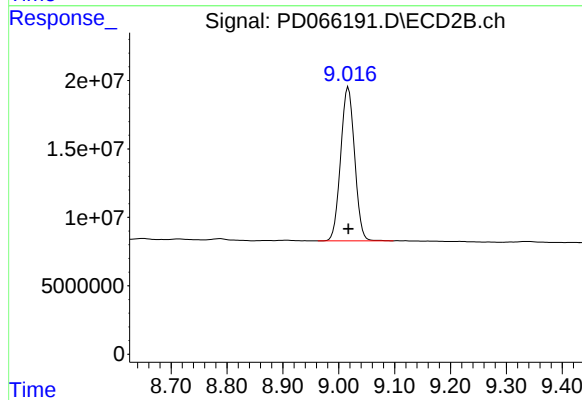

#27 Decachlorobiphenyl

R.T.: 9.017 min
Delta R.T.: 0.000 min
Response: 195076875
Conc: 40.00 ng/ml