

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101321\
 Data File : PD066193.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2021 22:21
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 05:45:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101321CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 13 05:43:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	3.972	73238046	254.6E6	38.586	37.488
27)	SA Decachlor...	8.167	9.017	149.3E6	362.1E6	74.551	74.246
Target Compounds							
2)	A alpha-BHC	3.879	4.364	116.1E6	376.9E6	39.864	37.408
3)	MA gamma-BHC...	4.160	4.648	113.5E6	365.8E6	38.325	37.914
4)	MA Heptachlor	4.454	5.148	96977445	339.2E6	39.327	37.502
9)	A Endosulfan I	5.477	6.196	92997285	339.6E6	39.718	37.617
13)	MA Dieldrin	5.719	6.454	207.0E6	722.7E6	79.982	75.827
14)	MA Endrin	5.975	6.673	154.4E6	588.7E6	79.005	75.944
16)	A 4,4'-DDD	6.101	6.797	160.7E6	580.3E6	79.697	76.541
17)	MA 4,4'-DDT	6.339	7.094	146.6E6	564.0E6	82.566	74.448
20)	A Methoxychlor	6.886	7.555	394.4E6	1255.7E6	383.557	367.895


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101321\
Data File : PD066193.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2021 22:21
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 05:45:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101321CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 13 05:43:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

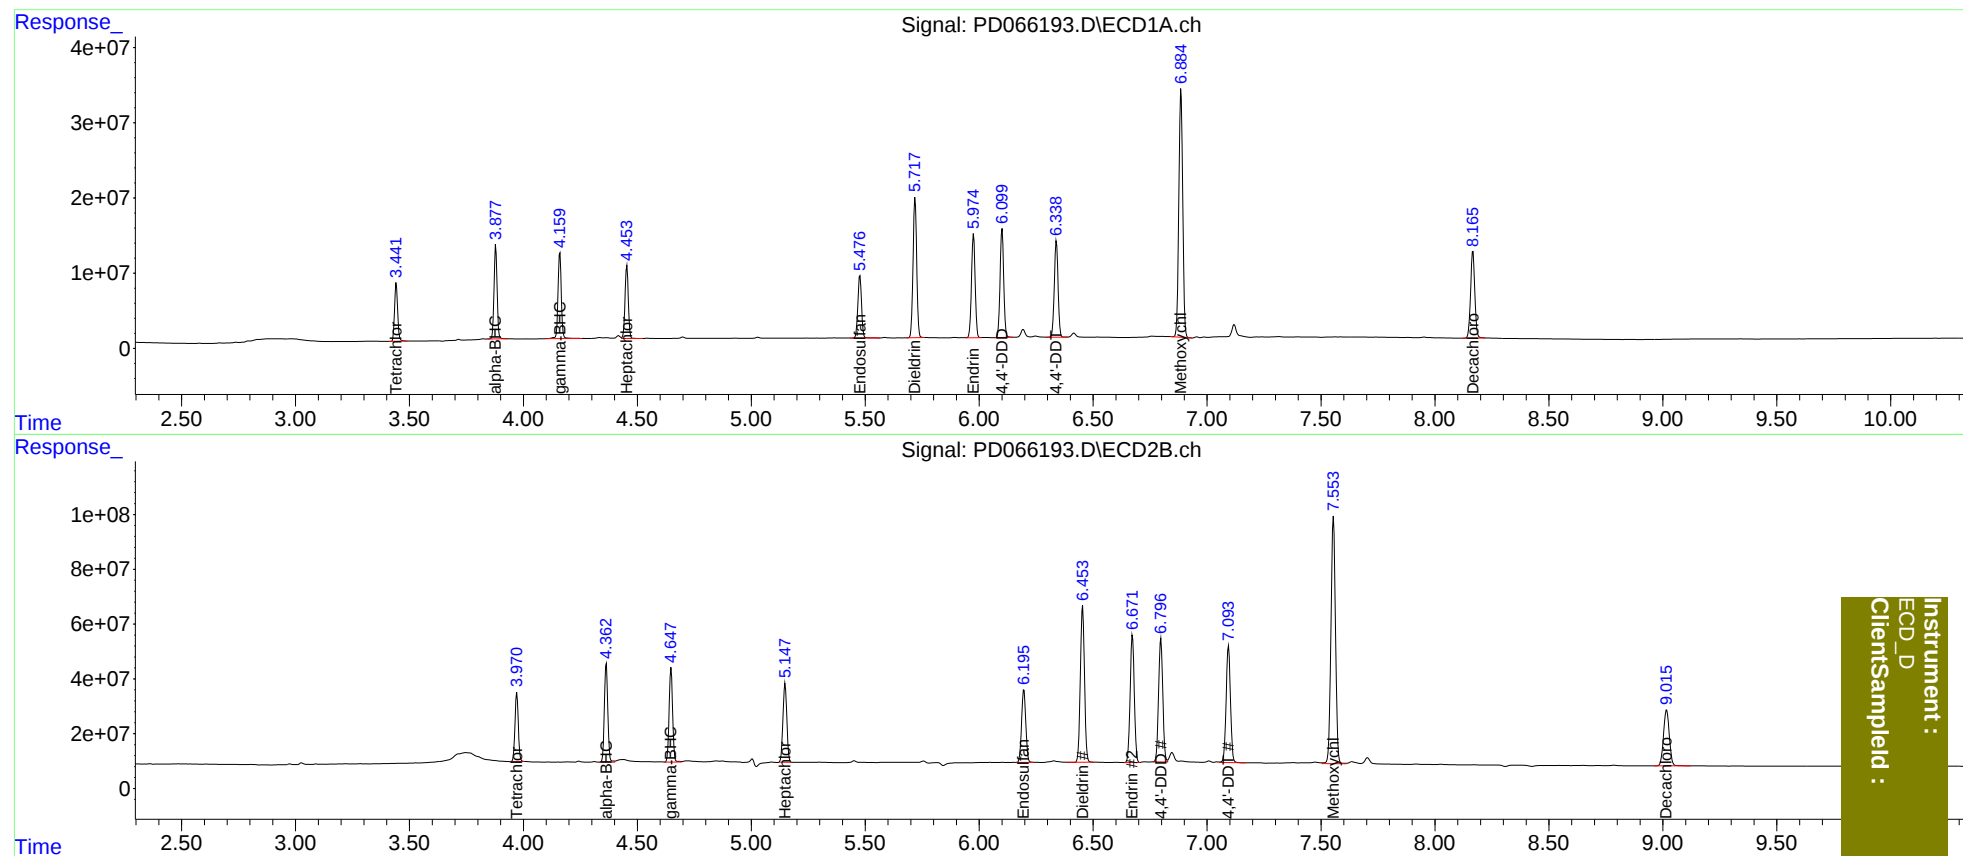


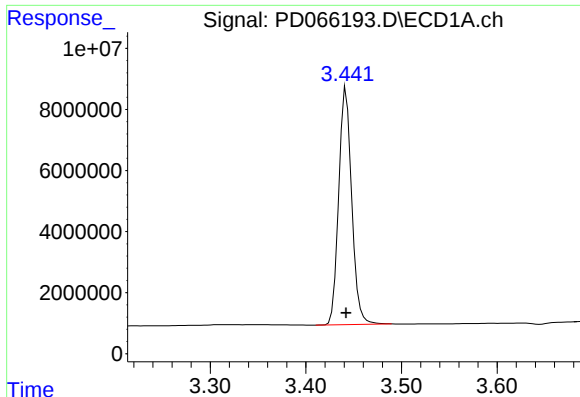

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 73238046
Conc: 38.59 ng/ml

Instrument :
ECD_D
ClientSampleId :

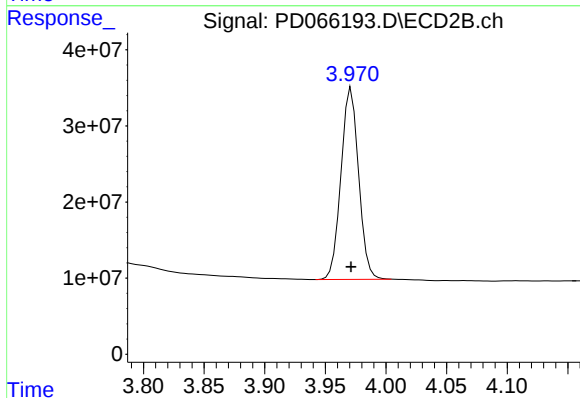


#1 Tetrachloro-m-xylene

R.T.: 3.972 min
Delta R.T.: 0.000 min
Response: 254637289
Conc: 37.49 ng/ml

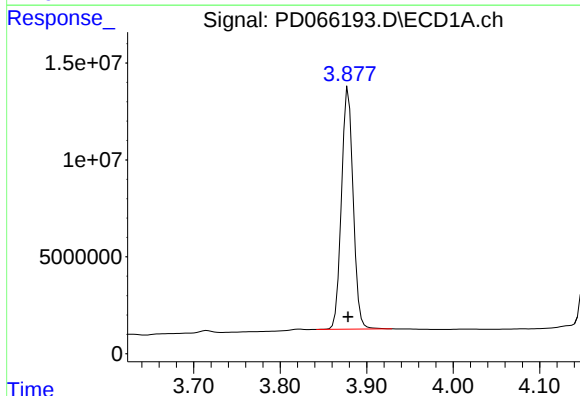


#2 alpha-BHC

R.T.: 3.879 min
Delta R.T.: 0.000 min
Response: 116071224
Conc: 39.86 ng/ml

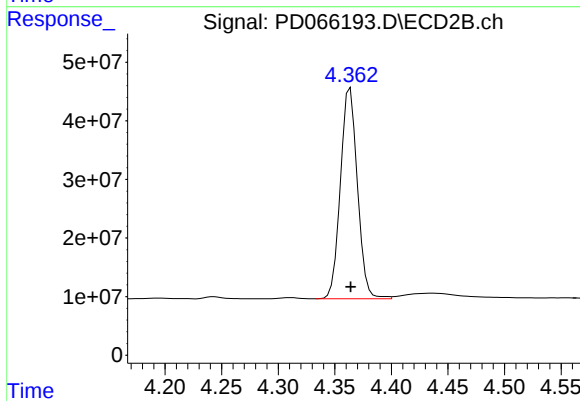

#2 alpha-BHC

R.T.: 4.364 min
Delta R.T.: 0.000 min
Response: 376864641
Conc: 37.41 ng/ml

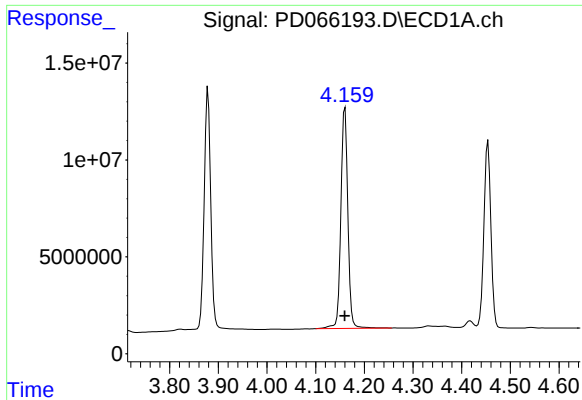

#3 gamma-BHC (Lindane)


R.T.: 4.160 min

Delta R.T.: 0.000 min

Response: 113518623

Conc: 38.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

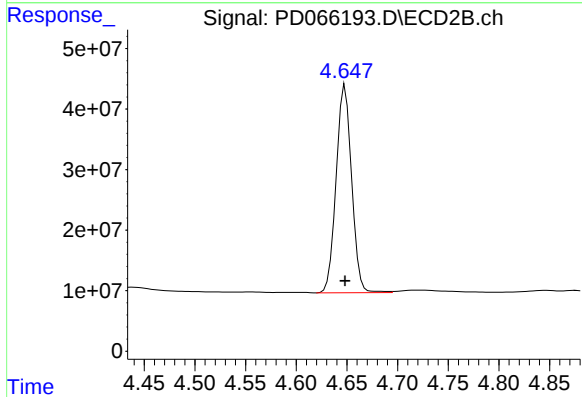


#3 gamma-BHC (Lindane)

R.T.: 4.648 min

Delta R.T.: 0.000 min

Response: 365785225

Conc: 37.91 ng/ml

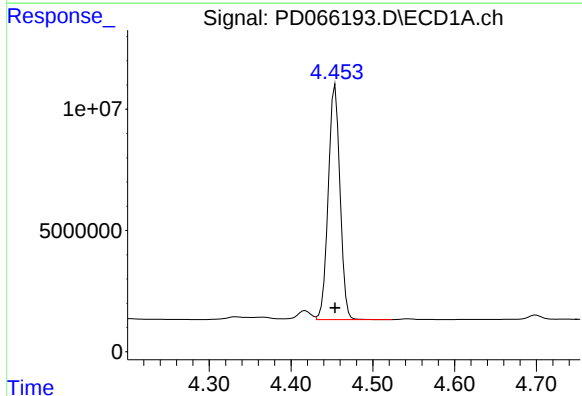


#4 Heptachlor

R.T.: 4.454 min

Delta R.T.: 0.000 min

Response: 96977445

Conc: 39.33 ng/ml

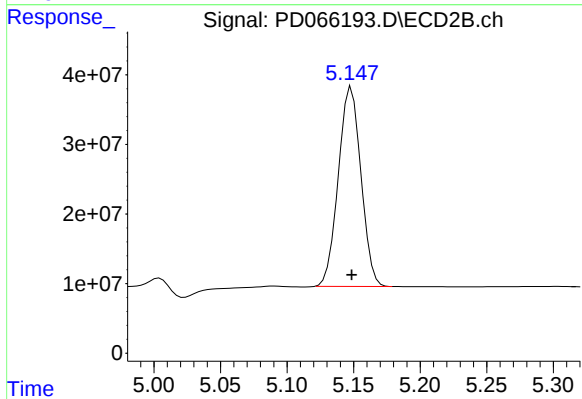


#4 Heptachlor

R.T.: 5.148 min

Delta R.T.: 0.000 min

Response: 339167151


Conc: 37.50 ng/ml

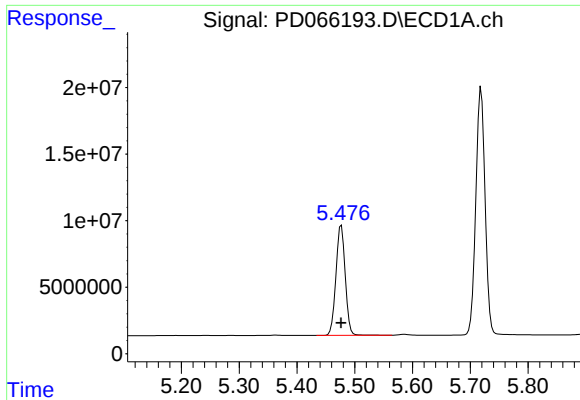

#9 Endosulfan I


R.T.: 5.477 min
Delta R.T.: 0.000 min
Response: 92997285
Conc: 39.72 ng/ml

Instrument :
ECD_D
ClientSampleId :

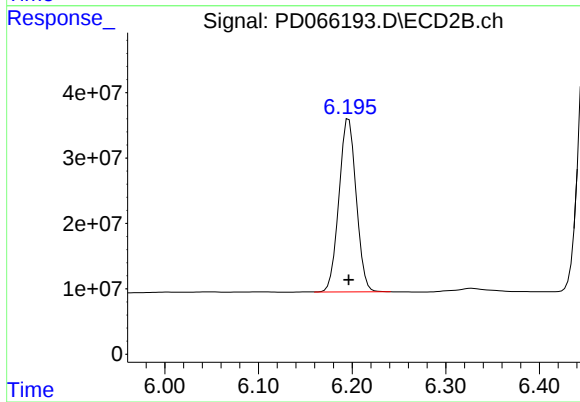


#9 Endosulfan I

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 339640302
Conc: 37.62 ng/ml

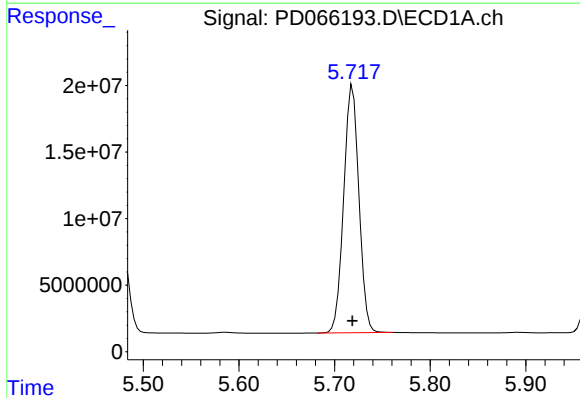


#13 Dieldrin

R.T.: 5.719 min
Delta R.T.: 0.000 min
Response: 207031245
Conc: 79.98 ng/ml

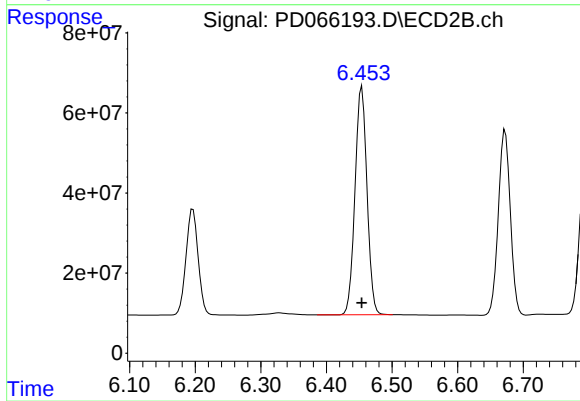

#13 Dieldrin


R.T.: 6.454 min
Delta R.T.: 0.000 min
Response: 722655969
Conc: 75.83 ng/ml

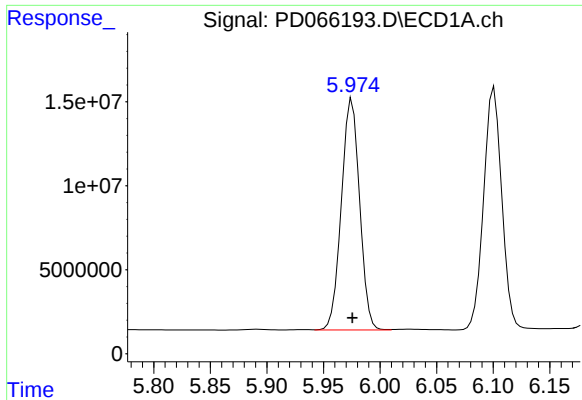

#14 Endrin


R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 154396967
Conc: 79.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

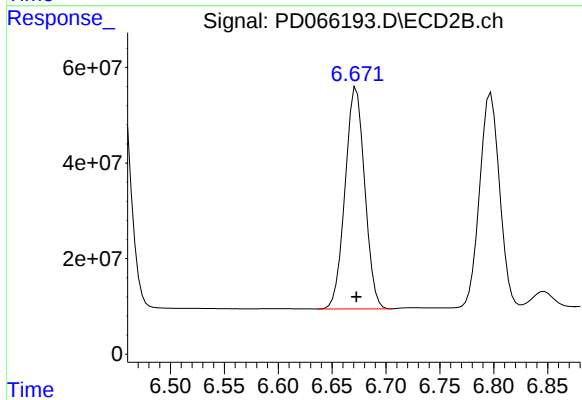


#14 Endrin

R.T.: 6.673 min
Delta R.T.: 0.000 min
Response: 588703146
Conc: 75.94 ng/ml

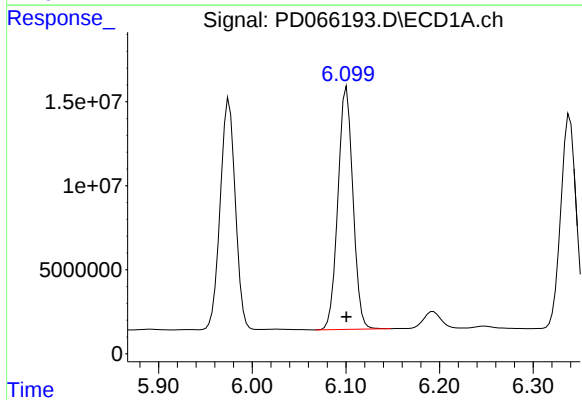


#16 4,4'-DDD

R.T.: 6.101 min
Delta R.T.: 0.000 min
Response: 160664335
Conc: 79.70 ng/ml

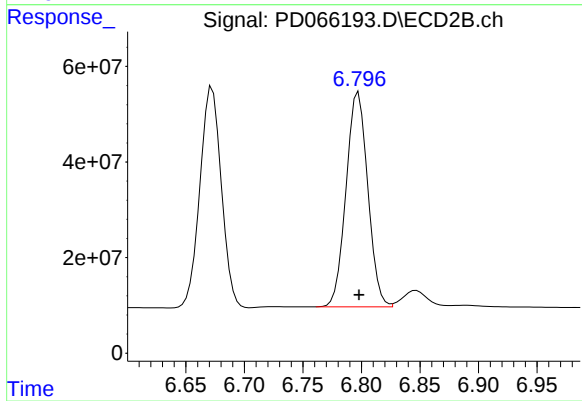

#16 4,4'-DDD


R.T.: 6.797 min
Delta R.T.: 0.000 min
Response: 580304074
Conc: 76.54 ng/ml

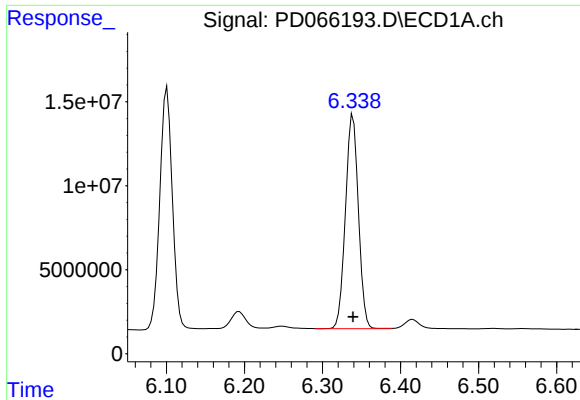

#17 4,4'-DDT


R.T.: 6.339 min
Delta R.T.: 0.000 min
Response: 146594016
Conc: 82.57 ng/ml

Instrument :
ECD_D
ClientSampleId :

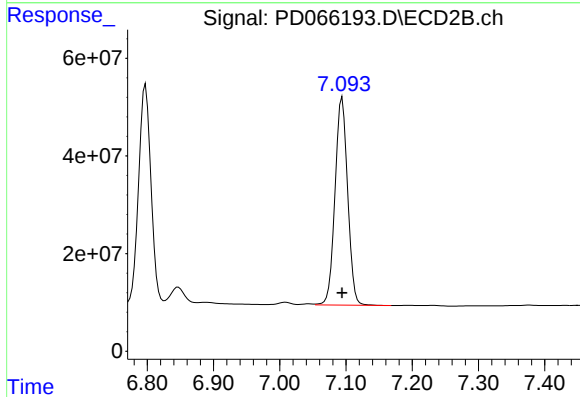


#17 4,4'-DDT

R.T.: 7.094 min
Delta R.T.: 0.000 min
Response: 563967331
Conc: 74.45 ng/ml

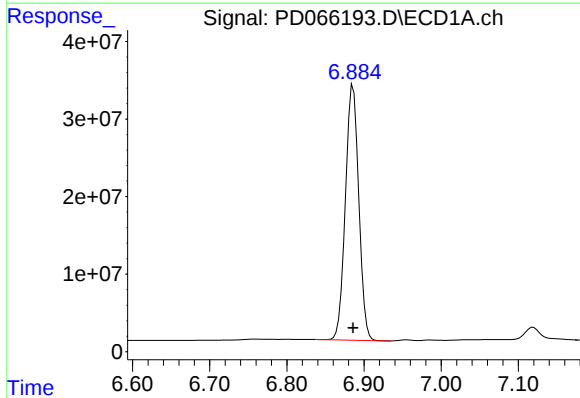


#20 Methoxychlor

R.T.: 6.886 min
Delta R.T.: 0.000 min
Response: 394435081
Conc: 383.56 ng/ml

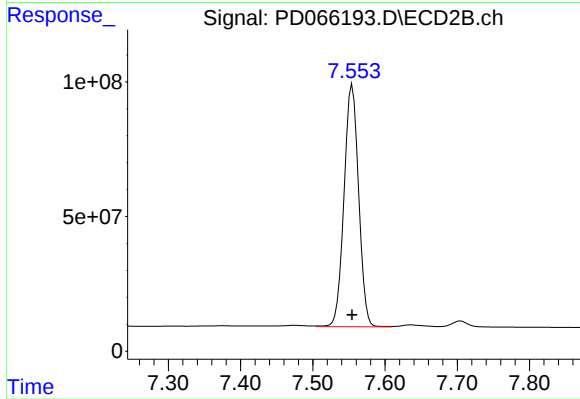

#20 Methoxychlor


R.T.: 7.555 min
Delta R.T.: 0.000 min
Response: 1255733420
Conc: 367.89 ng/ml

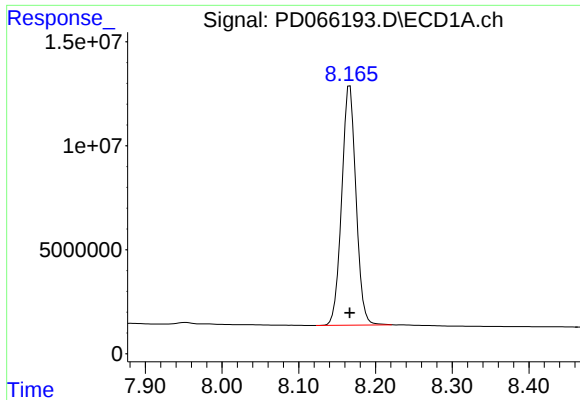

#27 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: 0.000 min
Response: 149273234
Conc: 74.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

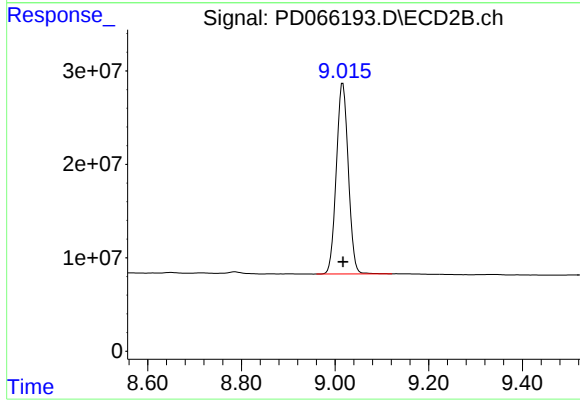

#27 Decachlorobiphenyl

R.T.: 9.017 min
Delta R.T.: 0.000 min
Response: 362092442
Conc: 74.25 ng/ml