

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101321\
 Data File : PD066195.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2021 22:48
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 05:45:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101321CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 13 05:43:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	3.971	147.7E6	488.5E6	77.824	71.921
27)	SA Decachlor...	8.168	9.018	295.4E6	672.8E6	147.526	137.957
Target Compounds							
2)	A alpha-BHC	3.879	4.364	236.8E6	732.5E6	81.345	72.711
3)	MA gamma-BHC...	4.160	4.649	221.9E6	705.5E6	74.930	73.123
4)	MA Heptachlor	4.454	5.148	192.4E6	648.4E6	78.040	71.697
9)	A Endosulfan I	5.477	6.197	186.0E6	643.7E6	79.436	71.296
13)	MA Dieldrin	5.719	6.455	421.5E6	1396.7E6	162.847	146.554
14)	MA Endrin	5.976	6.672	309.0E6	1121.8E6	158.092	144.710
16)	A 4,4'-DDD	6.101	6.798	328.5E6	1111.3E6	162.950	146.583
17)	MA 4,4'-DDT	6.339	7.095	297.0E6	1072.2E6	167.254	141.538
20)	A Methoxychlor	6.887	7.555	765.8E6	2290.9E6	744.677	671.172


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101321\
Data File : PD066195.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2021 22:48
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 05:45:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101321CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 13 05:43:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

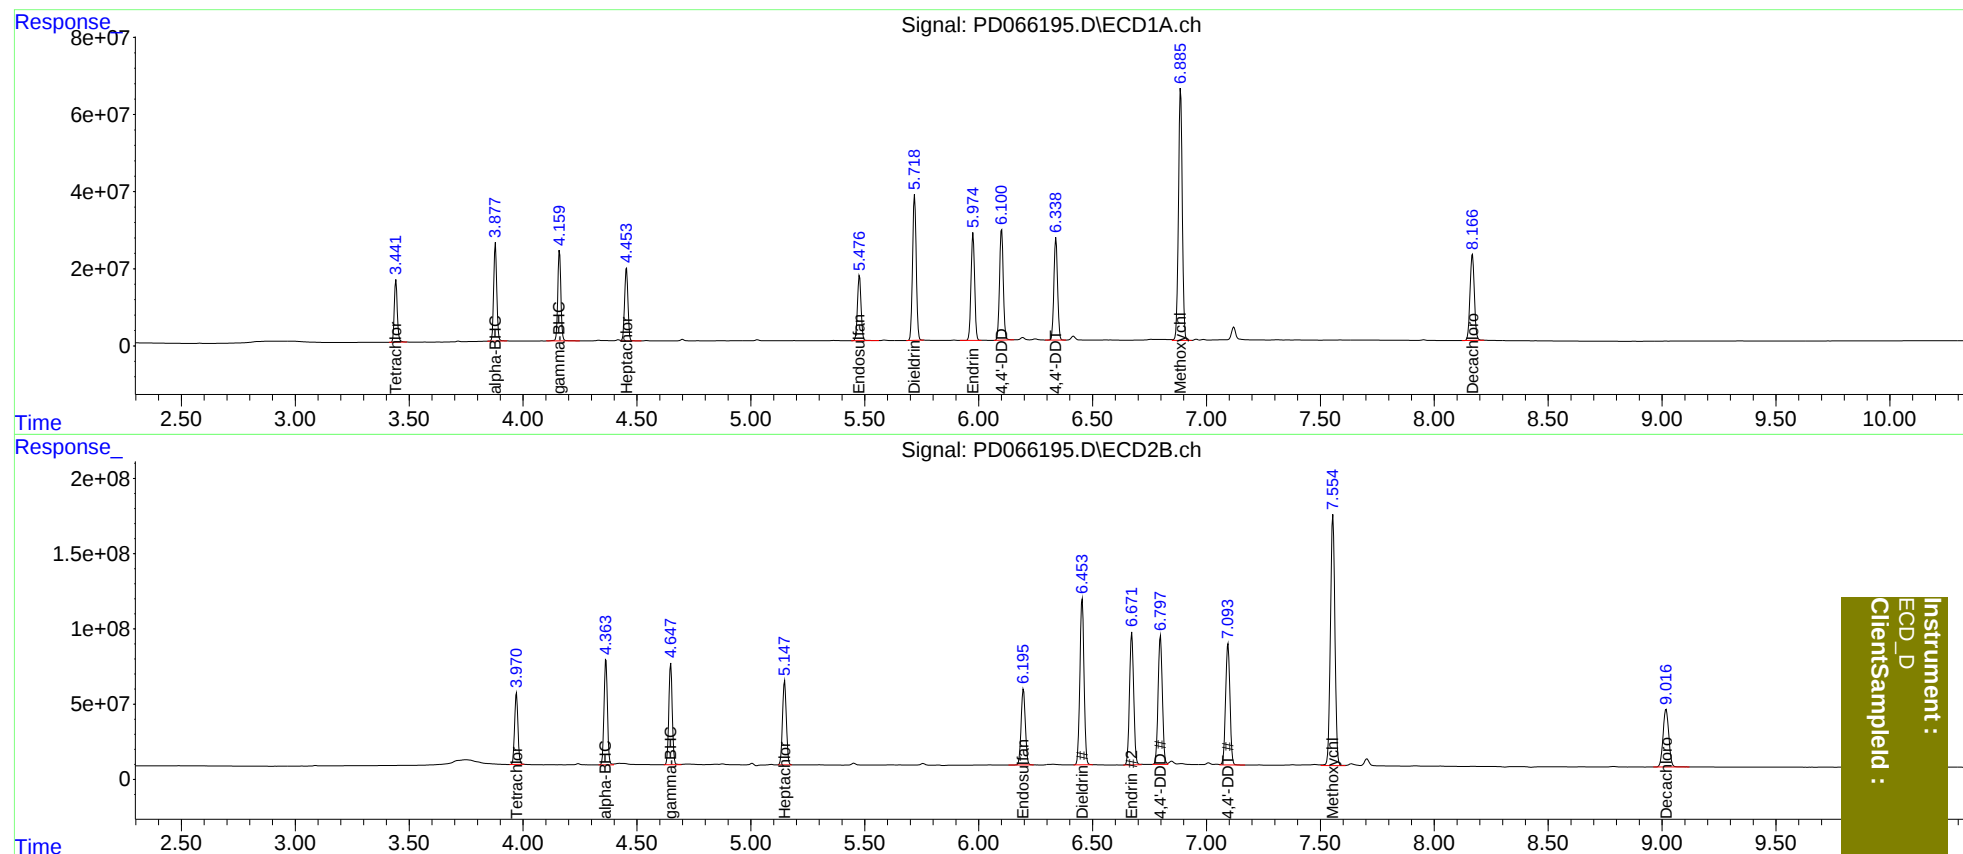


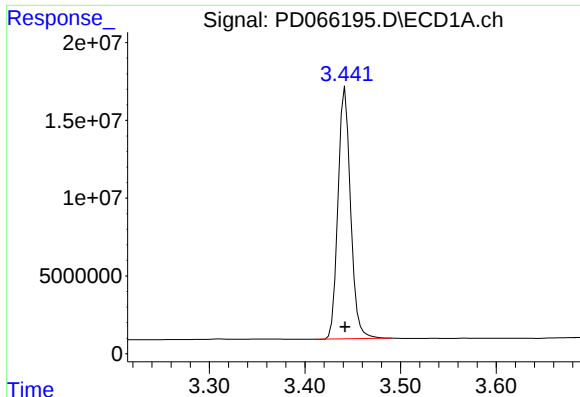

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 147713589
Conc: 77.82 ng/ml

Instrument :
ECD_D
ClientSampleId :

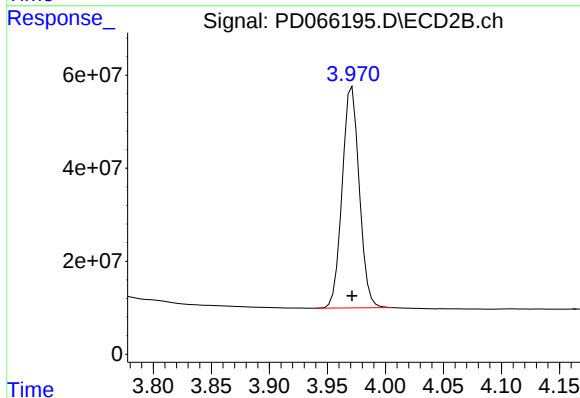


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 488529403
Conc: 71.92 ng/ml

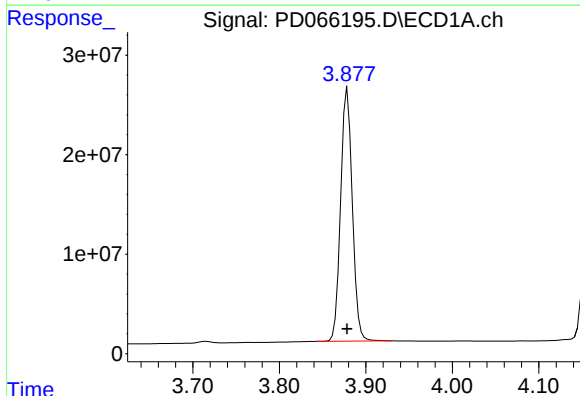


#2 alpha-BHC

R.T.: 3.879 min
Delta R.T.: 0.000 min
Response: 236848824
Conc: 81.34 ng/ml

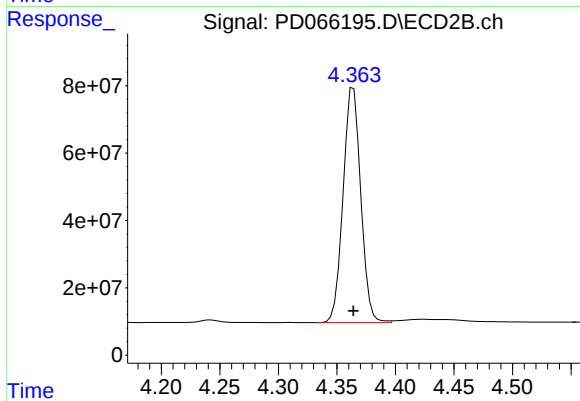

#2 alpha-BHC


R.T.: 4.364 min
Delta R.T.: 0.000 min
Response: 732520826
Conc: 72.71 ng/ml

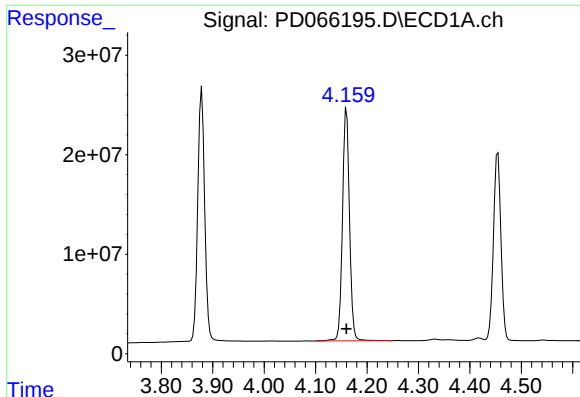

#3 gamma-BHC (Lindane)


R.T.: 4.160 min
Delta R.T.: 0.000 min
Response: 221943630
Conc: 74.93 ng/ml

Instrument :
ECD_D
ClientSampleId :

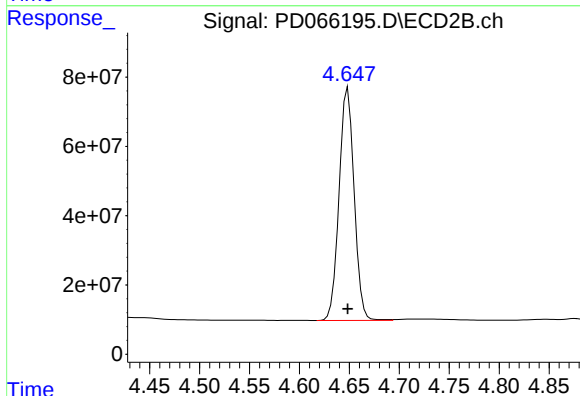


#3 gamma-BHC (Lindane)

R.T.: 4.649 min
Delta R.T.: 0.000 min
Response: 705481235
Conc: 73.12 ng/ml

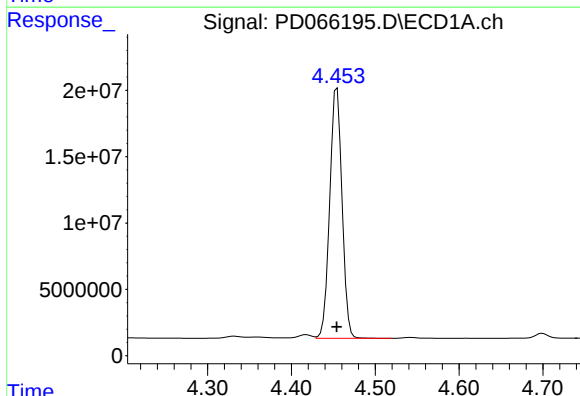


#4 Heptachlor

R.T.: 4.454 min
Delta R.T.: 0.000 min
Response: 192438582
Conc: 78.04 ng/ml

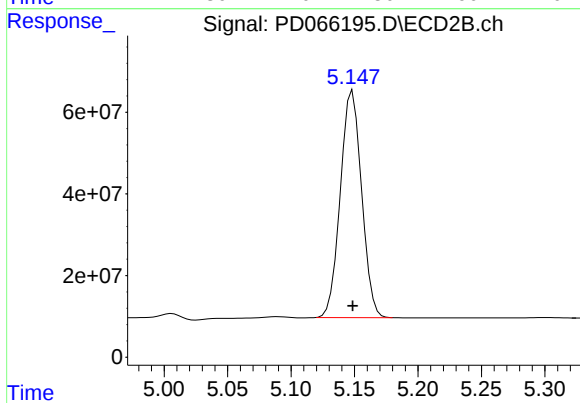

#4 Heptachlor


R.T.: 5.148 min
Delta R.T.: 0.000 min
Response: 648430585
Conc: 71.70 ng/ml

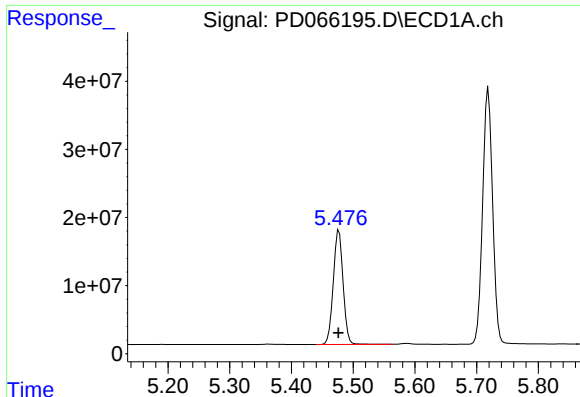

#9 Endosulfan I


R.T.: 5.477 min
Delta R.T.: 0.000 min
Response: 185993023
Conc: 79.44 ng/ml

Instrument :
ECD_D
ClientSampleId :

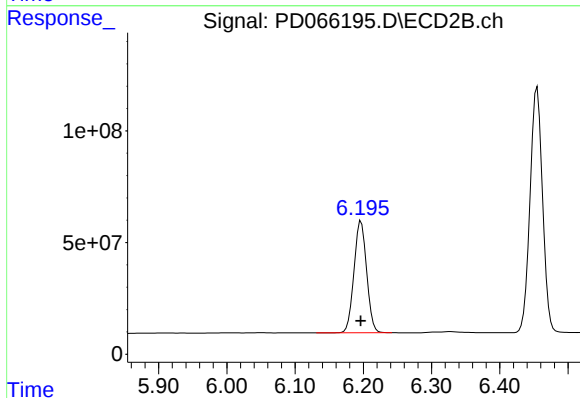


#9 Endosulfan I

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 643727573
Conc: 71.30 ng/ml

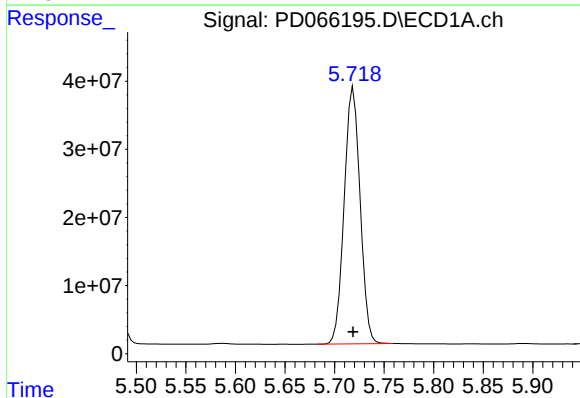


#13 Dieldrin

R.T.: 5.719 min
Delta R.T.: 0.000 min
Response: 421523260
Conc: 162.85 ng/ml

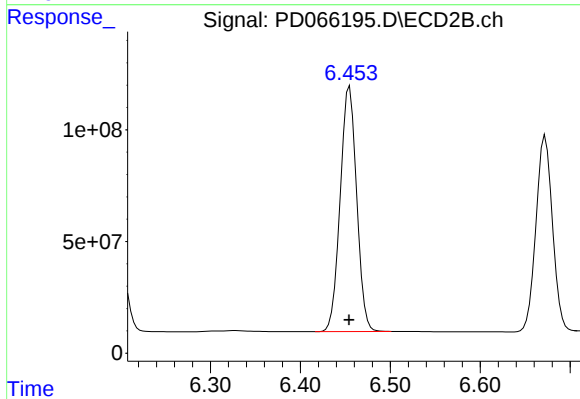

#13 Dieldrin


R.T.: 6.455 min
Delta R.T.: 0.000 min
Response: 1396696477
Conc: 146.55 ng/ml

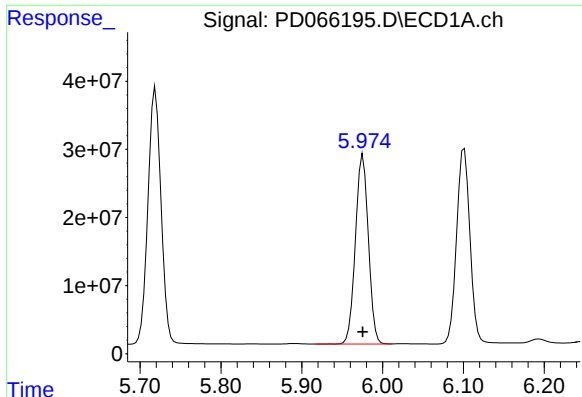

#14 Endrin


R.T.: 5.976 min
Delta R.T.: 0.000 min
Response: 308954610
Conc: 158.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

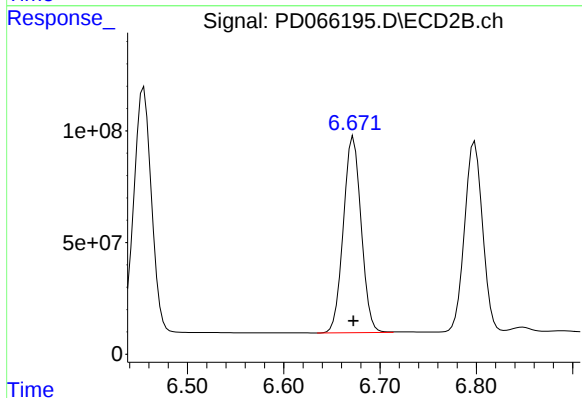


#14 Endrin

R.T.: 6.672 min
Delta R.T.: 0.000 min
Response: 1121756542
Conc: 144.71 ng/ml

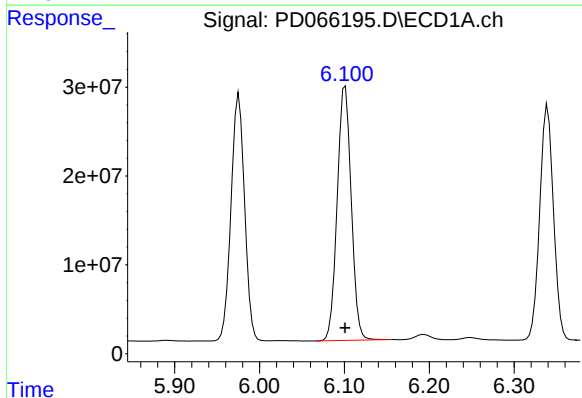


#16 4,4'-DDD

R.T.: 6.101 min
Delta R.T.: 0.000 min
Response: 328499616
Conc: 162.95 ng/ml

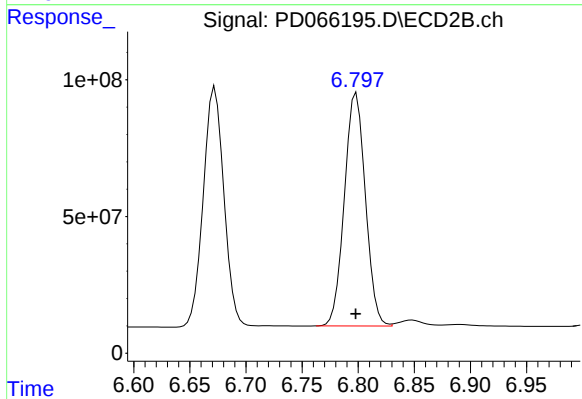

#16 4,4'-DDD


R.T.: 6.798 min
Delta R.T.: 0.000 min
Response: 1111332679
Conc: 146.58 ng/ml

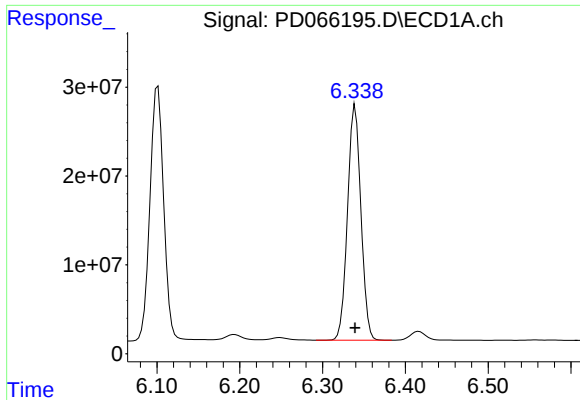

#17 4,4'-DDT


R.T.: 6.339 min
Delta R.T.: 0.000 min
Response: 296953873
Conc: 167.25 ng/ml

Instrument :
ECD_D
ClientSampleId :

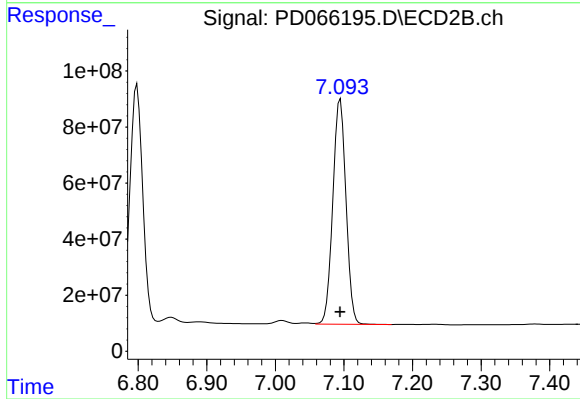


#17 4,4'-DDT

R.T.: 7.095 min
Delta R.T.: 0.000 min
Response: 1072202386
Conc: 141.54 ng/ml

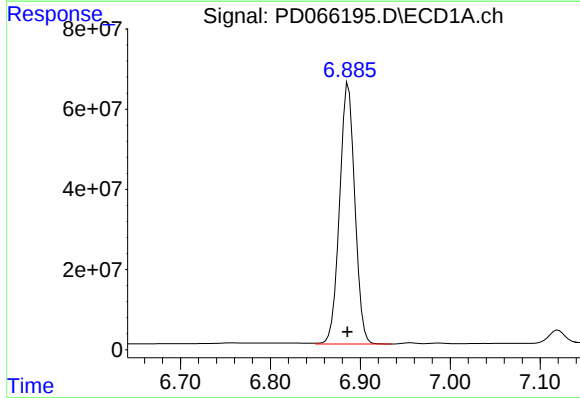


#20 Methoxychlor

R.T.: 6.887 min
Delta R.T.: 0.001 min
Response: 765797760
Conc: 744.68 ng/ml

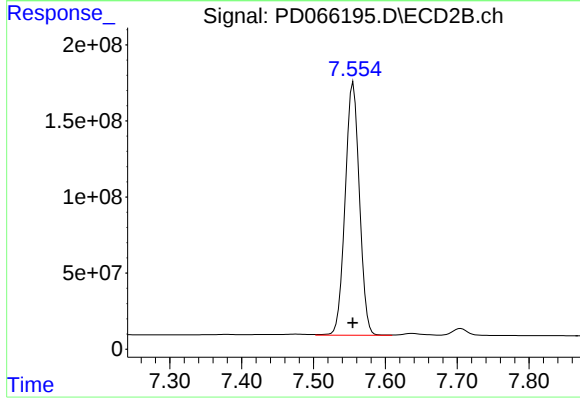

#20 Methoxychlor


R.T.: 7.555 min
Delta R.T.: 0.000 min
Response: 2290909903
Conc: 671.17 ng/ml

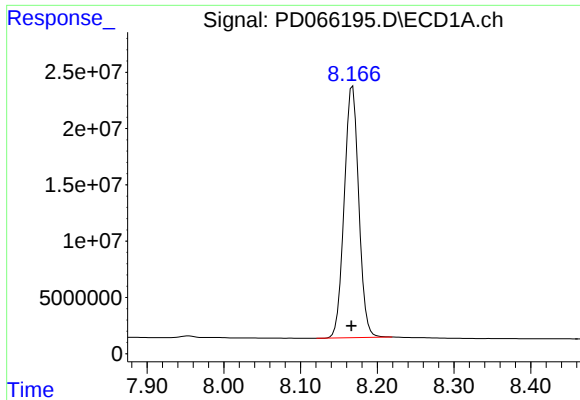

#27 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: 0.001 min
Response: 295390184
Conc: 147.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

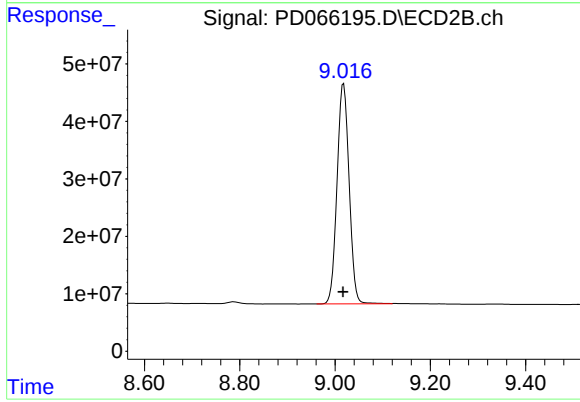

#27 Decachlorobiphenyl

R.T.: 9.018 min
Delta R.T.: 0.000 min
Response: 672803630
Conc: 137.96 ng/ml