

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101323\
Data File : PD078831.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2023 17:35
Operator : AR\AJ
Sample : 04696-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT4-2023-07

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 10/12/2023
Supervised By :Ankita Jodhani 10/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 22:18:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 01:02:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

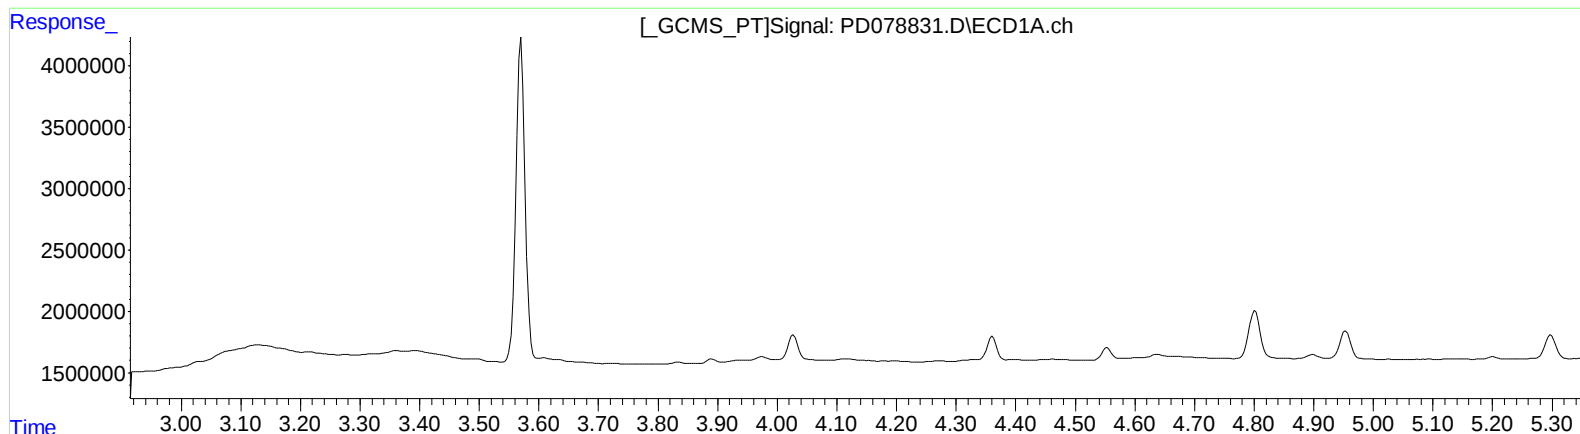

(6) beta-BHC (B)

0.000min 0.000 ng/ml

response 0

(6) beta-BHC #2 (B)

3.937min 0.696 ng/ml

response 865962

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101323\
Data File : PD078831.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2023 17:35
Operator : AR\AJ
Sample : 04696-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT4-2023-07

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 10/12/2023
Supervised By :Ankita Jodhani 10/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 22:18:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 01:02:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

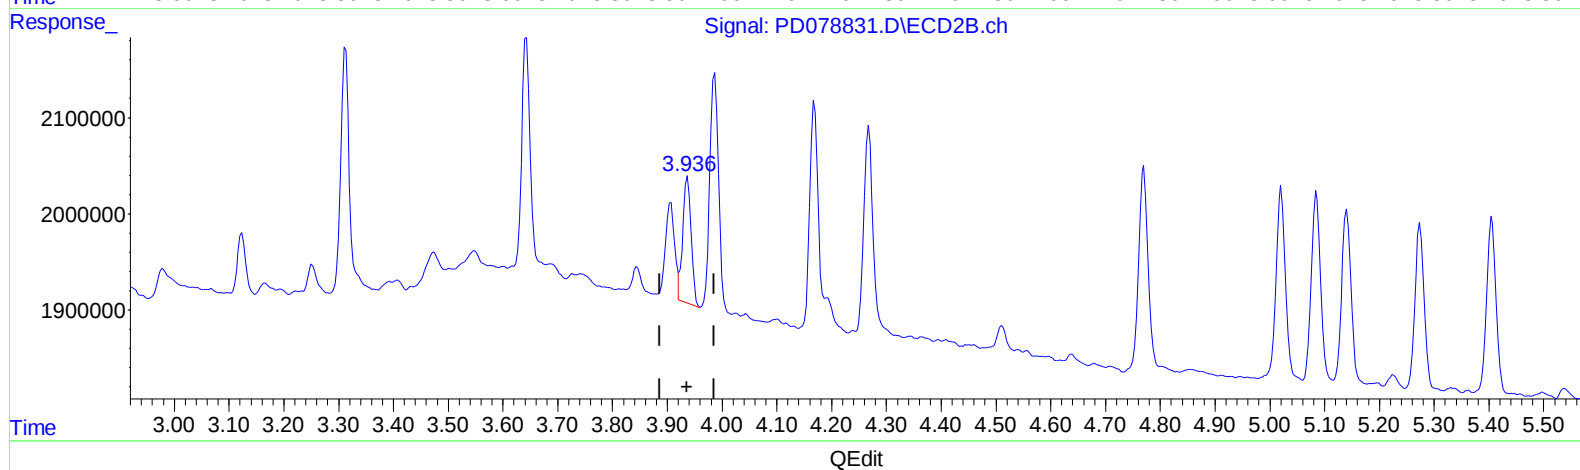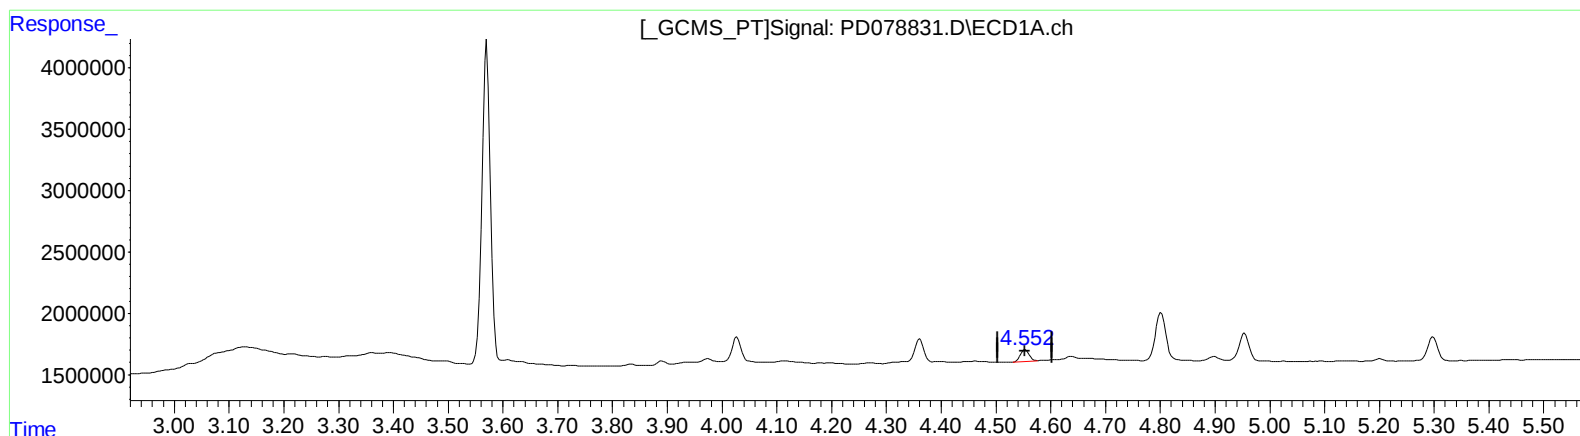

(6) beta-BHC (B)

4.552min 0.935 ng/ml m

response 1085053

(6) beta-BHC #2 (B)

3.936min 1.118 ng/ml m

response 1392028

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101323\
Data File : PD078831.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2023 17:35
Operator : AR\AJ
Sample : 04696-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT4-2023-07

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 10/12/2023
Supervised By :Ankita Jodhani 10/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 22:18:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 01:02:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

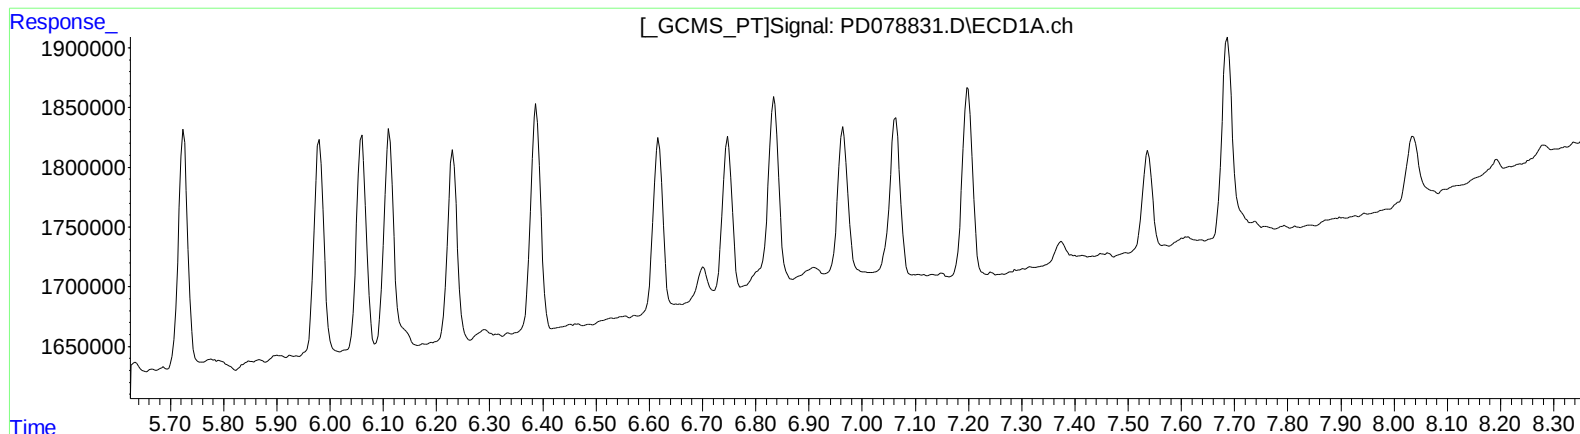

(20) Methoxychlor (A)

0.000min 0.000 ng/ml

response 0

(20) Methoxychlor #2 (A)

6.655min 1.414 ng/ml

response 1105532

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101323\
 Data File : PD078831.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2023 17:35
 Operator : AR\AJ
 Sample : 04696-01
 Misc : PEST MDL WATER
 ALS Vial : 6 Sample Multiplier: 1


Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-QT4-2023-07

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 10/12/2023
 Supervised By :Ankita Jodhani 10/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 22:18:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 11 01:02:10 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

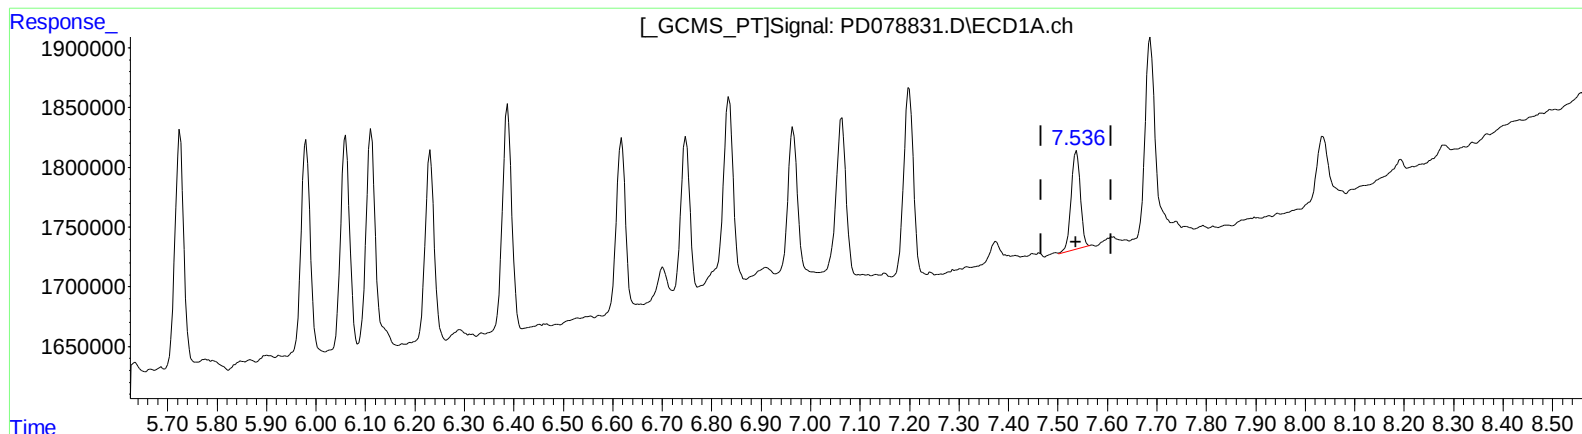

(20) Methoxychlor (A)
 7.536min 1.130 ng/ml m
 response 1061526

(20) Methoxychlor #2 (A)
 6.655min 1.414 ng/ml
 response 1105532

QEdit