

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101419\
Data File : PD055250.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2019 11:26
Operator : SG\AJ
Sample : PB123911BS
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PLCS11

Manual Integrations
APPROVED

Ankita
10/15/2019 11:38:32 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 02:28:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
Quant Title : GC Extractables
QLast Update : Tue Sep 24 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

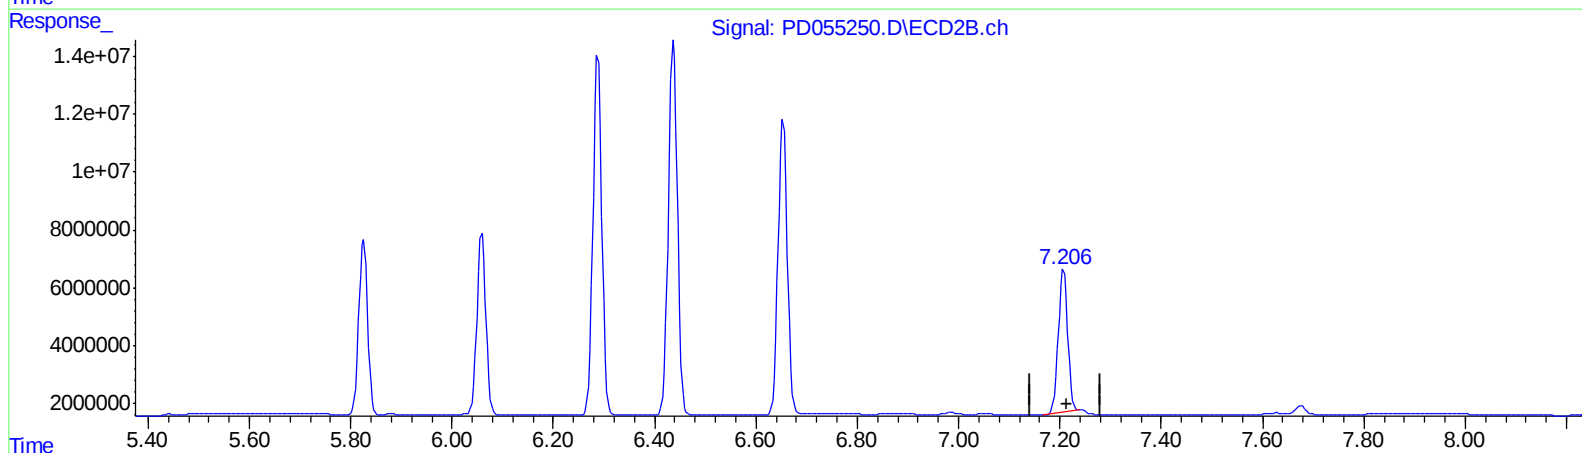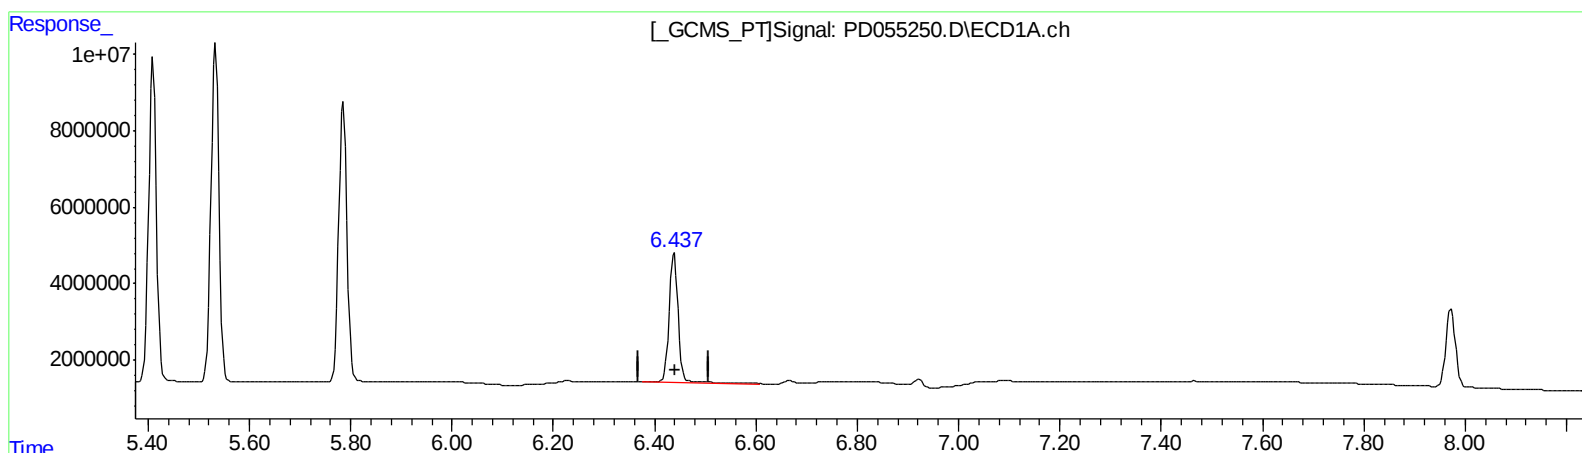

QEdit

(19) Endosulfan Sulfate (B)

6.439min 50.779 ng/ml

response 41214319

(19) Endosulfan Sulfate #2 (B)

7.208min 52.100 ng/ml

response 61883153

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101419\
Data File : PD055250.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2019 11:26
Operator : SG\AJ
Sample : PB123911BS
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampled :
PLCS11

Manual Integrations
APPROVED

Ankita
10/15/2019 11:38:32 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 02:28:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
Quant Title : GC Extractables
QLast Update : Tue Sep 24 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

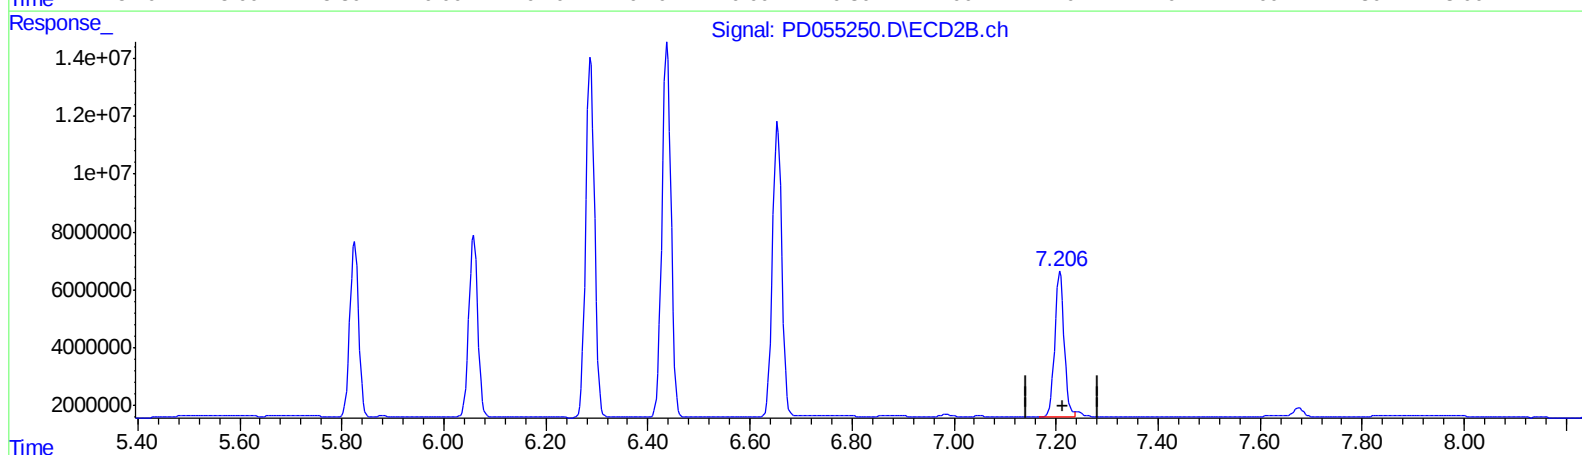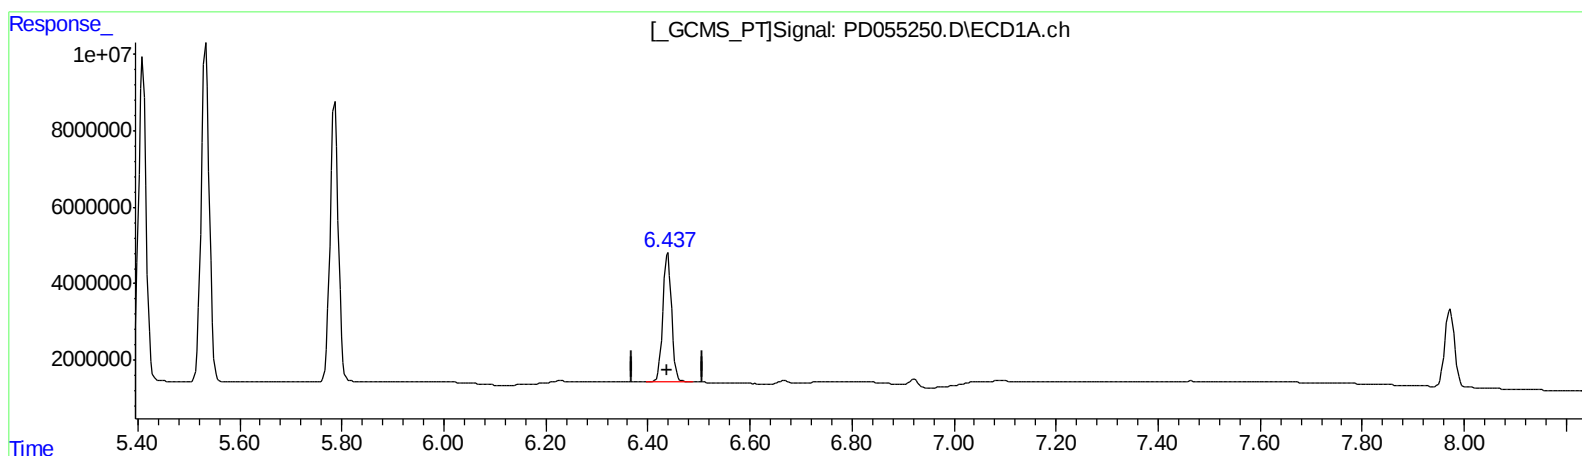

QEdit

(19) Endosulfan Sulfate (B)

6.437min 49.217 ng/ml m

response 39946476

(19) Endosulfan Sulfate #2 (B)

7.206min 55.533 ng/ml m

response 65960993

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101419\
 Data File : PD055250.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2019 11:26
 Operator : SG\AJ
 Sample : PB123911BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS11

Manual Integrations
 APPROVED

Ankita
 10/15/2019 11:38:32 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 02:28:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 24 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.295	3.961	13043839	19671151	17.146	19.169
27) SA Decachlor...	7.973	9.000	27225947	40240404	32.312	34.539
Target Compounds						
3) MA gamma-BHC...	3.999	4.631	41643867	65839465	38.837	47.021
8) B Heptachlo...	4.962	5.826	46292163	73047017	50.448	55.548
10) B trans-Chl...	5.184	6.059	46877740	76152069	49.624	56.184
12) B 4,4'-DDE	5.410	6.288	89391048	150.2E6	99.630	116.058
13) MA Dieldrin	5.533	6.437	98602607	159.8E6	100.173	114.493
14) MA Endrin	5.786	6.654	82799978	128.3E6	99.581	116.524
19) B Endosulfa...	6.437	7.206	39946476	65960993	49.217m	55.533m

13
 10124119

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.