

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101421\
 Data File : PD066233.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2021 16:53
 Operator : AR\AJ
 Sample : M4029-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C00R0

Manual Integrations
 APPROVED

mohammad
 10/14/2021 2:16:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 08:45:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101321CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 13 06:25:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.442	3.971	37213147	123.1E6	19.543	18.220
2) SA Decachlor...	8.167	9.016	51383744	157.6E6	25.402	32.490m#
Target Compounds						
11) B cis-Chlor...	5.420	6.144	1985055	17562803	0.766m	1.826m#
13) MA Dieldrin	5.725	6.442	16563974	33976121	6.446m	3.577 #
16) A 4,4'-DDD	6.106	6.798	2401801	126.6E6	1.202	16.805m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101421\
Data File : PD066233.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2021 16:53
Operator : AR\AJ
Sample : M4029-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 08:45:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101321CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 13 06:25:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

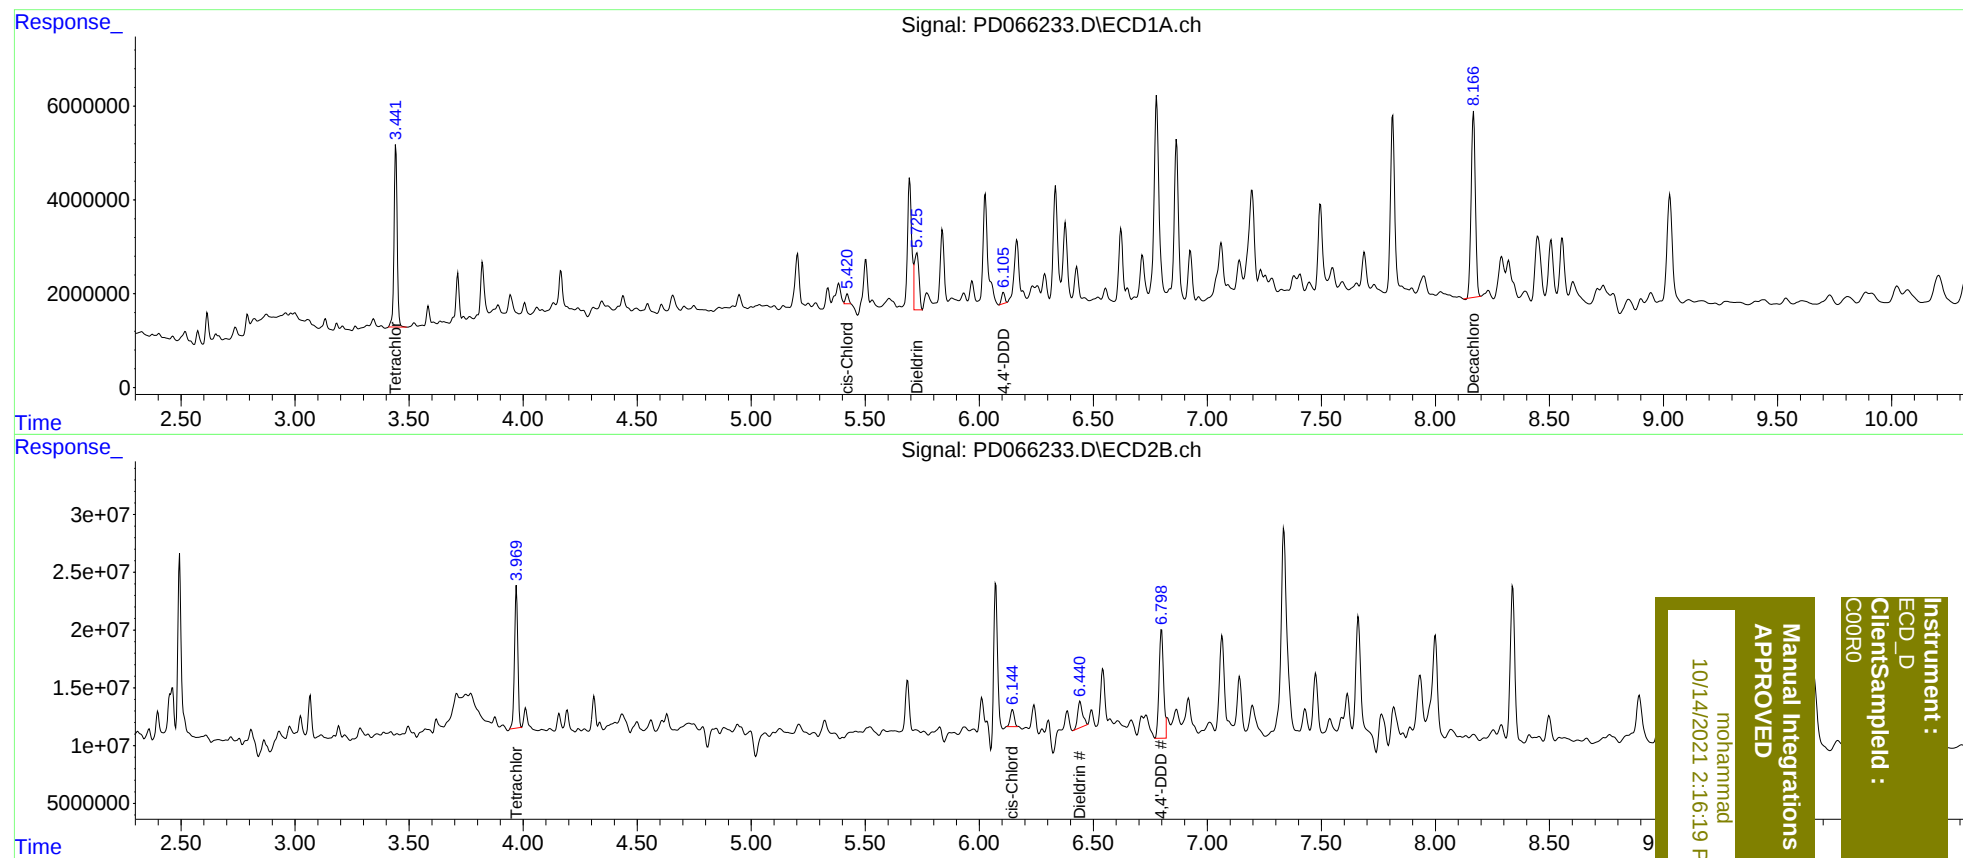

Manual Integrations
APPROVED

mohammad
10/14/2021 2:16:19 PM

Instrument :
ECD_D
ClientSampled :
C00R0