

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101422\
 Data File : PD072422.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2022 14:00
 Operator : AR\AJ
 Sample : N5060-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 00:21:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 06:06:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.709	3.469	80319680	881.8E6	32.905	36.876
27)	SA Decachlor...	7.845	8.929	92951650	330.3E6	47.585	65.392 #
Target Compounds							
2)	A alpha-BHC	3.203	0.000	870381	0	0.244	N.D. #
4)	MA Heptachlor	3.881	0.000	103431	0	<MDL	N.D. #
5)	MB Aldrin	4.203f	0.000	194057	0	<MDL	N.D. #
6)	B beta-BHC	3.881f	4.460f	103431	10720732	<MDL	1.062 #
7)	B delta-BHC	4.096	4.708	9600363	29257086	2.845	1.543 #
8)	B Heptachlo...	4.672	0.000	149744	0	<MDL	N.D. #
9)	A Endosulfan I	5.062	0.000	159684	0	<MDL	N.D. #
10)	B trans-Chl...	4.922	0.000	155523	0	<MDL	N.D. #
11)	B cis-Chlor...	4.949	0.000	240225	0	<MDL	N.D. #
12)	B 4,4'-DDE	5.184	0.000	263183	0	<MDL	N.D. #
13)	MA Dieldrin	5.296	6.272	249054	12268068	<MDL	1.287 #
14)	MA Endrin	5.571	0.000	93616	0	<MDL	N.D. #
15)	B Endosulfa...	0.000	6.787f	0	5197189	N.D.	0.720
17)	MA 4,4'-DDT	6.006	0.000	92797	0	<MDL	N.D. #
18)	B Endrin al...	6.045	0.000	82361	0	<MDL	N.D. #
20)	A Methoxychlor	6.554	0.000	438073	0	0.372	N.D. #
21)	B Endrin ke...	6.859f	0.000	206318	0	<MDL	N.D. #
22)	Toxaphene-1	5.247	0.000	188136	0	15.930	N.D. #
23)	Toxaphene-2	5.571f	0.000	93616	0	7.474	N.D. #
25)	Toxaphene-4	6.606f	0.000	76072	0	1.082	N.D. #
26)	Toxaphene-5	6.992	0.000	245703	0	6.135	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101422\
Data File : PD072422.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2022 14:00
Operator : AR\AJ
Sample : N5060-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 00:21:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 06:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

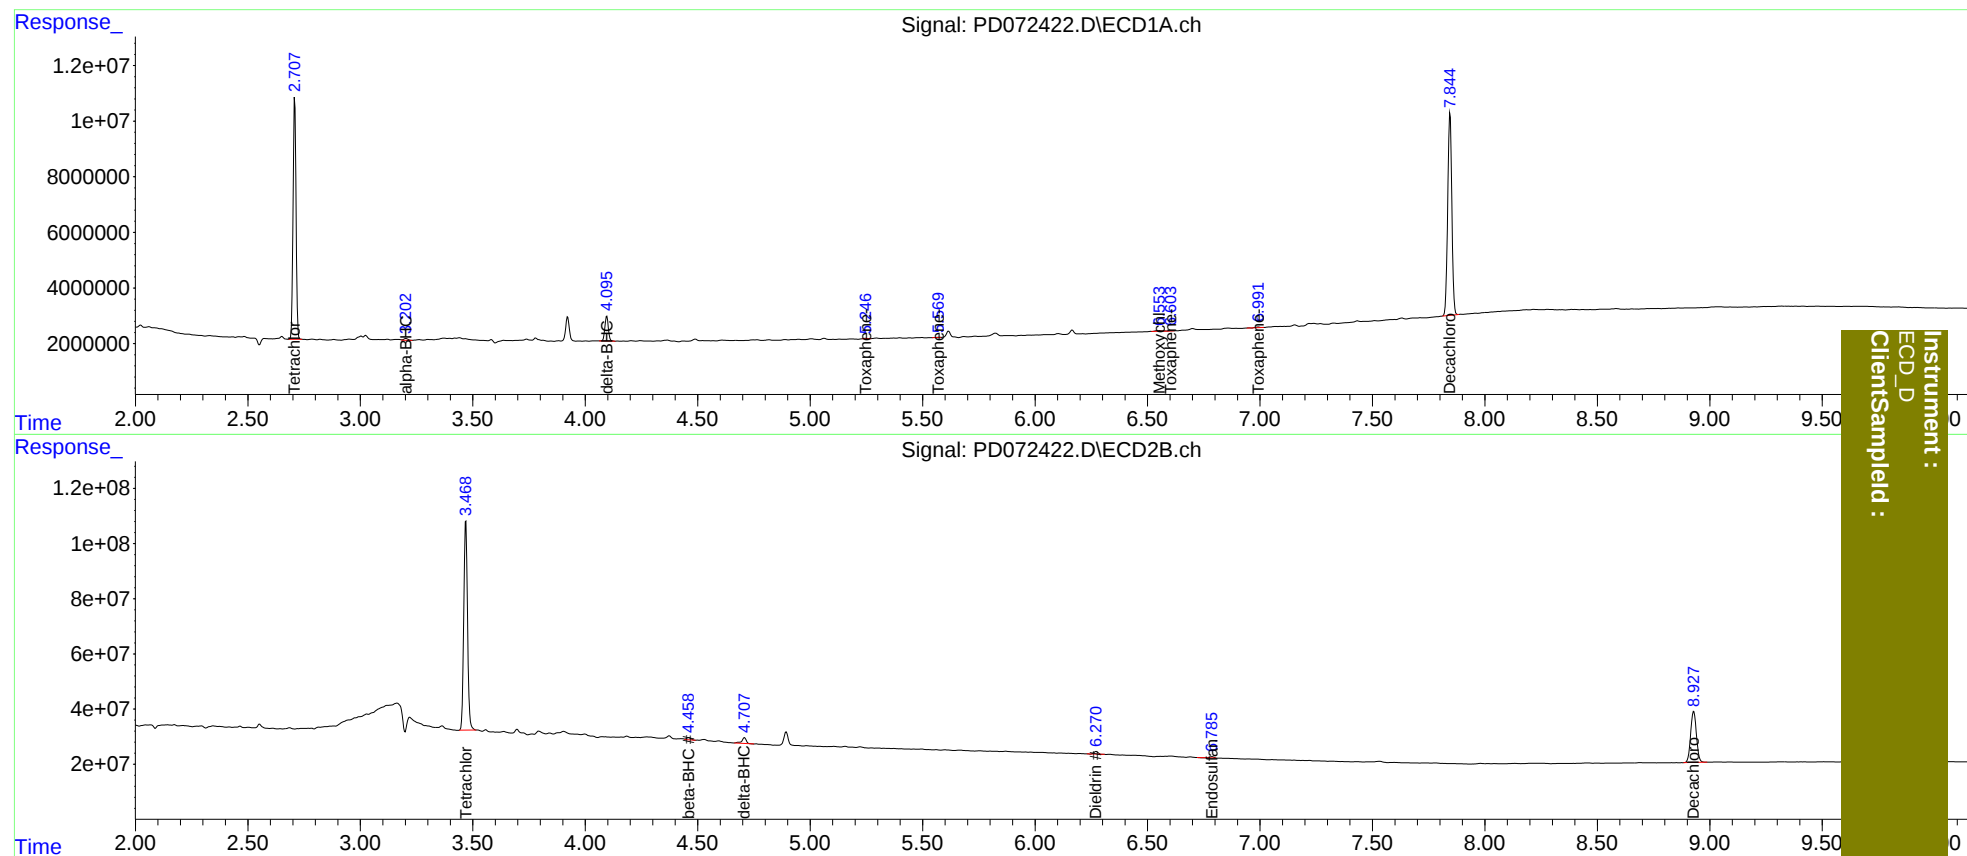


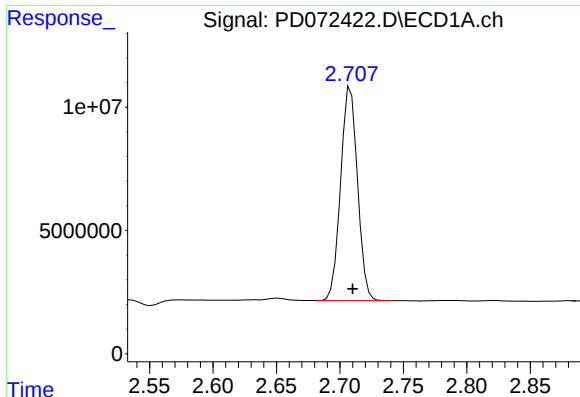

#1 Tetrachloro-m-xylene


R.T.: 2.709 min
Delta R.T.: -0.001 min
Response: 80319680
Conc: 32.91 ng/ml

Instrument :
ECD_D
ClientSampleId :

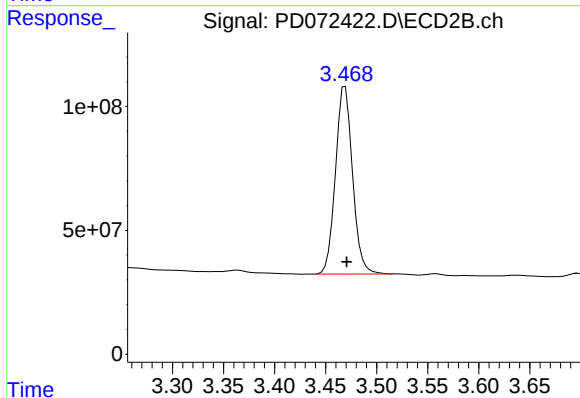


#1 Tetrachloro-m-xylene

R.T.: 3.469 min
Delta R.T.: -0.001 min
Response: 881838570
Conc: 36.88 ng/ml

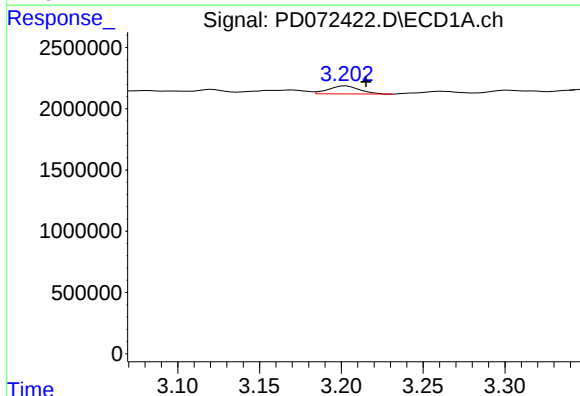


#2 alpha-BHC

R.T.: 3.203 min
Delta R.T.: -0.012 min
Response: 870381
Conc: 0.24 ng/ml

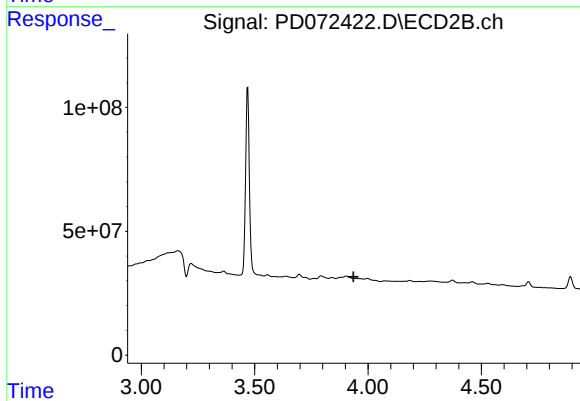

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 3.936 min
Response: 0
Conc: N.D.

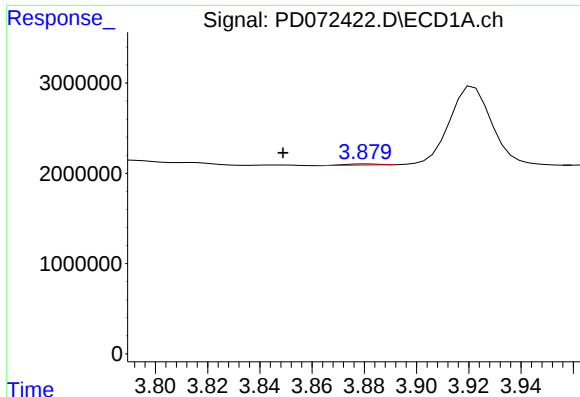

#6 beta-BHC


R.T.: 3.881 min
Delta R.T.: 0.032 min
Response: 103431
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

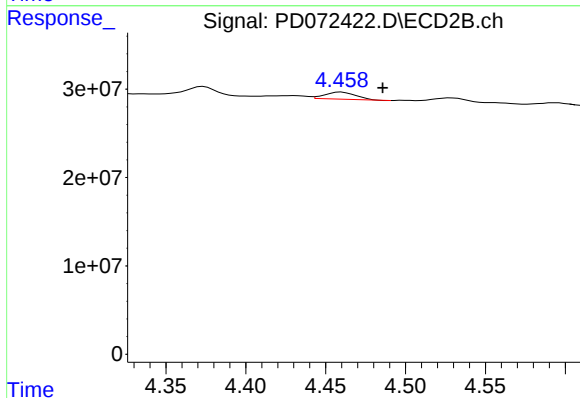


#6 beta-BHC

R.T.: 4.460 min
Delta R.T.: -0.026 min
Response: 10720732
Conc: 1.06 ng/ml

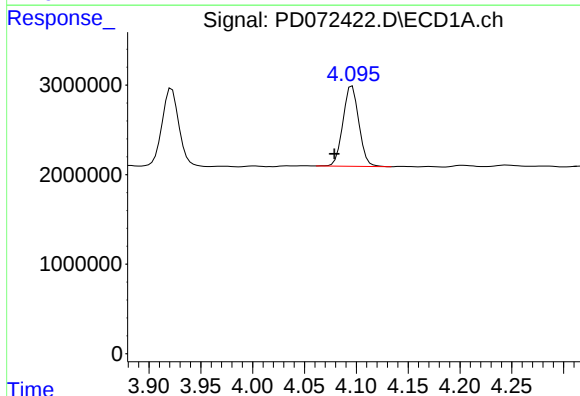


#7 delta-BHC

R.T.: 4.096 min
Delta R.T.: 0.017 min
Response: 9600363
Conc: 2.84 ng/ml

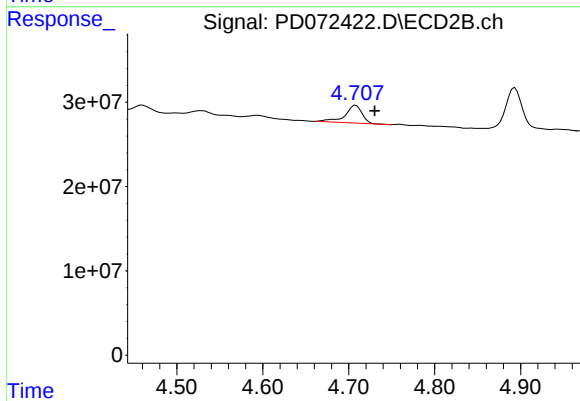

#7 delta-BHC


R.T.: 4.708 min
Delta R.T.: -0.022 min
Response: 29257086
Conc: 1.54 ng/ml

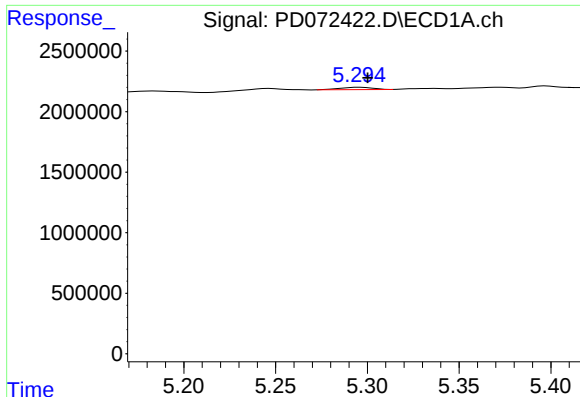

#13 Dieldrin


R.T.: 5.296 min
Delta R.T.: -0.004 min
Response: 249054
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

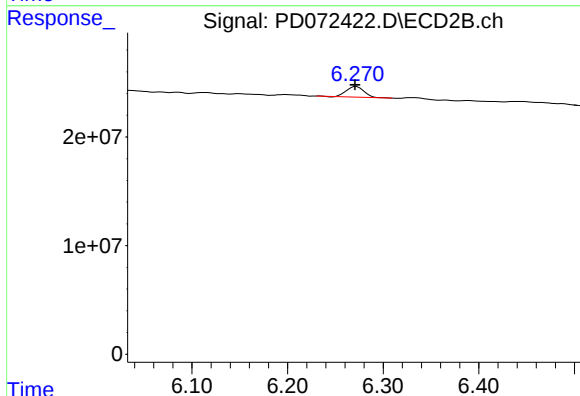


#13 Dieldrin

R.T.: 6.272 min
Delta R.T.: 0.001 min
Response: 12268068
Conc: 1.29 ng/ml

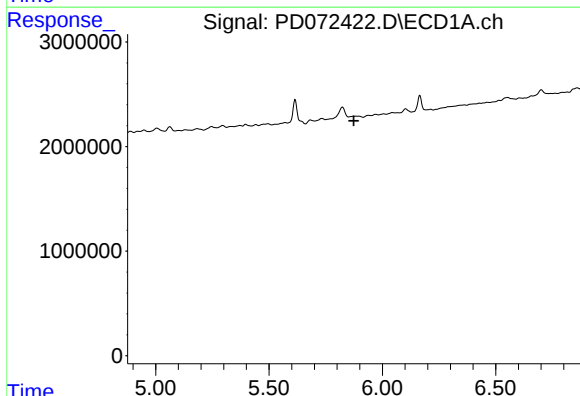


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.874 min
Response: 0
Conc: N.D.

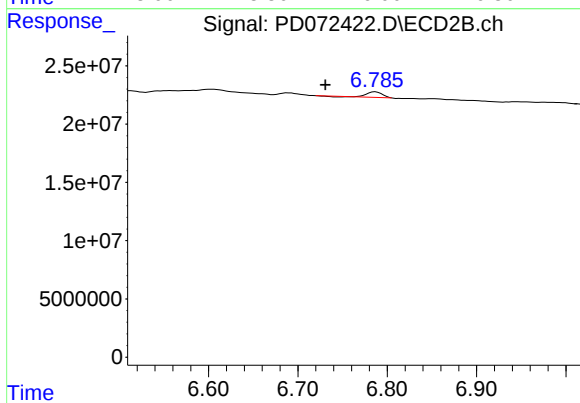

#15 Endosulfan II


R.T.: 6.787 min
Delta R.T.: 0.056 min
Response: 5197189
Conc: 0.72 ng/ml

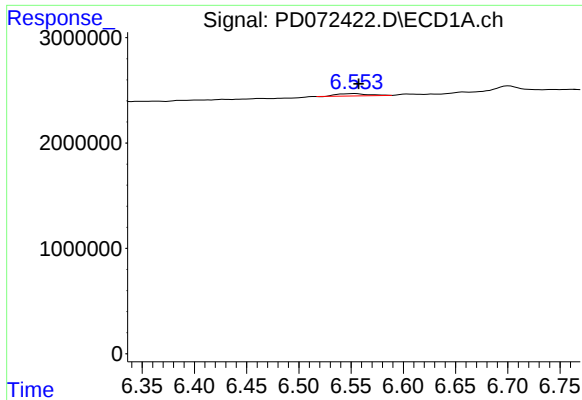

#20 Methoxychlor


R.T.: 6.554 min
Delta R.T.: -0.004 min
Response: 438073
Conc: 0.37 ng/ml

Instrument :
ECD_D
ClientSampleId :

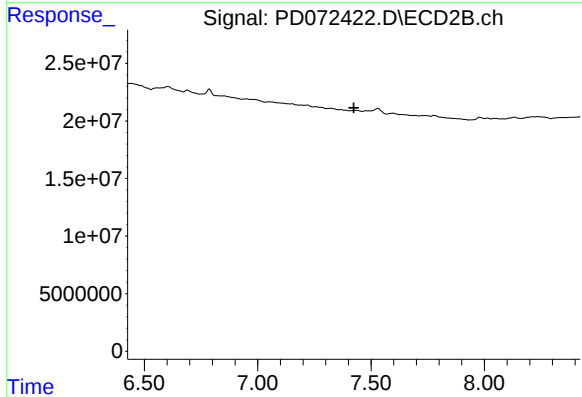


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.424 min
Response: 0
Conc: N.D.

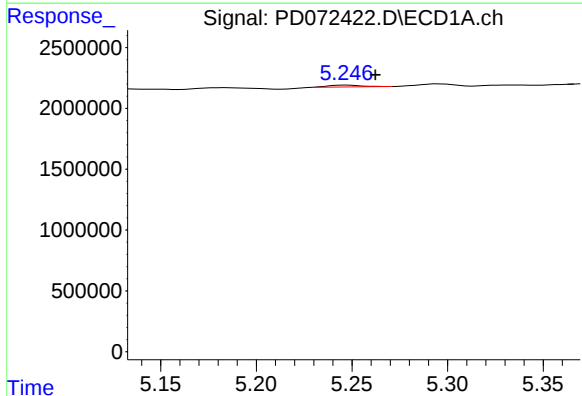


#22 Toxaphene-1

R.T.: 5.247 min
Delta R.T.: -0.015 min
Response: 188136
Conc: 15.93 ng/ml

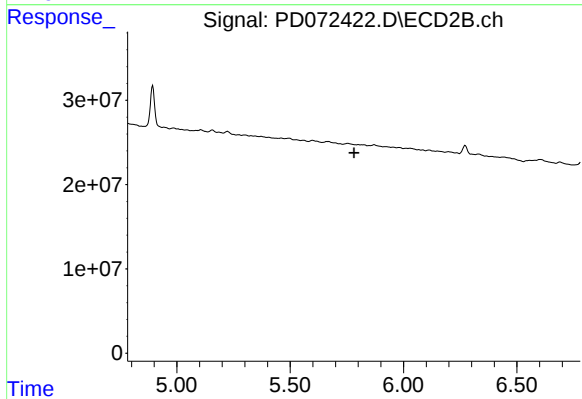

#22 Toxaphene-1


R.T.: 0.000 min
Exp R.T. : 5.782 min
Response: 0
Conc: N.D.

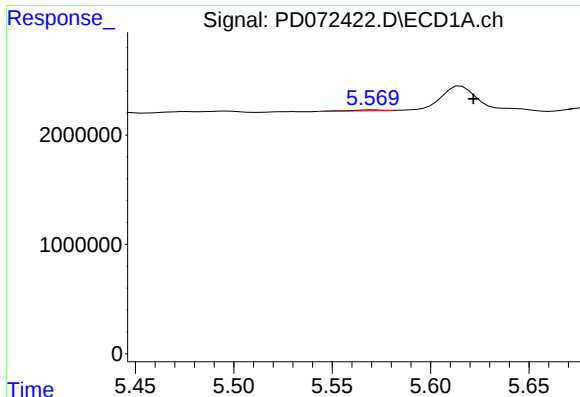

#23 Toxaphene-2


R.T.: 5.571 min
Delta R.T.: -0.051 min
Response: 93616
Conc: 7.47 ng/ml

Instrument :
ECD_D
ClientSampleId :

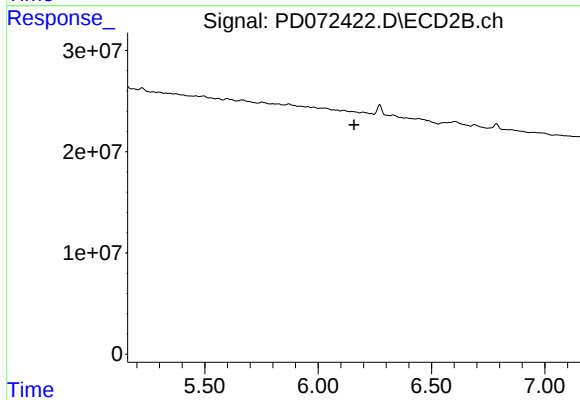


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T. : 6.159 min
Response: 0
Conc: N.D.

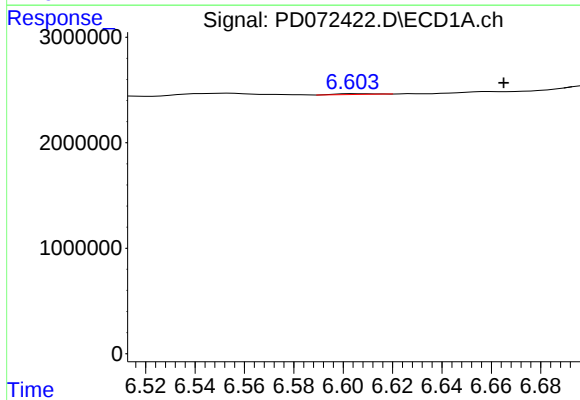


#25 Toxaphene-4

R.T.: 6.606 min
Delta R.T.: -0.060 min
Response: 76072
Conc: 1.08 ng/ml

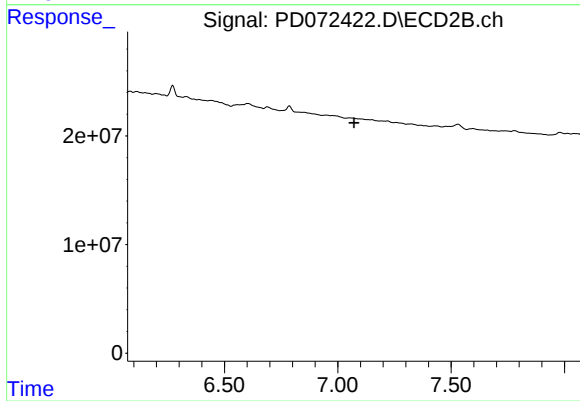

#25 Toxaphene-4


R.T.: 0.000 min
Exp R.T. : 7.072 min
Response: 0
Conc: N.D.

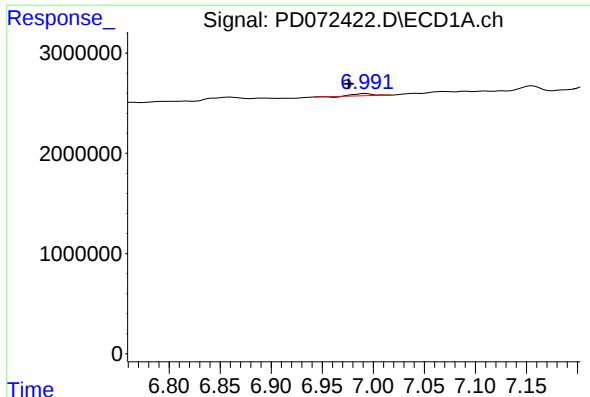

#26 Toxaphene-5


R.T.: 6.992 min
Delta R.T.: 0.016 min
Response: 245703
Conc: 6.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

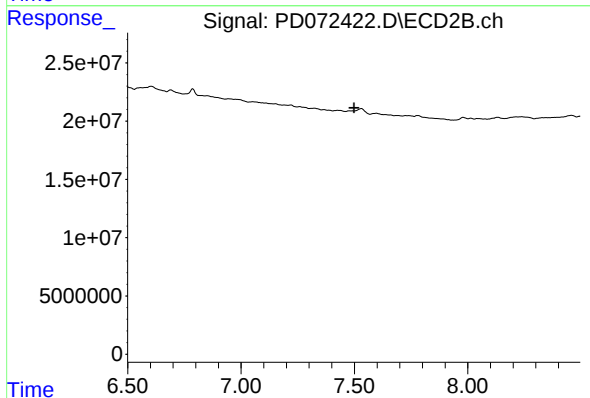


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T. : 7.499 min
Response: 0
Conc: N.D.

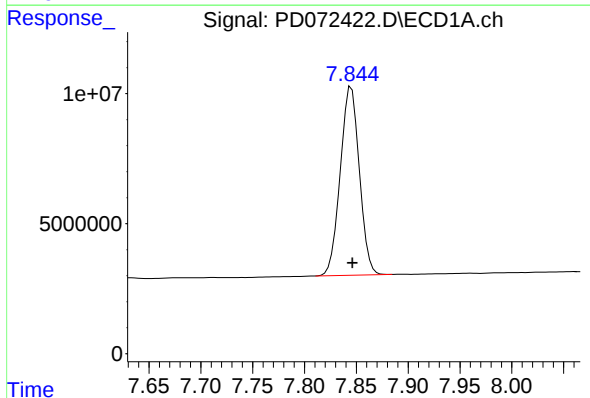

#27 Decachlorobiphenyl

R.T.: 7.845 min
Delta R.T.: 0.000 min
Response: 92951650
Conc: 47.58 ng/ml

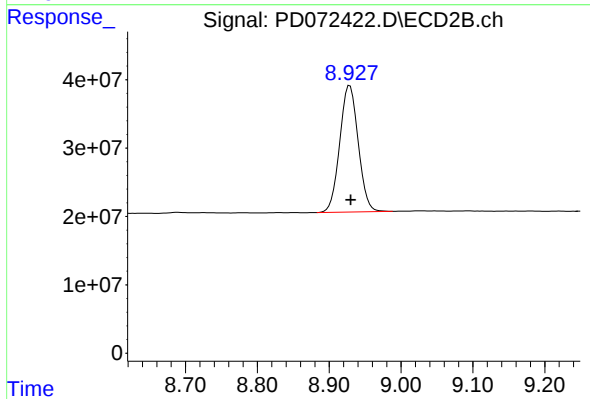

#27 Decachlorobiphenyl

R.T.: 8.929 min
Delta R.T.: -0.001 min
Response: 330303821
Conc: 65.39 ng/ml