

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101422\
 Data File : PD072424.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2022 14:27
 Operator : AR\AJ
 Sample : N5060-09MS
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C1BG8MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/17/2022
 Supervised By : Ankita Jodhani 10/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 00:22:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 06:06:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.708	3.469	39031737	481.5E6	15.991m	20.136m#
2)	SA Decachlor...	7.845	8.929	57476002	204.8E6	29.424	40.546 #
Target Compounds							
2)	A alpha-BHC	3.214	3.935	164.6E6	1475.8E6	46.108	48.759
3)	MA gamma-BHC...	3.545	4.269	152.4E6	1304.4E6	51.501	50.151
4)	MA Heptachlor	3.878	4.836	144.1E6	781.9E6	43.974	45.670
5)	MB Aldrin	4.157	5.175	152.8E6	670.8E6	46.465	46.417
6)	B beta-BHC	3.847	4.485	59591898	444.7E6	39.517	44.070
7)	B delta-BHC	4.078	4.729	114.7E6	626.0E6	33.998	33.008
8)	B Heptachlo...	4.663	5.607	137.9E6	589.5E6	46.438	52.242
9)	A Endosulfan I	5.031	5.991	120.6E6	523.4E6	46.444m	54.719m
10)	B trans-Chl...	4.911	5.861	136.2E6	569.3E6	44.832	51.422
11)	B cis-Chlor...	4.974	5.937	125.5E6	530.5E6	42.694m	50.254
12)	B 4,4'-DDE	5.164	6.110	269.4E6	1013.8E6	93.387	107.819
13)	MA Dieldrin	5.299	6.269	290.1E6	1481.0E6	101.102	155.349m#
14)	MA Endrin	5.575	6.501	244.3E6	939.0E6	97.955	117.035
15)	B Endosulfa...	5.874	6.731	241.2E6	851.7E6	102.911	117.915
16)	A 4,4'-DDD	5.721	6.635	211.9E6	874.3E6	94.403m	122.757 #
17)	MA 4,4'-DDT	5.972	6.943	212.5E6	850.1E6	98.518	126.095 #
18)	B Endrin al...	6.057	6.862	169.0E6	666.9E6	84.053	108.129 #
19)	B Endosulfa...	6.280	7.095	206.0E6	757.5E6	86.923	110.894 #
20)	A Methoxychlor	6.556	7.423	620.6E6	2072.2E6	527.273	645.570
21)	B Endrin ke...	6.791	7.585	269.9E6	981.0E6	96.951	133.563 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101422\
Data File : PD072424.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2022 14:27
Operator : AR\AJ
Sample : N5060-09MS
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 00:22:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 06:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

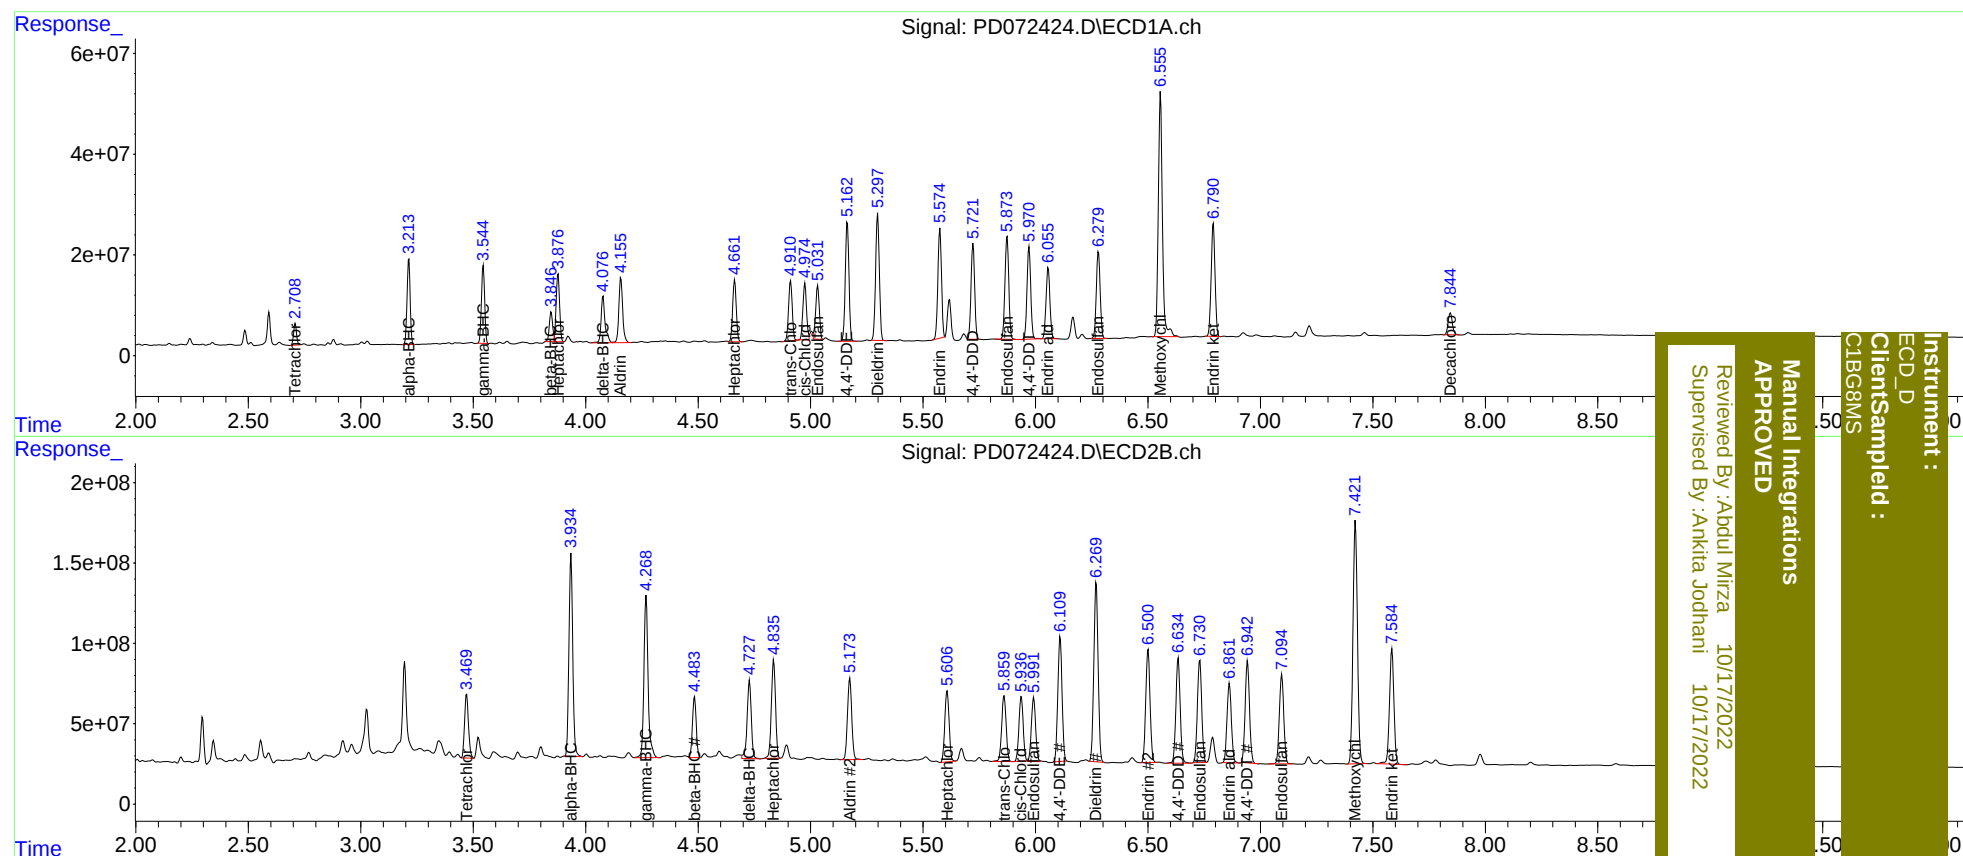

Reviewed By: Abdul Mirza 10/17/2022
Supervised By: Ankita Jodhani 10/17/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
C1BG8MS