

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101422\
 Data File : PD072419.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2022 13:20
 Operator : AR\AJ
 Sample : N4982-04MS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C1BB2MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/17/2022
 Supervised By : Ankita Jodhani 10/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 00:19:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 06:06:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.709	3.471	46237799	638.3E6	18.943	26.691 #
27)	SA Decachlor...	7.845	8.928	62197244	223.9E6	31.841	44.330 #
Target Compounds							
2)	A alpha-BHC	3.214	3.935	180.0E6	1686.3E6	50.437	55.712
3)	MA gamma-BHC...	3.545	4.269	170.4E6	1423.2E6	57.567	54.716
4)	MA Heptachlor	3.877	4.836	170.4E6	971.3E6	52.016	56.730
5)	MB Aldrin	4.157	5.175	167.2E6	816.0E6	50.845	56.466
6)	B beta-BHC	3.847	4.484	72160224	560.9E6	47.851	55.590
7)	B delta-BHC	4.077	4.728	54799439	404.9E6	16.238	21.351 #
8)	B Heptachlo...	4.662	5.607	152.9E6	683.3E6	51.508	60.552
9)	A Endosulfan I	5.032	5.990	139.1E6	596.1E6	53.546	62.320m
10)	B trans-Chl...	4.910	5.861	148.8E6	635.5E6	48.986m	57.402
11)	B cis-Chlor...	4.975	5.937	146.4E6	600.7E6	49.828	56.906
12)	B 4,4'-DDE	5.164	6.110	297.4E6	1139.6E6	103.079	121.197
13)	MA Dieldrin	5.299	6.269	312.9E6	1230.7E6	109.047	129.099
14)	MA Endrin	5.575	6.501	268.8E6	1003.3E6	107.802	125.049
15)	B Endosulfa...	5.873	6.730	254.0E6	965.2E6	108.376	133.635
16)	A 4,4'-DDD	5.722	6.634	242.5E6	921.0E6	108.020	129.319
17)	MA 4,4'-DDT	5.971	6.942	227.4E6	866.1E6	105.412	128.478
18)	B Endrin al...	6.056	6.862	197.5E6	769.8E6	98.197	124.813 #
19)	B Endosulfa...	6.280	7.095	195.1E6	726.0E6	82.337	106.282 #
20)	A Methoxychlor	6.555	7.422	591.3E6	2019.4E6	502.378	629.136 #
21)	B Endrin ke...	6.790	7.584	286.5E6	981.0E6	102.902	133.571 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101422\
Data File : PD072419.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2022 13:20
Operator : AR\AJ
Sample : N4982-04MS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 00:19:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 06:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

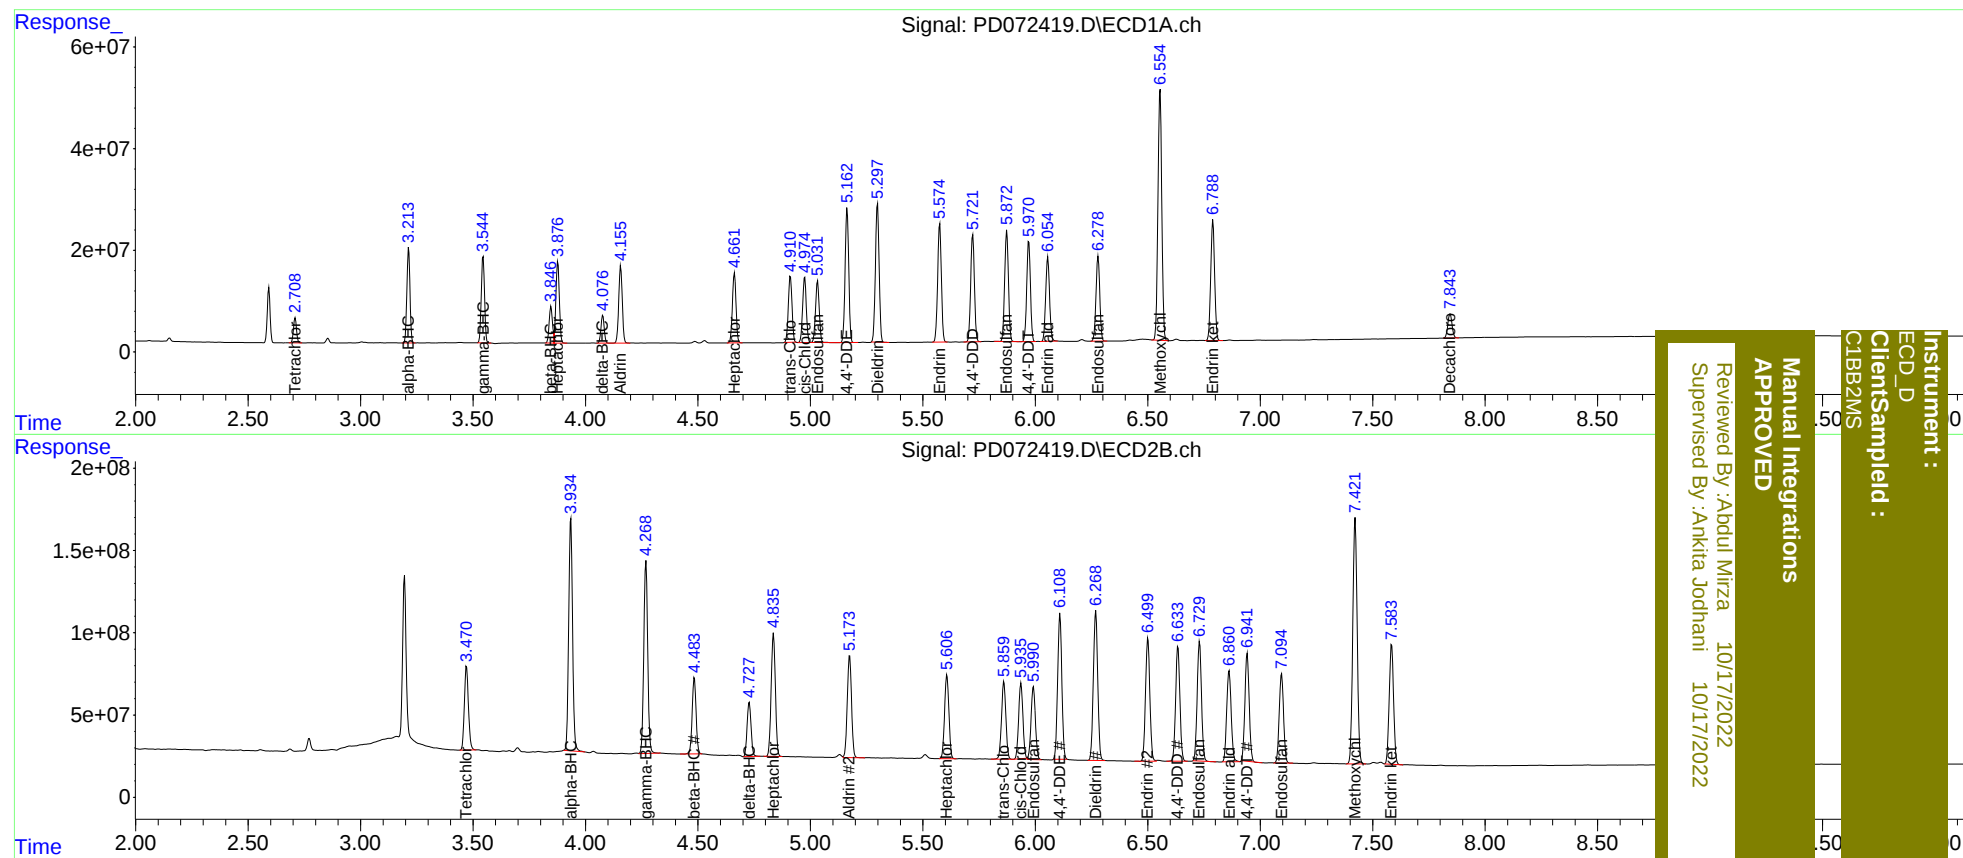

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/17/2022
Supervised By: Ankita Jodhani 10/17/2022

Instrument :
ECD_D
Client Sampled :
C1BB2MS