

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101422\
 Data File : PD072425.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2022 14:40
 Operator : AR\AJ
 Sample : N5060-10MSD
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C1BG8MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/21/2022
 Supervised By :Ankita Jodhani 10/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 00:23:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 06:06:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.707	3.469	38810559	483.4E6	15.900m	20.216m#
27)	SA Decachlor...	7.846	8.930	58458530	210.9E6	29.927	41.744 #
Target Compounds							
2)	A alpha-BHC	3.214	3.935	168.1E6	1499.7E6	47.086	49.548
3)	MA gamma-BHC...	3.545	4.269	154.4E6	1314.8E6	52.179	50.549
4)	MA Heptachlor	3.877	4.836	146.4E6	788.6E6	44.696	46.060
5)	MB Aldrin	4.157	5.175	155.4E6	679.7E6	47.244	47.034
6)	B beta-BHC	3.847	4.484	60609427	450.7E6	40.191	44.669
7)	B delta-BHC	4.077	4.728	117.1E6	635.6E6	34.689	33.515
8)	B Heptachlo...	4.663	5.608	139.8E6	600.2E6	47.086	53.192
9)	A Endosulfan I	5.031	5.991	124.2E6	530.5E6	47.830m	55.459m
10)	B trans-Chl...	4.910	5.861	141.1E6	576.4E6	46.436m	52.062
11)	B cis-Chlor...	4.974	5.937	131.5E6	538.8E6	44.736m	51.041
12)	B 4,4'-DDE	5.164	6.110	272.8E6	1033.6E6	94.556	109.921
13)	MA Dieldrin	5.298	6.269	294.8E6	1533.0E6	102.761	160.802m#
14)	MA Endrin	5.575	6.501	249.2E6	956.2E6	99.947	119.178
15)	B Endosulfa...	5.874	6.731	244.7E6	864.6E6	104.389	119.708
16)	A 4,4'-DDD	5.722	6.635	216.7E6	885.5E6	96.537m	124.336 #
17)	MA 4,4'-DDT	5.972	6.943	215.6E6	865.5E6	99.984	128.376 #
18)	B Endrin al...	6.057	6.863	171.9E6	678.4E6	85.470	109.991 #
19)	B Endosulfa...	6.281	7.096	208.7E6	768.5E6	88.056	112.506 #
20)	A Methoxychlor	6.556	7.423	629.9E6	2108.4E6	535.143	656.854
21)	B Endrin ke...	6.791	7.585	273.6E6	996.7E6	98.279	135.697 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101422\
Data File : PD072425.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2022 14:40
Operator : AR\AJ
Sample : N5060-10MSD
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 00:23:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 06:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

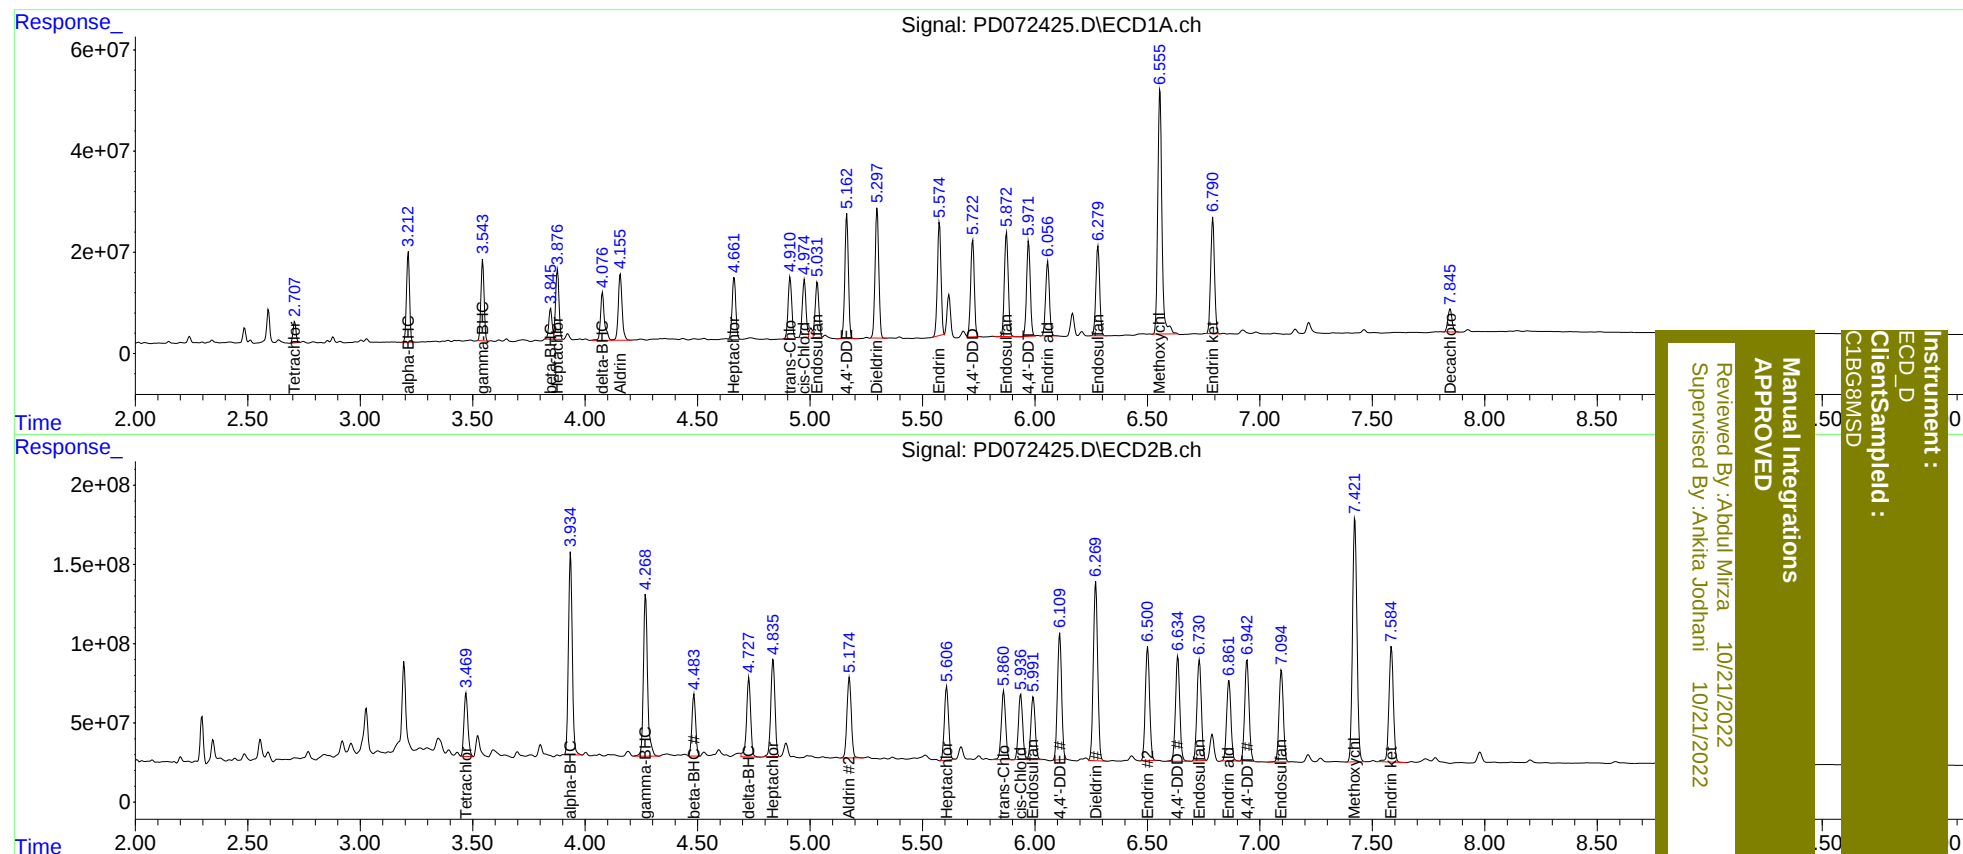

Reviewed By: Abdul Mirza 10/21/2022
Supervised By: Ankita Jodhani 10/21/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
C1BG8MSD