

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101424\
 Data File : PD086015.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2024 18:00
 Operator : AR\AJ
 Sample : PB164087BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK087

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 01:45:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 09 17:21:49 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.452	2.876	25488317	133.7E6	22.283	21.526
27)	SA Decachlor...	8.912	8.062	46039844	128.2E6	23.872	26.361
Target Compounds							
3)	MA gamma-BHC...	4.180f	3.738	16979855	1534972	8.515	0.178 #
4)	MA Heptachlor	4.841f	0.000	56179	0	<MDL	N.D. #
5)	MB Aldrin	5.170f	0.000	17125	0	<MDL	N.D. #
6)	B beta-BHC	0.000	3.978f	0	8592529	N.D.	1.905
7)	B delta-BHC	4.672f	0.000	1407513	0	0.640	N.D. #
8)	B Heptachlo...	5.503f	0.000	94872	0	<MDL	N.D. #
9)	A Endosulfan I	0.000	5.288f	0	94523	N.D.	<MDL
10)	B trans-Chl...	5.832	0.000	37648	0	<MDL	N.D. #
11)	B cis-Chlor...	5.832f	0.000	37648	0	<MDL	N.D. #
12)	B 4,4'-DDE	0.000	5.414f	0	455389	N.D.	<MDL
13)	MA Dieldrin	0.000	5.479	0	218256	N.D.	<MDL
14)	MA Endrin	6.478	0.000	86286	0	<MDL	N.D. #
15)	B Endosulfa...	0.000	6.113f	0	82854	N.D.	<MDL
17)	MA 4,4'-DDT	6.921	6.189	465210	-58225	0.345	N.D. #
18)	B Endrin al...	0.000	6.254	0	250515	N.D.	<MDL
19)	B Endosulfa...	0.000	6.408f	0	50769	N.D.	<MDL
20)	A Methoxychlor	7.354	6.692f	281703	135617	0.352	<MDL #
21)	B Endrin ke...	0.000	6.939f	0	277476	N.D.	<MDL
23)	Toxaphene-2	6.314	0.000	75233	0	4.364	N.D. #
24)	Toxaphene-3	6.921	6.692f	465210	135617	10.435	1.143 #
26)	Toxaphene-5	0.000	7.283	0	149724	N.D.	2.712


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101424\
Data File : PD086015.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2024 18:00
Operator : AR\AJ
Sample : PB164087BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 01:45:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 09 17:21:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

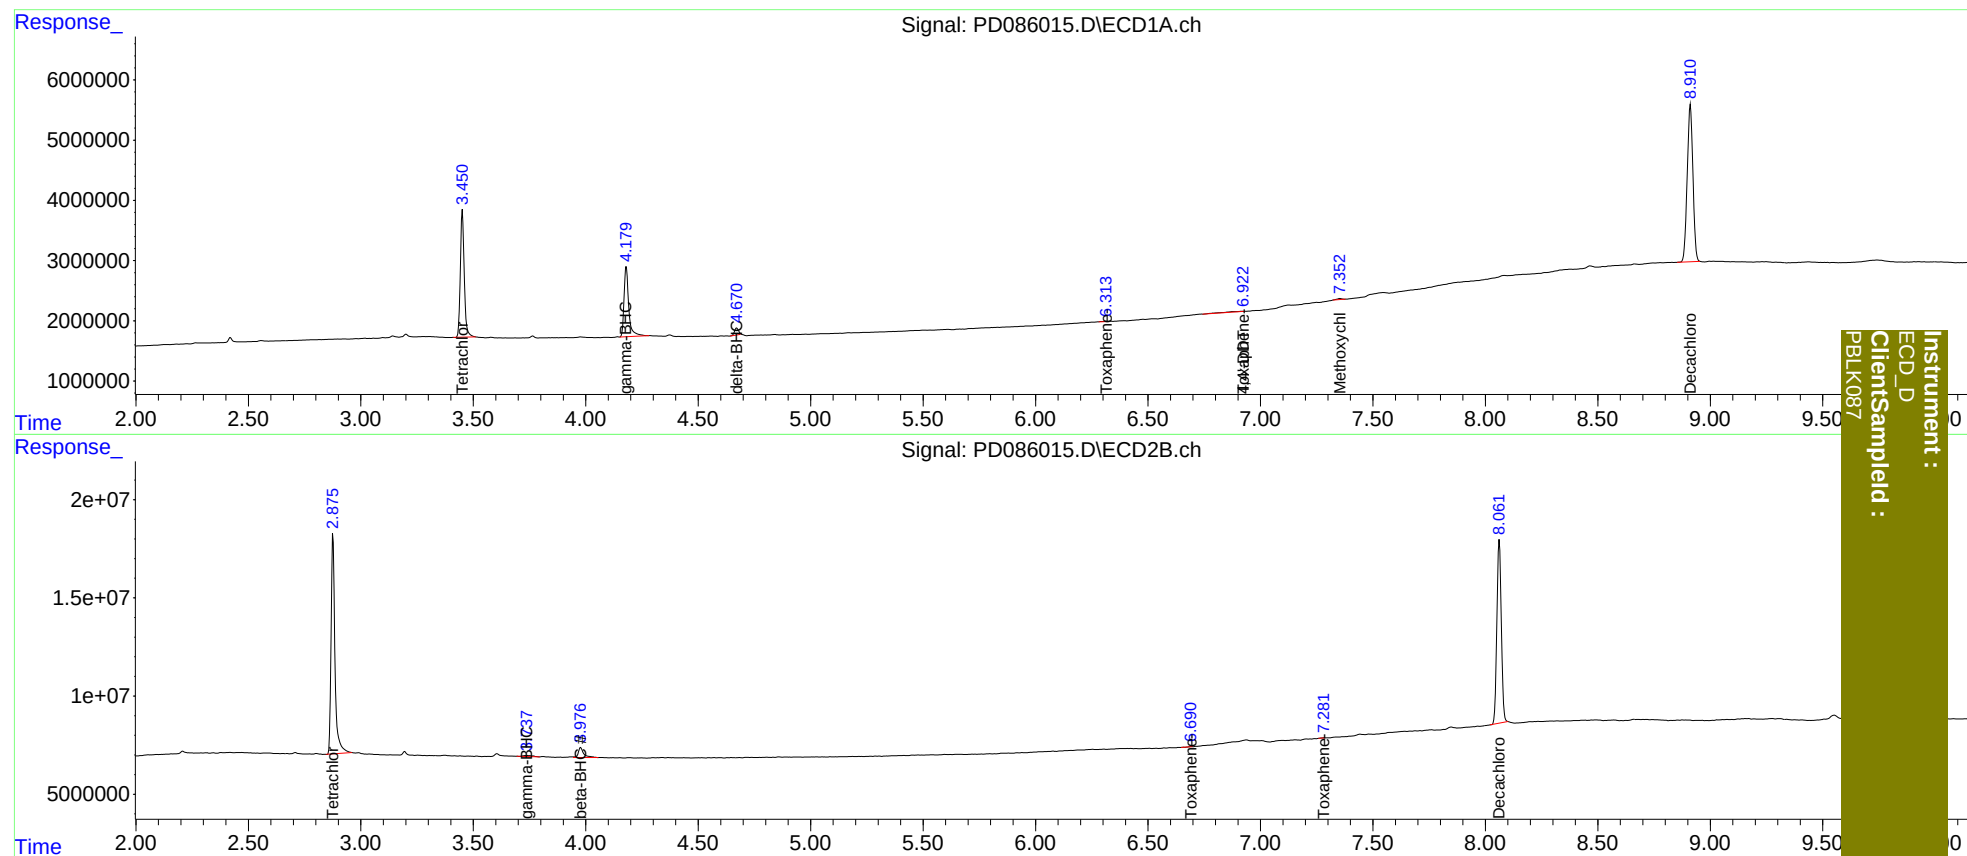


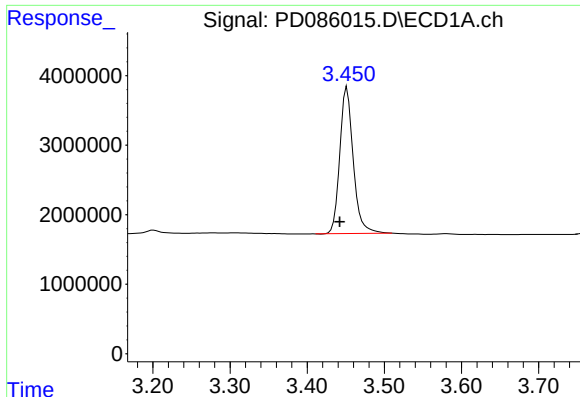

#1 Tetrachloro-m-xylene


R.T.: 3.452 min
Delta R.T.: 0.010 min
Response: 25488317
Conc: 22.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK087

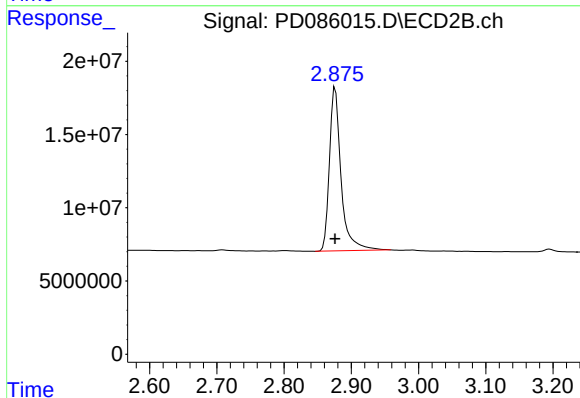


#1 Tetrachloro-m-xylene

R.T.: 2.876 min
Delta R.T.: 0.000 min
Response: 133679491
Conc: 21.53 ng/ml

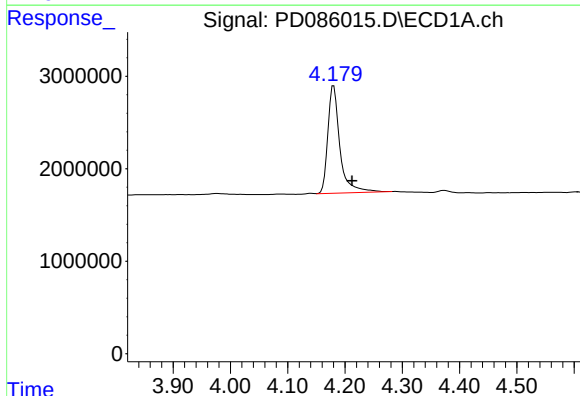


#3 gamma-BHC (Lindane)

R.T.: 4.180 min
Delta R.T.: -0.032 min
Response: 16979855
Conc: 8.51 ng/ml

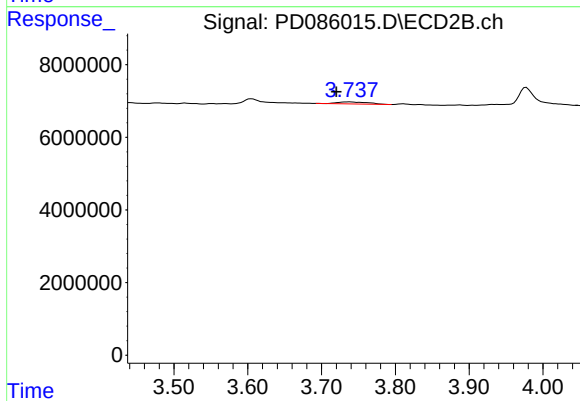

#3 gamma-BHC (Lindane)


R.T.: 3.738 min
Delta R.T.: 0.018 min
Response: 1534972
Conc: 0.18 ng/ml

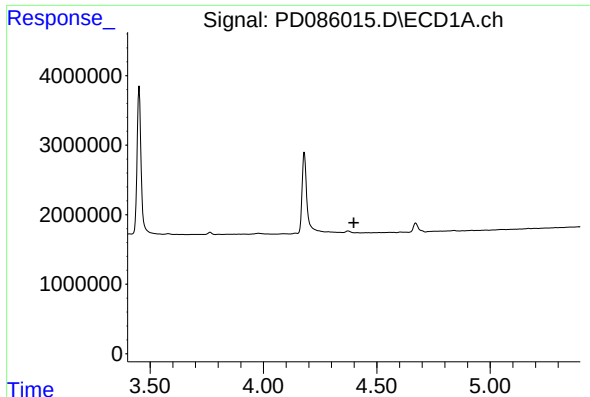

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.399 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PBLK087

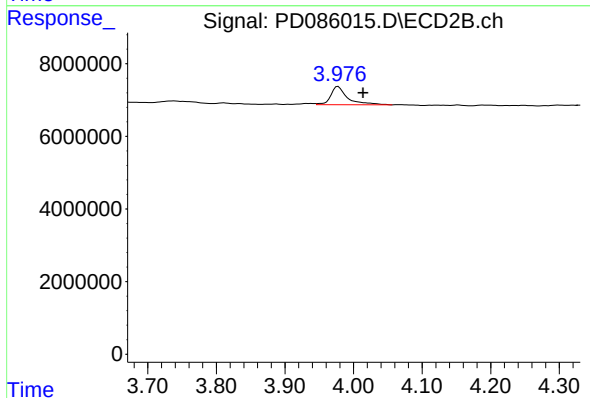


#6 beta-BHC

R.T.: 3.978 min
Delta R.T.: -0.037 min
Response: 8592529
Conc: 1.91 ng/ml

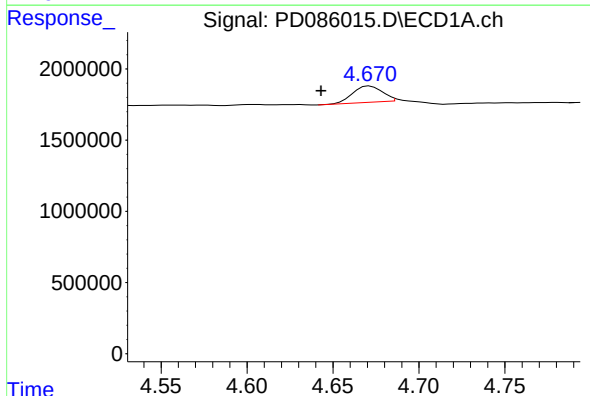


#7 delta-BHC

R.T.: 4.672 min
Delta R.T.: 0.028 min
Response: 1407513
Conc: 0.64 ng/ml

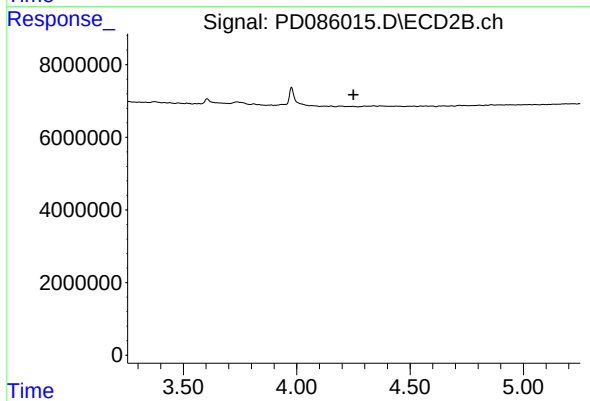

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.251 min
Response: 0
Conc: N.D.

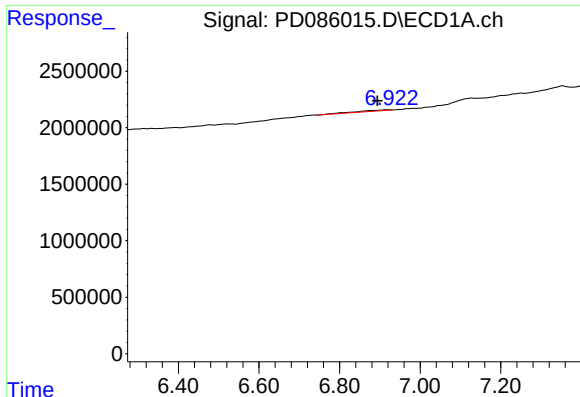

#17 4,4'-DDT


R.T.: 6.921 min
Delta R.T.: 0.027 min
Response: 465210
Conc: 0.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK087

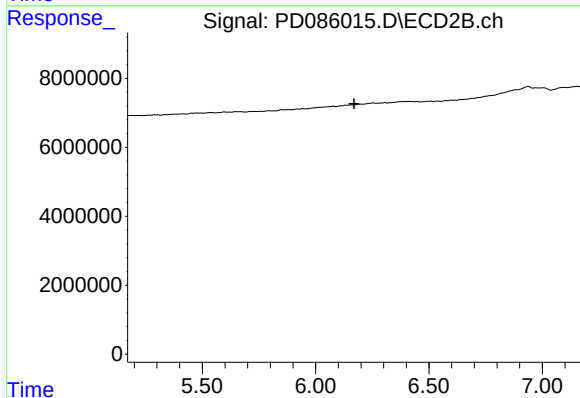


#17 4,4'-DDT

R.T.: 6.189 min
Delta R.T.: 0.019 min
Response: -58225
Conc: N.D.

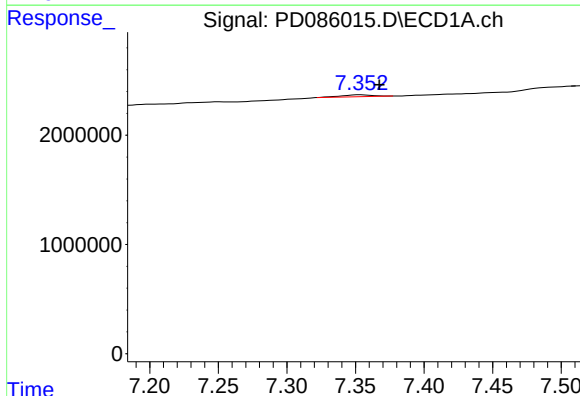


#20 Methoxychlor

R.T.: 7.354 min
Delta R.T.: -0.014 min
Response: 281703
Conc: 0.35 ng/ml

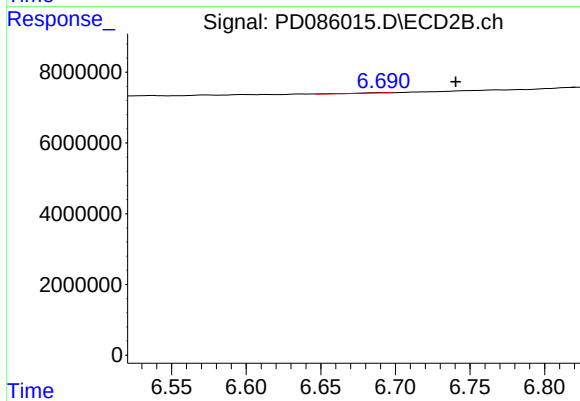

#20 Methoxychlor


R.T.: 6.692 min
Delta R.T.: -0.049 min
Response: 135617
Conc: N.D.

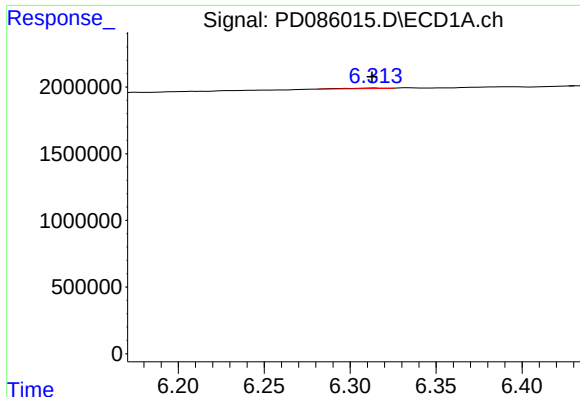

#23 Toxaphene-2


R.T.: 6.314 min
Delta R.T.: 0.002 min
Response: 75233
Conc: 4.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK087

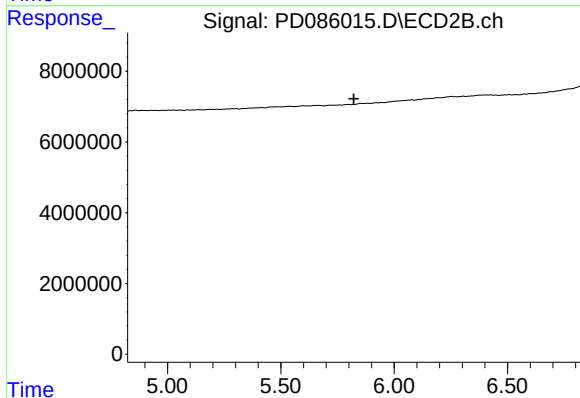


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T. : 5.822 min
Response: 0
Conc: N.D.

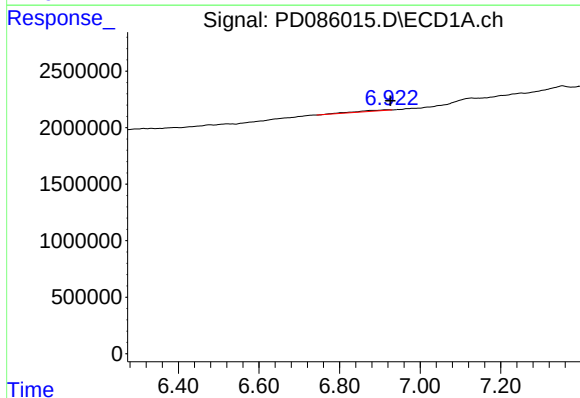


#24 Toxaphene-3

R.T.: 6.921 min
Delta R.T.: -0.005 min
Response: 465210
Conc: 10.43 ng/ml

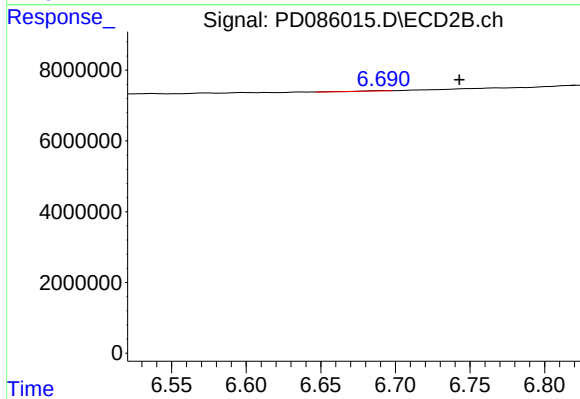

#24 Toxaphene-3


R.T.: 6.692 min
Delta R.T.: -0.051 min
Response: 135617
Conc: 1.14 ng/ml

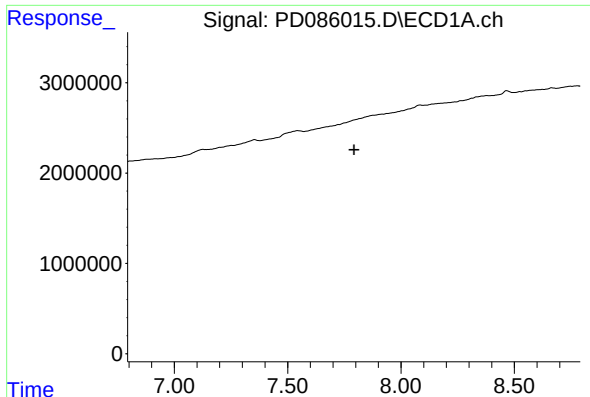

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T.: 7.793 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PBLK087

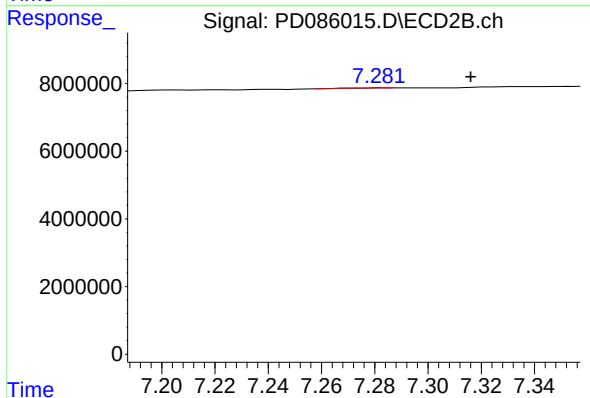


#26 Toxaphene-5

R.T.: 7.283 min
Delta R.T.: -0.033 min
Response: 149724
Conc: 2.71 ng/ml

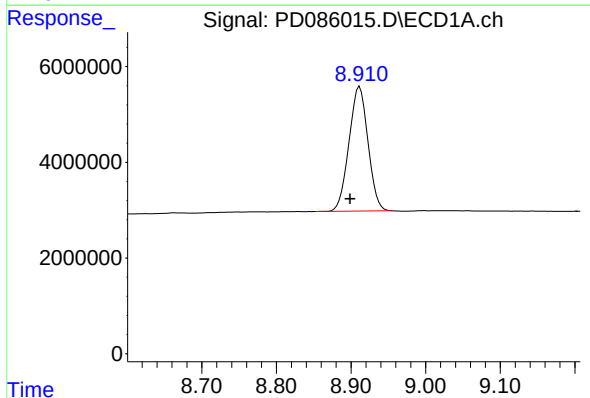

#27 Decachlorobiphenyl

R.T.: 8.912 min
Delta R.T.: 0.013 min
Response: 46039844
Conc: 23.87 ng/ml

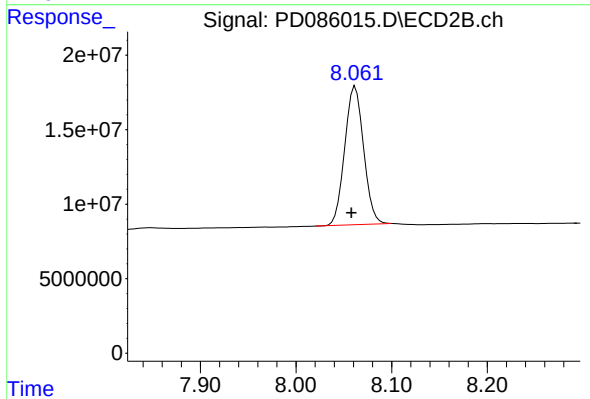

#27 Decachlorobiphenyl

R.T.: 8.062 min
Delta R.T.: 0.004 min
Response: 128202337
Conc: 26.36 ng/ml