

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101424\
 Data File : PD086010.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2024 15:44
 Operator : AR\AJ
 Sample : P4350-13MS
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EOAK1MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/15/2024
 Supervised By :Ankita Jodhani 10/15/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 01:43:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 09 17:21:49 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	2.877	19101643	102.5E6	16.699m	16.498
27)	SA Decachlor...	8.901	8.060	26366546	73036783	13.671	15.018
Target Compounds							
2)	A alpha-BHC	3.884	3.386	111.1E6	432.2E6	55.412m	46.840
3)	MA gamma-BHC...	4.214	3.721	108.5E6	409.7E6	54.423	47.545
4)	MA Heptachlor	4.807	4.072	107.3E6	367.7E6	55.632	50.003
5)	MB Aldrin	5.145	4.358	108.1E6	392.2E6	44.909	40.558
6)	B beta-BHC	4.400	4.015	43426277	176.2E6	41.218	39.078
7)	B delta-BHC	4.645	4.252	94468060	391.3E6	42.941	42.233
8)	B Heptachlo...	5.565	4.861	94852178	346.3E6	42.587	39.749
9)	A Endosulfan I	5.946	5.235	93609963	327.4E6	51.311	47.230
10)	B trans-Chl...	5.820	5.113	97985147	364.0E6	43.598	40.457
11)	B cis-Chlor...	5.900	5.177	100.2E6	360.7E6	43.925	40.175
12)	B 4,4'-DDE	6.072	5.362	189.3E6	665.0E6	99.284	88.467
13)	MA Dieldrin	6.219	5.501	210.7E6	687.9E6	107.024	92.932
14)	MA Endrin	6.444	5.778	176.1E6	589.4E6	114.006	99.944
15)	B Endosulfa...	6.657	6.070	170.1E6	569.7E6	85.675	81.472
16)	A 4,4'-DDD	6.580	5.917	150.1E6	518.3E6	120.367	108.637
17)	MA 4,4'-DDT	6.895	6.171	147.1E6	502.0E6	108.990	100.791
18)	B Endrin al...	6.786	6.248	127.0E6	409.1E6	82.847	78.980
19)	B Endosulfa...	7.020	6.472	167.2E6	519.1E6	91.300	85.702
20)	A Methoxychlor	7.369	6.742	415.1E6	1017.3E6	519.152	485.269
21)	B Endrin ke...	7.497	6.982	180.5E6	587.6E6	88.796m	80.681

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101424\
Data File : PD086010.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2024 15:44
Operator : AR\AJ
Sample : P4350-13MS
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 01:43:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 09 17:21:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

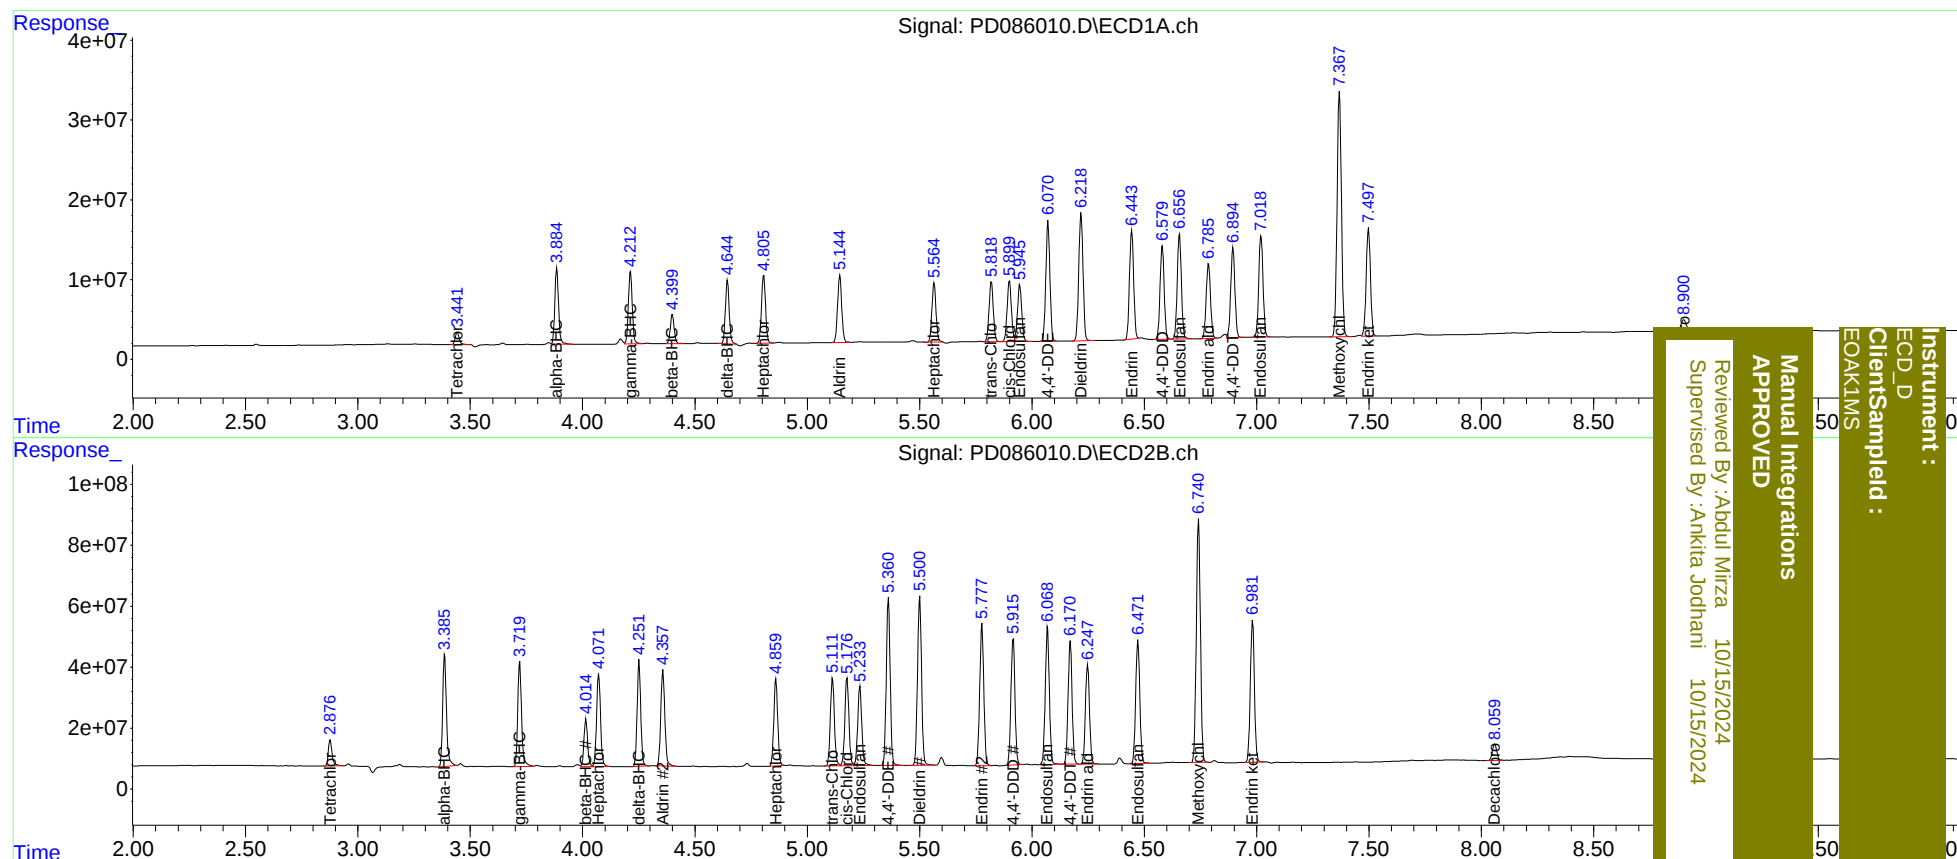

Instrument :
ECD_D
ClientSampled :
EOAKIMS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 10/15/2024
Supervised By: Ankita Jodhani 10/15/2024