

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101424\
 Data File : PD086006.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2024 14:50
 Operator : AR\AJ
 Sample : P4350-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EOAJ9

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/16/2024
 Supervised By : Ankita Jodhani 10/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 01:42:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 09 17:21:49 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.441	2.877	9274376	43207001	8.108m	6.958
2) SA Decachlor...	8.912	8.057	52322993	40430131	27.130m	8.313m#
Target Compounds						
9) A Endosulfan I	5.970	5.256	13471685	38640991	7.384	5.575m
10) B trans-Chl...	5.818	5.109	1285521	6770984	0.572m	0.753m#
12) B 4,4'-DDE	6.075	5.360	6004408	10673106	3.149m	1.420m#
13) MA Dieldrin	6.222	5.499	2706493	75969341	1.375m	10.263m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101424\
Data File : PD086006.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2024 14:50
Operator : AR\AJ
Sample : P4350-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 01:42:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 09 17:21:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

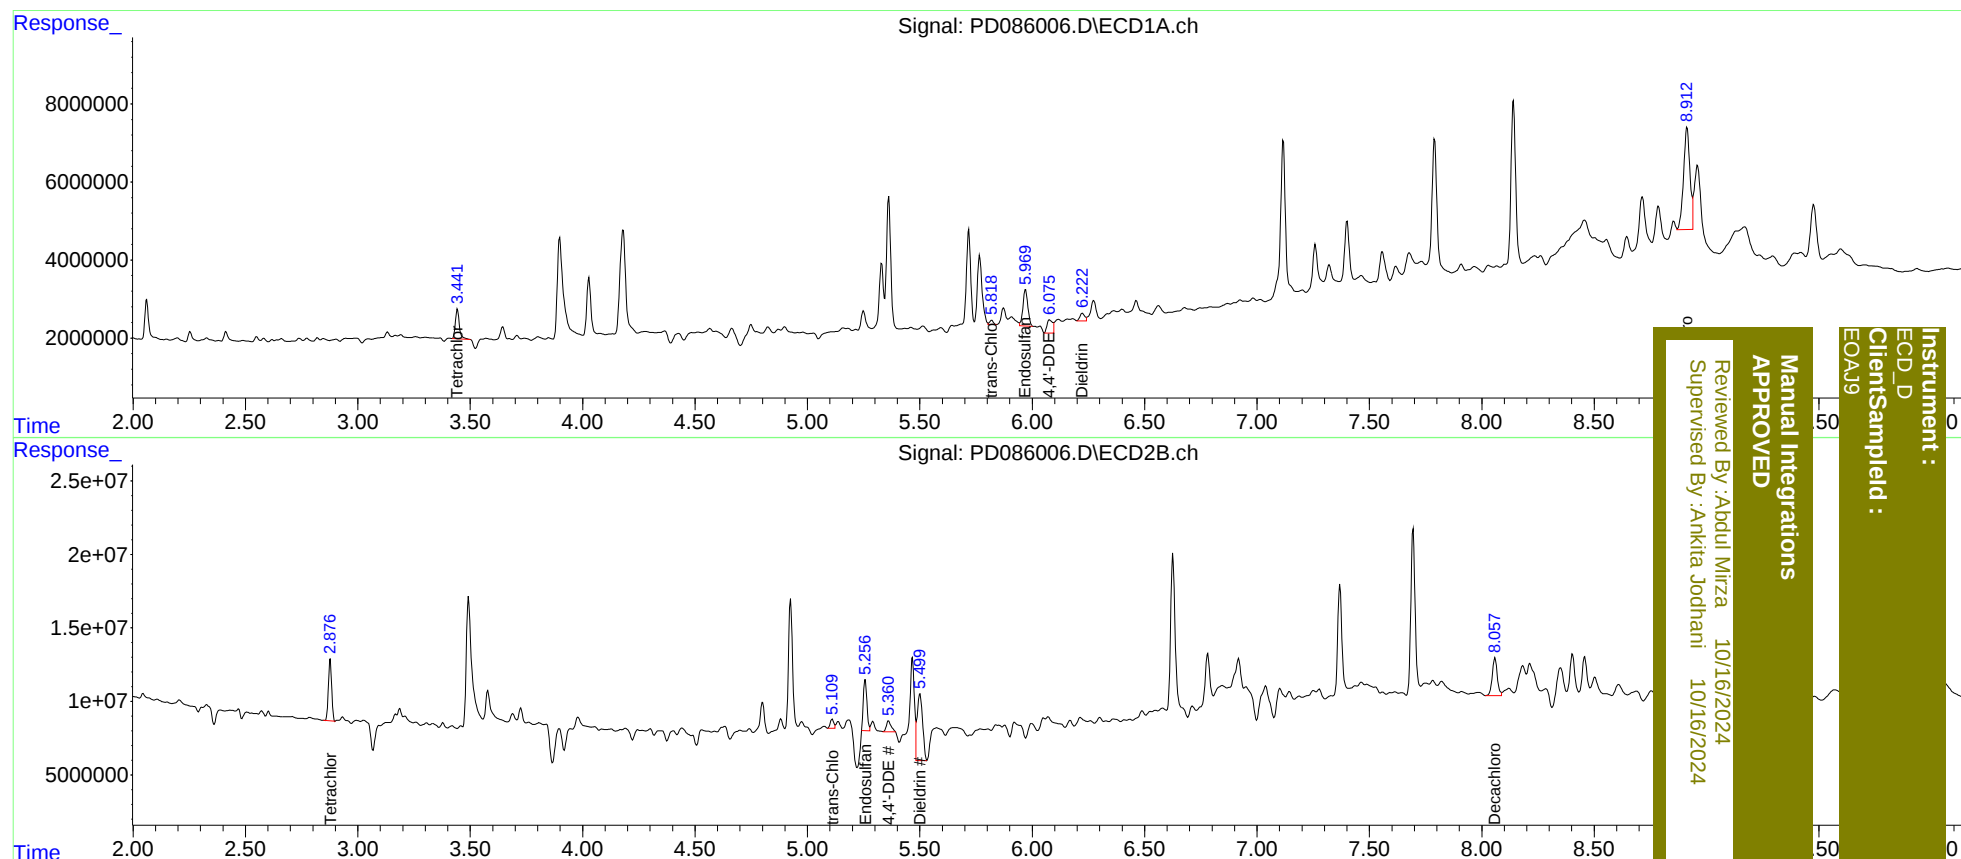

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/16/2024
Supervised By: Ankita Jodhani 10/16/2024

Instrument :
ECD_D
ClientSampled :
EOA39