

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101424\
 Data File : PD086011.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2024 15:58
 Operator : AR\AJ
 Sample : P4350-14MSD
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EOAK1MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/15/2024
 Supervised By :Ankita Jodhani 10/15/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 01:44:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 09 17:21:49 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	2.877	19164595	103.4E6	16.754m	16.655
27)	SA Decachlor...	8.901	8.061	25559278	63827174	13.253	13.124
Target Compounds							
2)	A alpha-BHC	3.885	3.387	112.6E6	434.5E6	56.167m	47.086
3)	MA gamma-BHC...	4.214	3.721	109.7E6	411.6E6	55.000	47.770
4)	MA Heptachlor	4.807	4.072	107.9E6	370.0E6	55.982	50.317
5)	MB Aldrin	5.146	4.358	108.6E6	394.3E6	45.128	40.772
6)	B beta-BHC	4.400	4.016	43717166	175.9E6	41.494	38.992
7)	B delta-BHC	4.646	4.252	94454122	395.0E6	42.934	42.634
8)	B Heptachlo...	5.566	4.860	95363371	348.1E6	42.817	39.956
9)	A Endosulfan I	5.946	5.235	95352632	323.6E6	52.266	46.685
10)	B trans-Chl...	5.819	5.113	98687840	356.3E6	43.910	39.611
11)	B cis-Chlor...	5.900	5.177	101.2E6	353.4E6	44.361	39.368
12)	B 4,4'-DDE	6.072	5.362	189.9E6	662.7E6	99.592	88.168
13)	MA Dieldrin	6.218	5.501	211.8E6	688.2E6	107.593	92.972
14)	MA Endrin	6.445	5.778	178.4E6	599.5E6	115.474	101.654
15)	B Endosulfa...	6.658	6.070	172.0E6	574.1E6	86.641	82.105
16)	A 4,4'-DDD	6.580	5.917	153.1E6	525.9E6	122.693	110.225
17)	MA 4,4'-DDT	6.895	6.171	148.9E6	508.3E6	110.318	102.048
18)	B Endrin al...	6.786	6.248	128.8E6	415.1E6	83.977	80.125
19)	B Endosulfa...	7.021	6.473	169.6E6	521.6E6	92.599	86.108
20)	A Methoxychlor	7.369	6.743	419.3E6	1037.7E6	524.356	494.975
21)	B Endrin ke...	7.497	6.982	183.8E6	592.2E6	90.384m	81.309

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101424\
Data File : PD086011.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2024 15:58
Operator : AR\AJ
Sample : P4350-14MSD
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 01:44:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 09 17:21:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

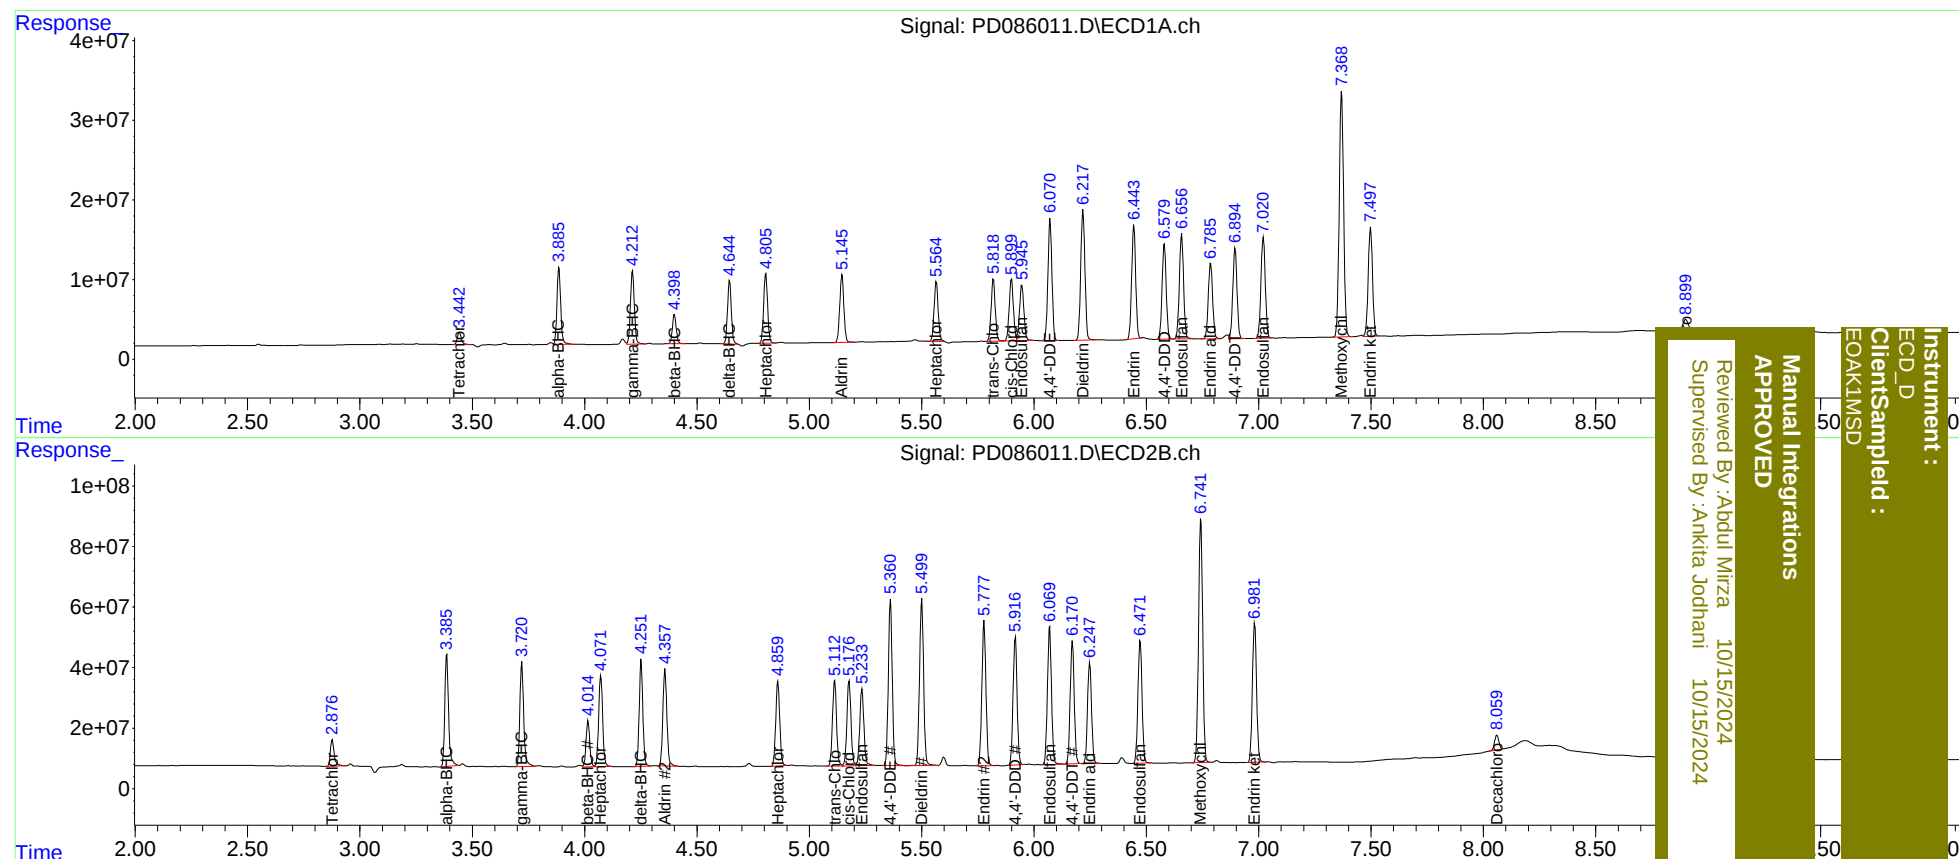

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 10/15/2024
Supervised By: Ankita Jodhani 10/15/2024

Instrument :
ECD_D
Client Sampled :
EOAK1MSD