

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101424\
 Data File : PD086034.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2024 22:15
 Operator : AR\AJ
 Sample : P4349-22MSD
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EOAG2MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/15/2024
 Supervised By :Ankita Jodhani 10/15/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 01:50:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 09 17:21:49 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	2.878	25008426	126.1E6	21.863	20.301
27)	SA Decachlor...	8.900	8.059	40520608	116.8E6	21.010	24.016
Target Compounds							
2)	A alpha-BHC	3.886	3.387	125.6E6	483.0E6	62.633	52.345
3)	MA gamma-BHC...	4.214	3.721	122.8E6	451.7E6	61.578	52.413
4)	MA Heptachlor	4.806	4.073	120.6E6	418.7E6	62.533	56.943
5)	MB Aldrin	5.146	4.358	124.8E6	436.0E6	51.866	45.081
6)	B beta-BHC	4.400	4.015	47645932	191.3E6	45.223	42.421
7)	B delta-BHC	4.644	4.252	121.8E6	434.7E6	55.381m	46.920
8)	B Heptachlo...	5.564	4.861	110.2E6	382.0E6	49.467	43.844
9)	A Endosulfan I	5.947	5.234	106.8E6	368.7E6	58.532	53.191
10)	B trans-Chl...	5.819	5.113	111.6E6	406.0E6	49.666	45.127
11)	B cis-Chlor...	5.900	5.177	113.5E6	401.6E6	49.750	44.731
12)	B 4,4'-DDE	6.072	5.361	212.5E6	731.9E6	111.415	97.369
13)	MA Dieldrin	6.218	5.499	240.7E6	779.1E6	122.282	105.246m
14)	MA Endrin	6.444	5.777	200.7E6	674.5E6	129.895	114.361
15)	B Endosulfa...	6.657	6.069	200.7E6	651.5E6	101.119	93.169
16)	A 4,4'-DDD	6.580	5.916	170.6E6	606.7E6	136.793	127.158
17)	MA 4,4'-DDT	6.895	6.170	166.3E6	582.2E6	123.268	116.893
18)	B Endrin al...	6.786	6.247	151.2E6	484.8E6	98.599	93.592
19)	B Endosulfa...	7.021	6.471	193.3E6	593.8E6	105.576	98.025
20)	A Methoxychlor	7.369	6.742	464.2E6	1213.0E6	580.547	578.607
21)	B Endrin ke...	7.497	6.982	212.5E6	695.4E6	104.527	95.477

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101424\
Data File : PD086034.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2024 22:15
Operator : AR\AJ
Sample : P4349-22MSD
Misc :
ALS Vial : 38 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 01:50:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 09 17:21:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

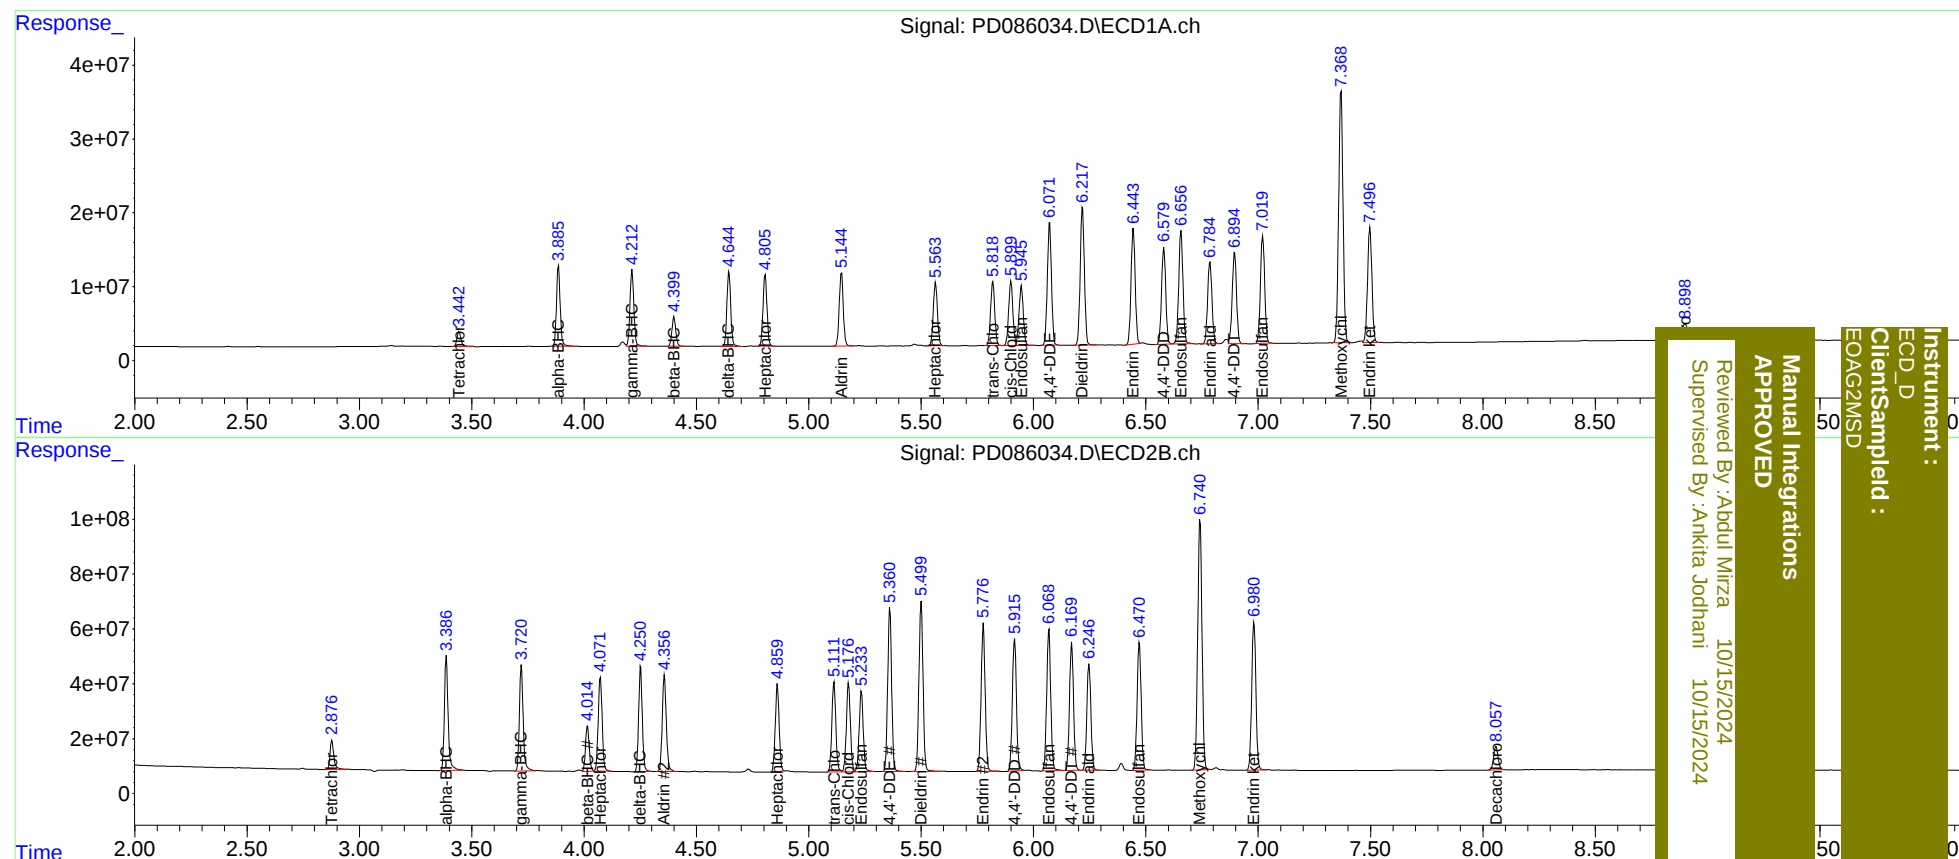

Reviewed By: Abdul Mirza 10/15/2024
Supervised By: Ankita Jodhani 10/15/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
EOAGZMSD