

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101519\
 Data File : PD055269.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2019 18:27
 Operator : SG\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA201

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:13:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101519CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 16 04:12:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.963	6385565	9321416	10.246	10.041
27)	SA Decachlor...	7.967	8.999	14210743	20874534	20.709	21.131
Target Compounds							
2)	A alpha-BHC	3.717	4.349	9051047	12398852	9.770	9.527
3)	MA gamma-BHC...	3.993	4.632	8510727	12689217	9.953	9.952
4)	MA Heptachlor	4.278	5.138	5162274	11780273	10.057	9.943
9)	A Endosulfan I	5.286	6.181	7250620	11097888	10.166	9.920
13)	MA Dieldrin	5.525	6.437	15546154	24445136	19.701	19.476
14)	MA Endrin	5.779	6.654	12865278	19201008	19.990	19.553
16)	A 4,4'-DDD	5.913	6.776	11450447	19769736	20.003	19.438
17)	MA 4,4'-DDT	6.148	7.074	7499712	17626458	18.684	18.925
20)	A Methoxychlor	6.697	7.530	21732793	54540831	99.408	99.391


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101519\
Data File : PD055269.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2019 18:27
Operator : SG\AJ
Sample : INDA201
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
INDA201

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:13:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101519CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 16 04:12:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

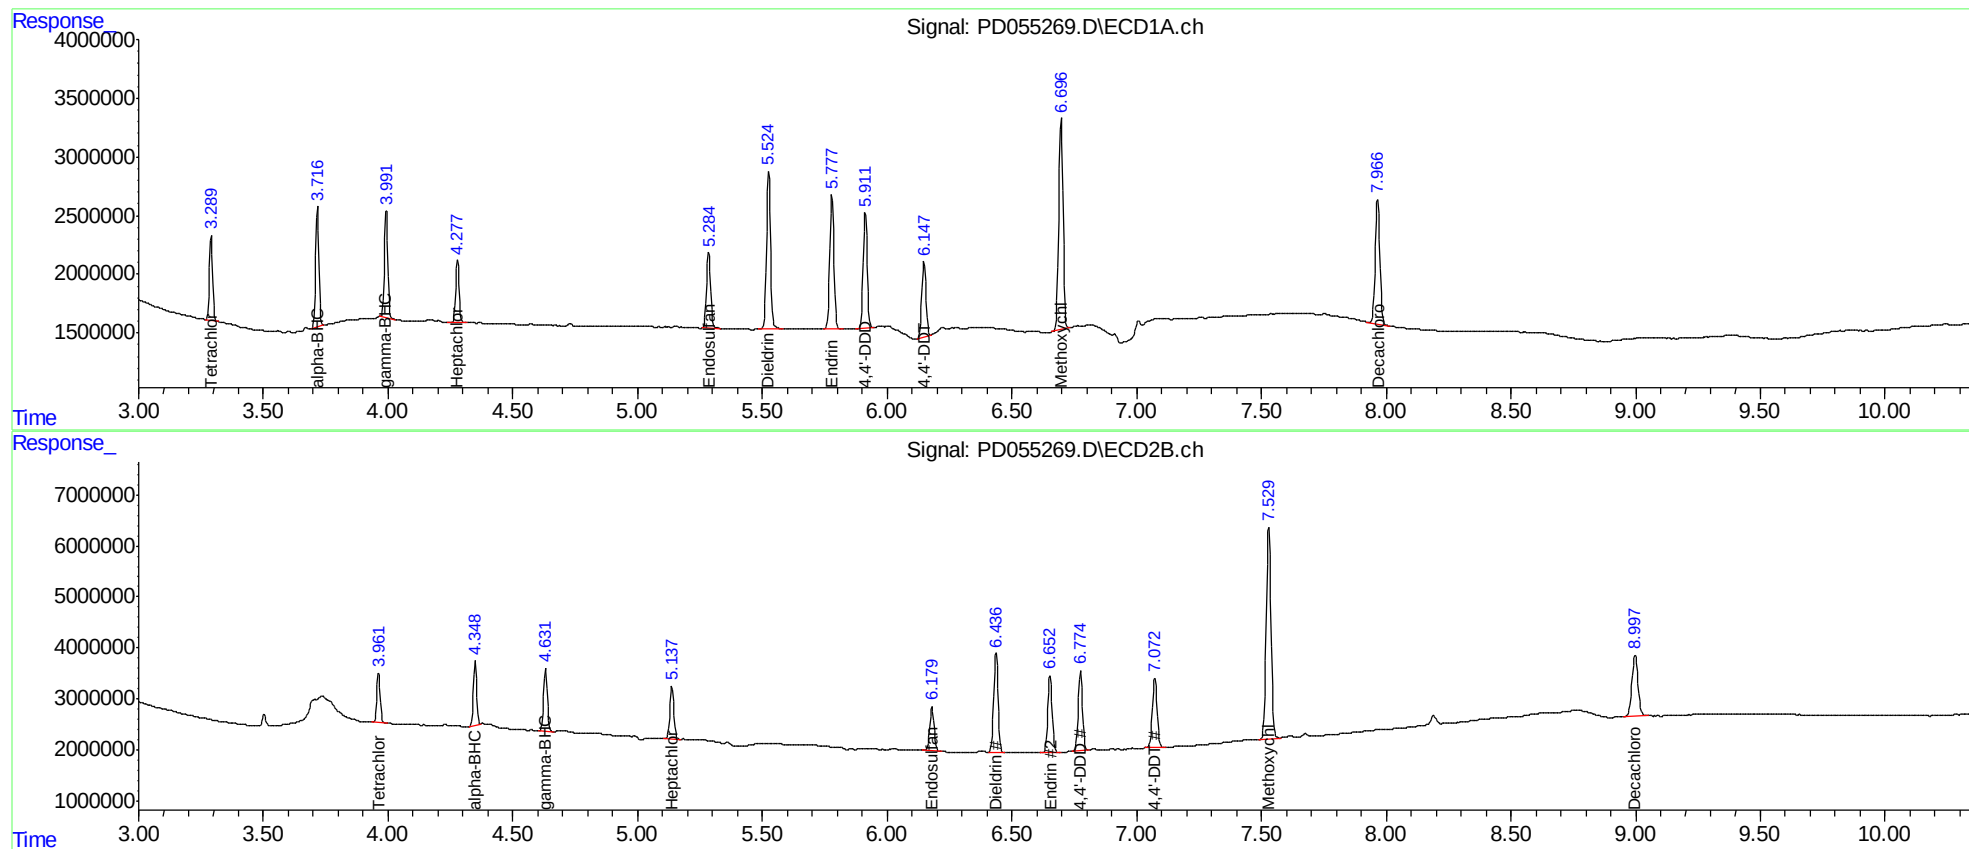


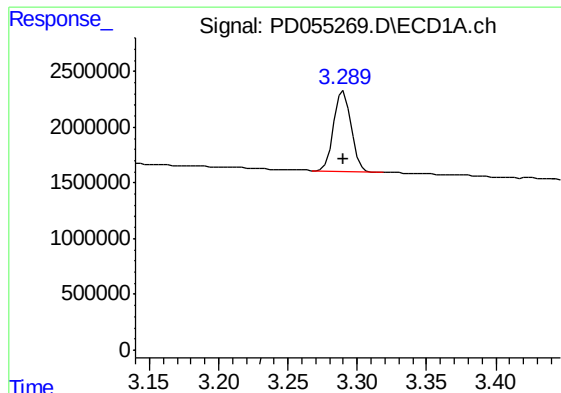

#1 Tetrachloro-m-xylene


R.T.: 3.290 min
Delta R.T.: 0.000 min
Response: 6385565
Conc: 10.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA201

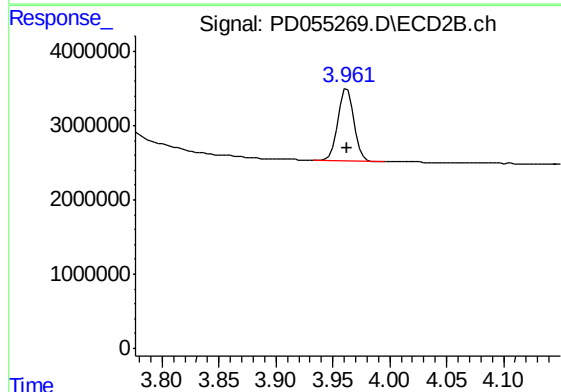


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 9321416
Conc: 10.04 ng/ml

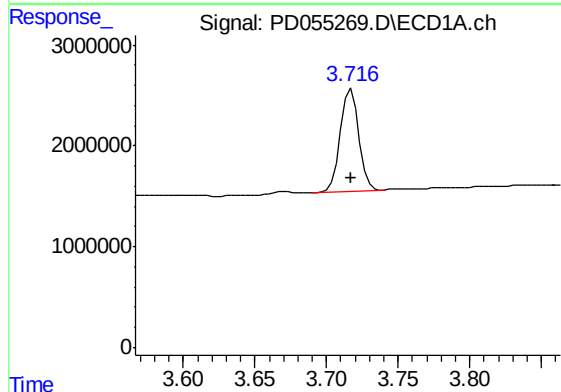


#2 alpha-BHC

R.T.: 3.717 min
Delta R.T.: 0.000 min
Response: 9051047
Conc: 9.77 ng/ml

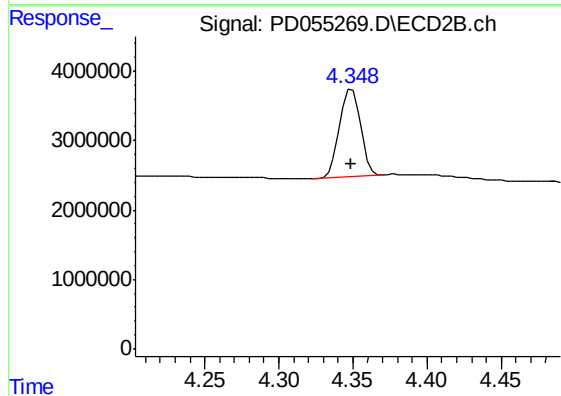

#2 alpha-BHC


R.T.: 4.349 min
Delta R.T.: 0.000 min
Response: 12398852
Conc: 9.53 ng/ml

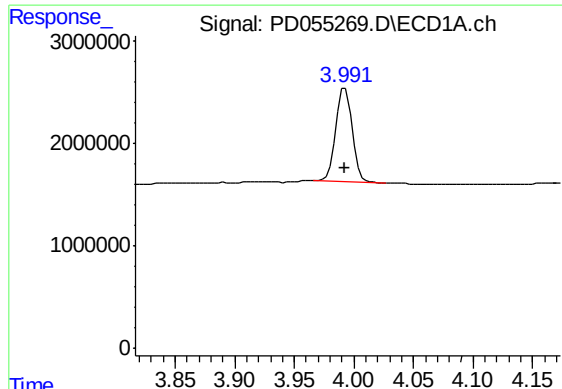

#3 gamma-BHC (Lindane)


R.T.: 3.993 min
Delta R.T.: 0.000 min
Response: 8510727
Conc: 9.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA201

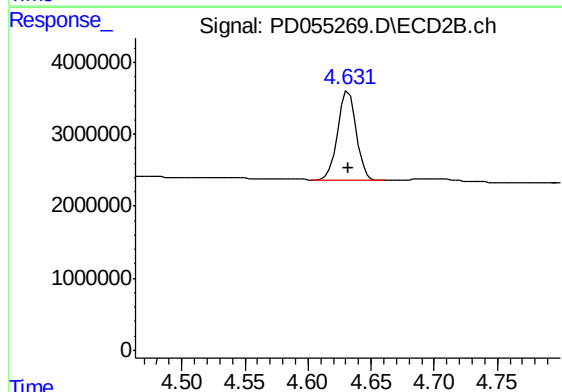


#3 gamma-BHC (Lindane)

R.T.: 4.632 min
Delta R.T.: 0.000 min
Response: 12689217
Conc: 9.95 ng/ml

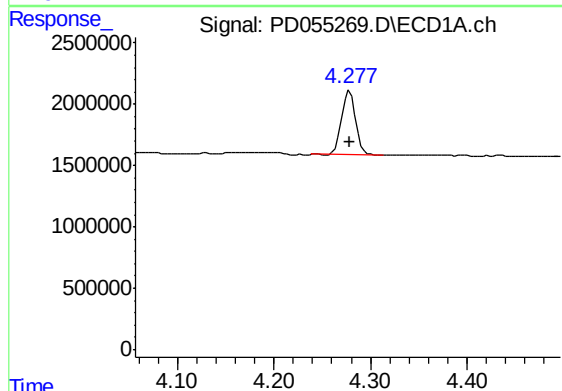


#4 Heptachlor

R.T.: 4.278 min
Delta R.T.: 0.000 min
Response: 5162274
Conc: 10.06 ng/ml

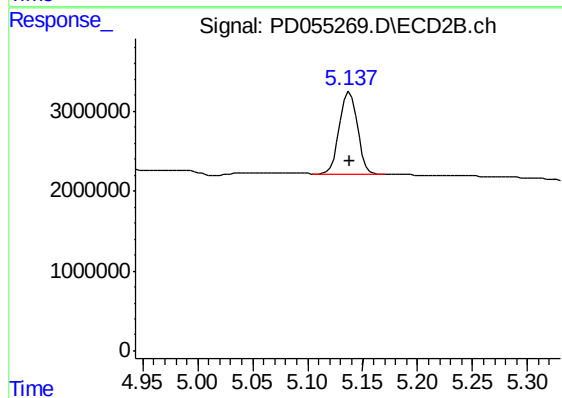

#4 Heptachlor


R.T.: 5.138 min
Delta R.T.: 0.000 min
Response: 11780273
Conc: 9.94 ng/ml

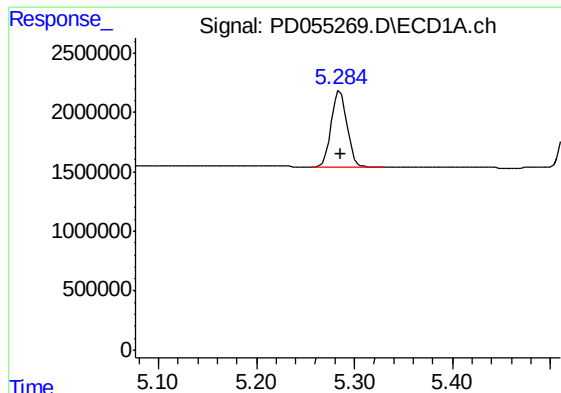

#9 Endosulfan I


R.T.: 5.286 min
Delta R.T.: 0.000 min
Response: 7250620
Conc: 10.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA201

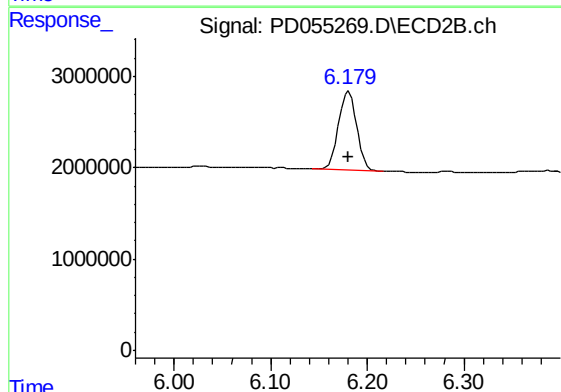


#9 Endosulfan I

R.T.: 6.181 min
Delta R.T.: 0.000 min
Response: 11097888
Conc: 9.92 ng/ml

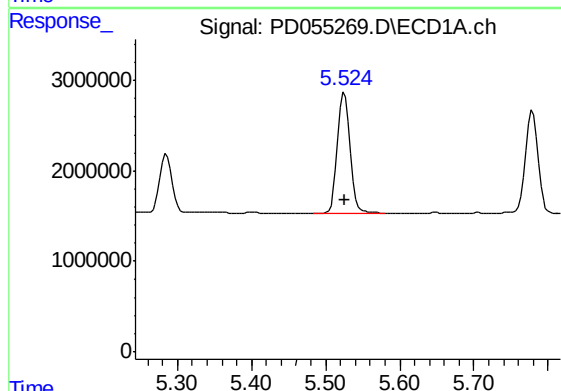


#13 Dieldrin

R.T.: 5.525 min
Delta R.T.: 0.000 min
Response: 15546154
Conc: 19.70 ng/ml

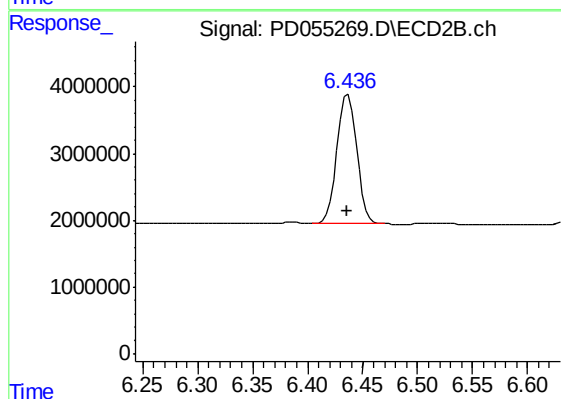

#13 Dieldrin


R.T.: 6.437 min
Delta R.T.: 0.000 min
Response: 24445136
Conc: 19.48 ng/ml

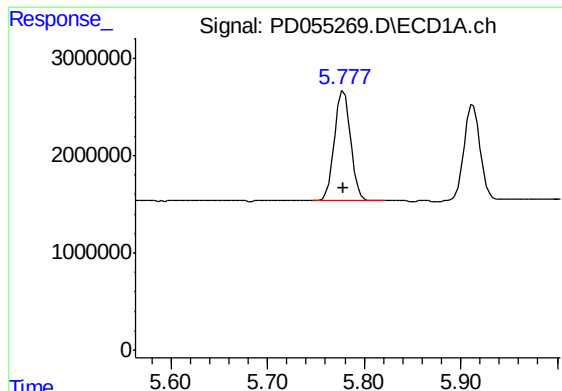

#14 Endrin


R.T.: 5.779 min
Delta R.T.: 0.000 min
Response: 12865278
Conc: 19.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA201

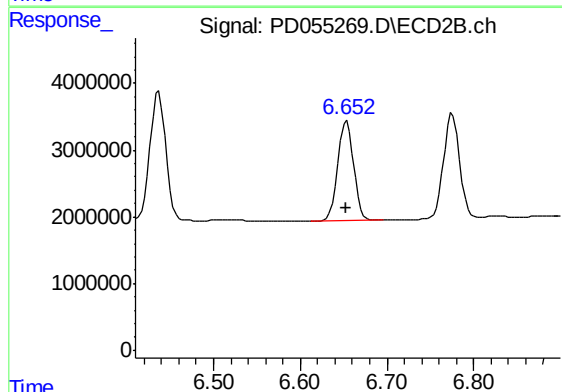


#14 Endrin

R.T.: 6.654 min
Delta R.T.: 0.000 min
Response: 19201008
Conc: 19.55 ng/ml

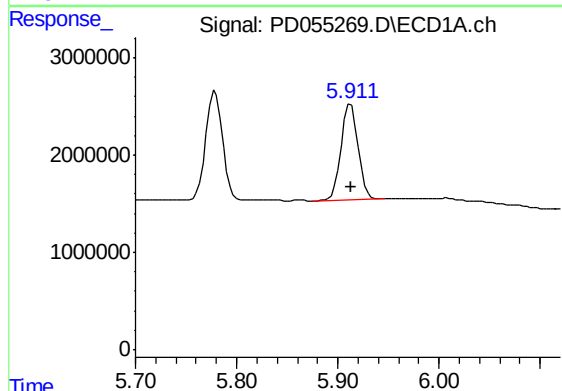


#16 4,4'-DDD

R.T.: 5.913 min
Delta R.T.: 0.000 min
Response: 11450447
Conc: 20.00 ng/ml

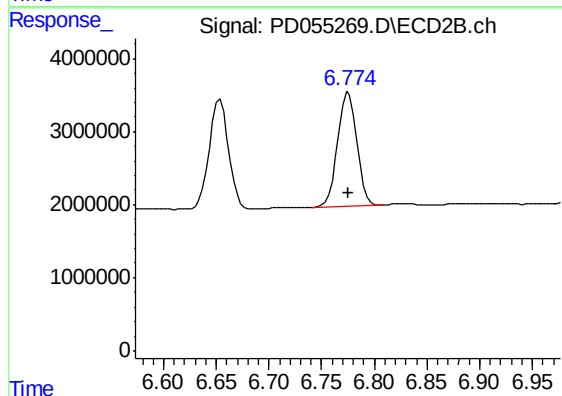

#16 4,4'-DDD


R.T.: 6.776 min
Delta R.T.: 0.000 min
Response: 19769736
Conc: 19.44 ng/ml

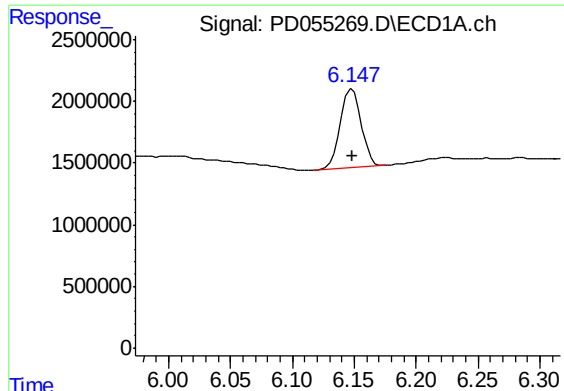

#17 4,4'-DDT


R.T.: 6.148 min
Delta R.T.: 0.000 min
Response: 7499712
Conc: 18.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA201

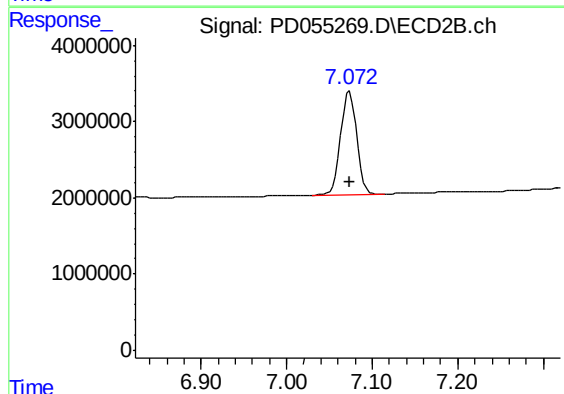


#17 4,4'-DDT

R.T.: 7.074 min
Delta R.T.: 0.000 min
Response: 17626458
Conc: 18.93 ng/ml

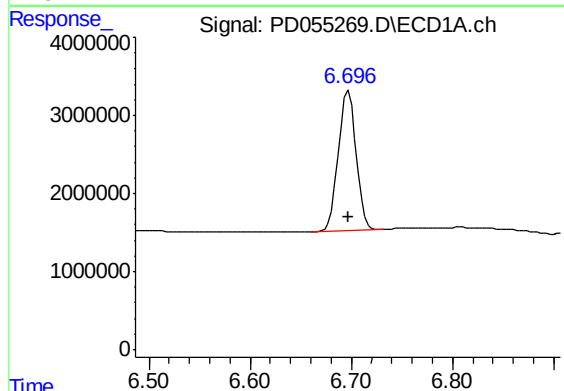


#20 Methoxychlor

R.T.: 6.697 min
Delta R.T.: 0.000 min
Response: 21732793
Conc: 99.41 ng/ml

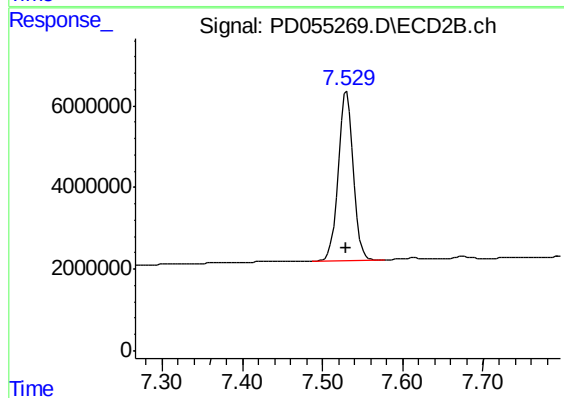

#20 Methoxychlor


R.T.: 7.530 min
Delta R.T.: 0.000 min
Response: 54540831
Conc: 99.39 ng/ml

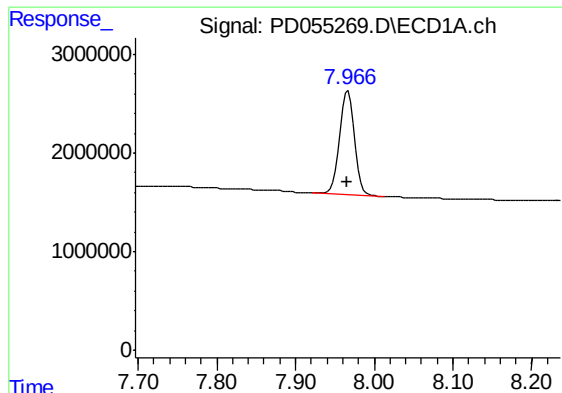

#27 Decachlorobiphenyl

R.T.: 7.967 min
Delta R.T.: 0.000 min
Response: 14210743
Conc: 20.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA201

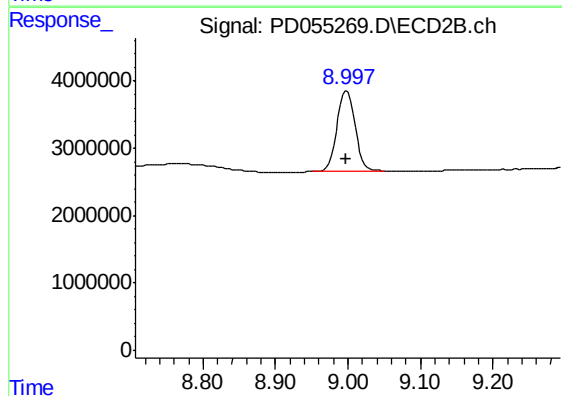

#27 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: 0.000 min
Response: 20874534
Conc: 21.13 ng/ml