

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101519\
 Data File : PD055271.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2019 18:55
 Operator : SG\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA301

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:14:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101519CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 16 04:12:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.963	12465043	18566987	20.000	20.000
27)	SA Decachlor...	7.966	8.998	27449088	39514433	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.717	4.349	18528077	26028238	20.000	20.000
3)	MA gamma-BHC...	3.993	4.632	17102538	25499735	20.000	20.000
4)	MA Heptachlor	4.278	5.138	10266499	23695660	20.000	20.000
9)	A Endosulfan I	5.286	6.181	14264945	22374323	20.000	20.000
13)	MA Dieldrin	5.525	6.436	31563984	50206163	40.000	40.000
14)	MA Endrin	5.779	6.653	25743145	39278931	40.000	40.000
16)	A 4,4'-DDD	5.913	6.776	22897019	40683293	40.000	40.000
17)	MA 4,4'-DDT	6.148	7.073	16056201	37255267	40.000	40.000
20)	A Methoxychlor	6.698	7.530	43724568	109.8E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101519\
Data File : PD055271.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2019 18:55
Operator : SG\AJ
Sample : INDA301
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
INDA301

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:14:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101519CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 16 04:12:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

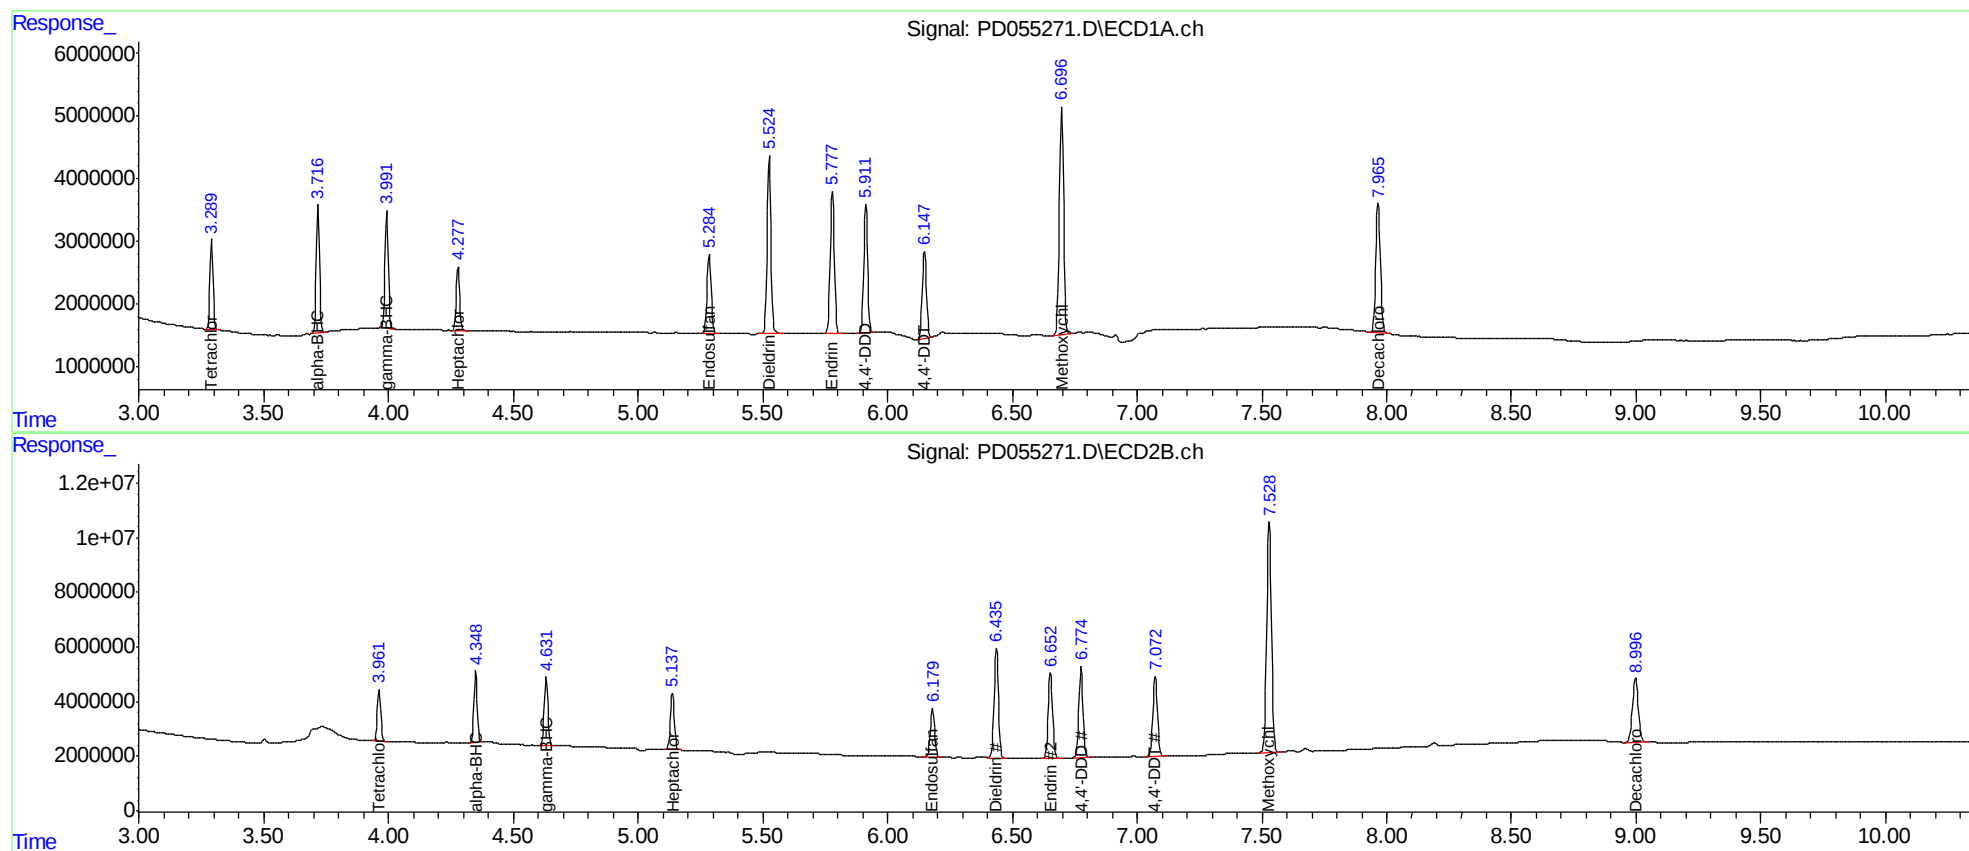


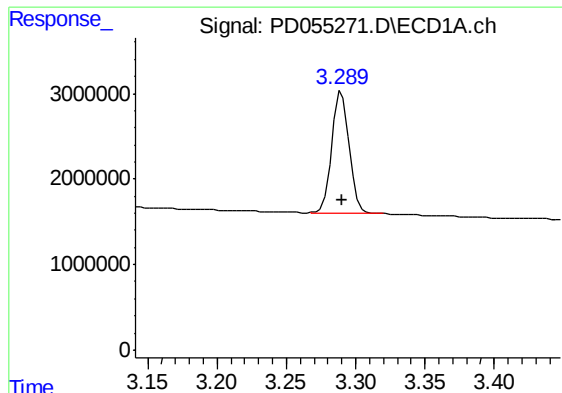

#1 Tetrachloro-m-xylene


R.T.: 3.290 min
Delta R.T.: 0.000 min
Response: 12465043
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA301

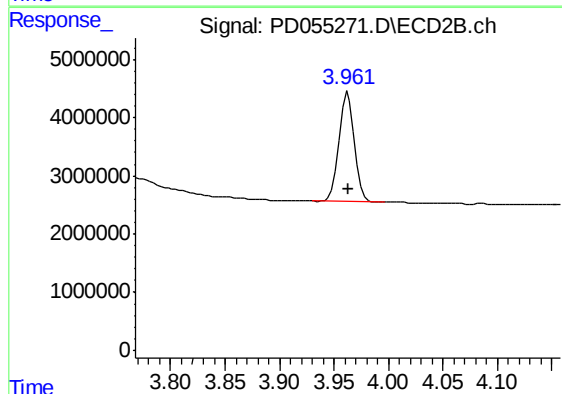


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 18566987
Conc: 20.00 ng/ml

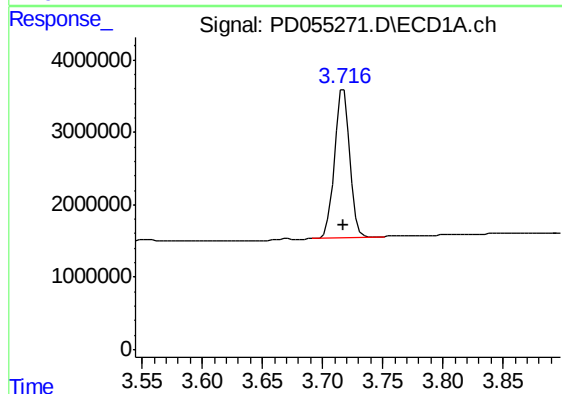


#2 alpha-BHC

R.T.: 3.717 min
Delta R.T.: 0.000 min
Response: 18528077
Conc: 20.00 ng/ml

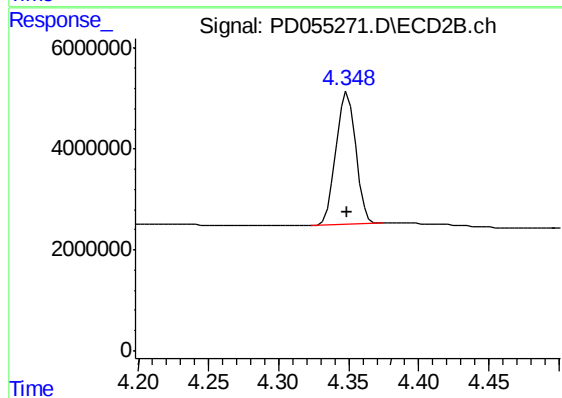

#2 alpha-BHC


R.T.: 4.349 min
Delta R.T.: 0.000 min
Response: 26028238
Conc: 20.00 ng/ml

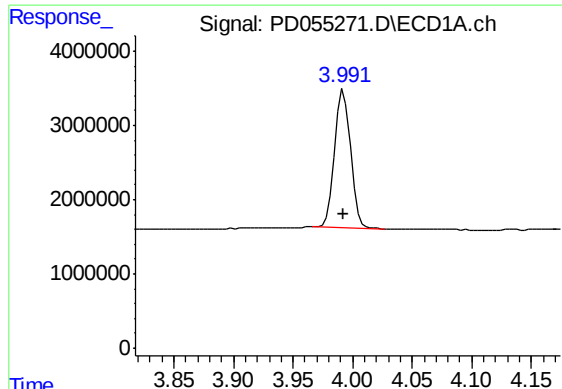

#3 gamma-BHC (Lindane)


R.T.: 3.993 min
Delta R.T.: 0.000 min
Response: 17102538
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA301

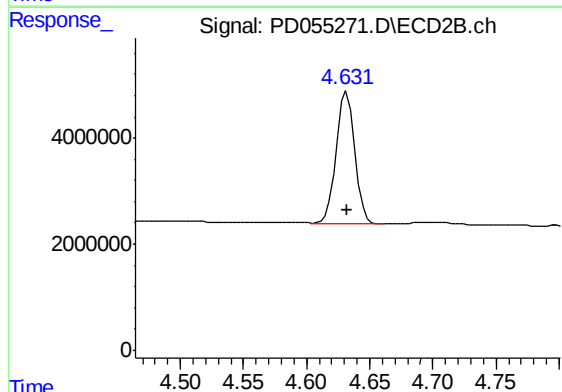


#3 gamma-BHC (Lindane)

R.T.: 4.632 min
Delta R.T.: 0.000 min
Response: 25499735
Conc: 20.00 ng/ml

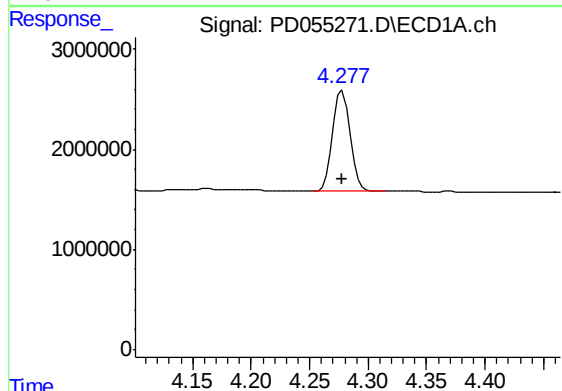


#4 Heptachlor

R.T.: 4.278 min
Delta R.T.: 0.000 min
Response: 10266499
Conc: 20.00 ng/ml

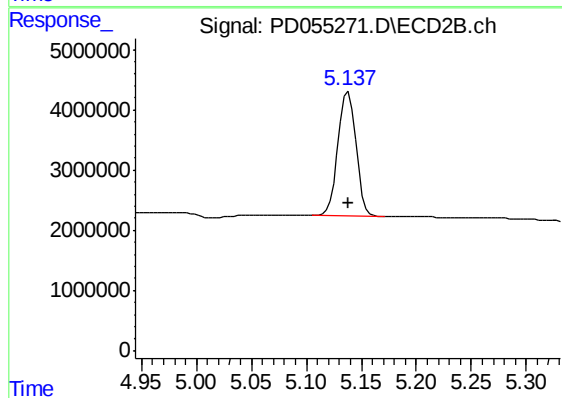

#4 Heptachlor


R.T.: 5.138 min
Delta R.T.: 0.000 min
Response: 23695660
Conc: 20.00 ng/ml

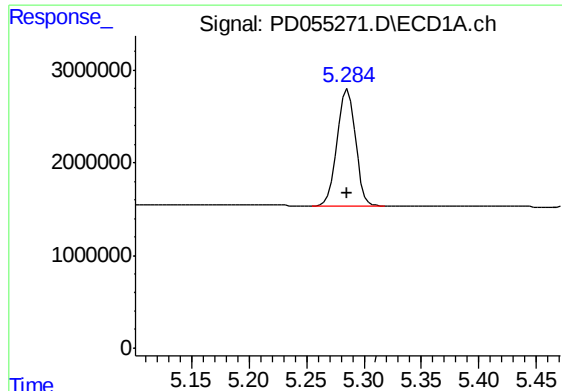

#9 Endosulfan I


R.T.: 5.286 min
Delta R.T.: 0.000 min
Response: 14264945
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA301

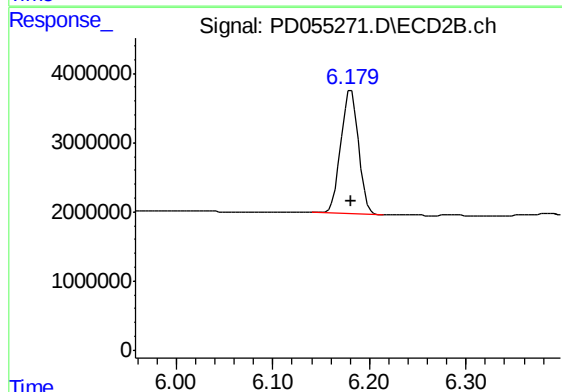


#9 Endosulfan I

R.T.: 6.181 min
Delta R.T.: 0.000 min
Response: 22374323
Conc: 20.00 ng/ml

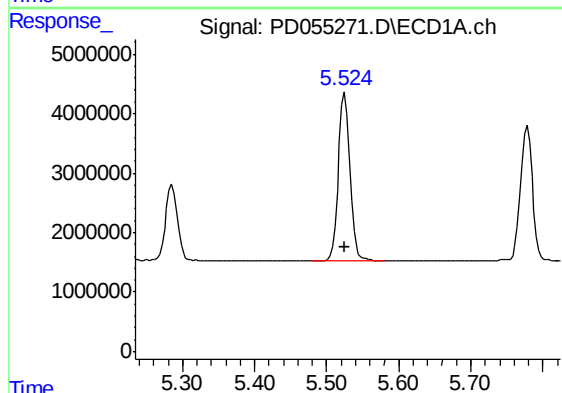


#13 Dieldrin

R.T.: 5.525 min
Delta R.T.: 0.000 min
Response: 31563984
Conc: 40.00 ng/ml

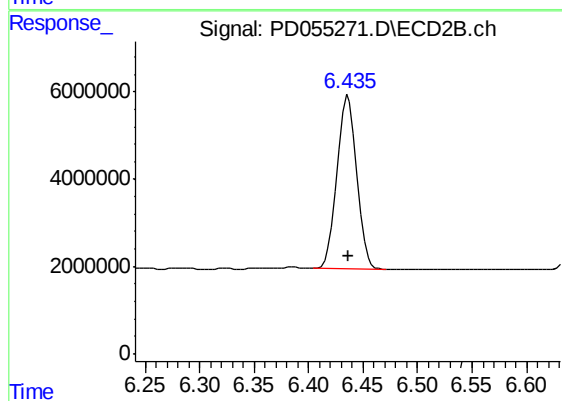

#13 Dieldrin


R.T.: 6.436 min
Delta R.T.: 0.000 min
Response: 50206163
Conc: 40.00 ng/ml

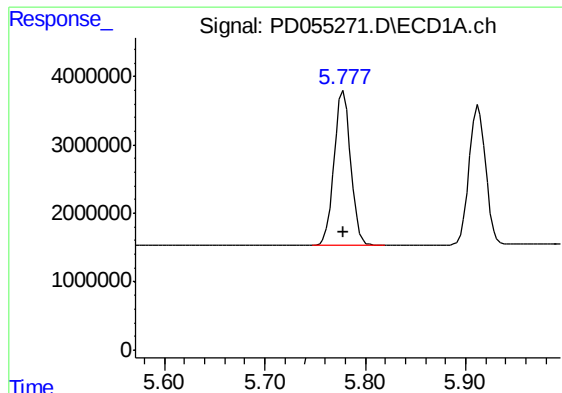

#14 Endrin


R.T.: 5.779 min
Delta R.T.: 0.000 min
Response: 25743145
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA301

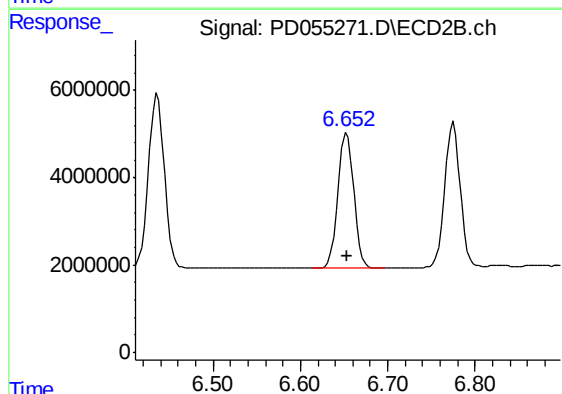


#14 Endrin

R.T.: 6.653 min
Delta R.T.: 0.000 min
Response: 39278931
Conc: 40.00 ng/ml

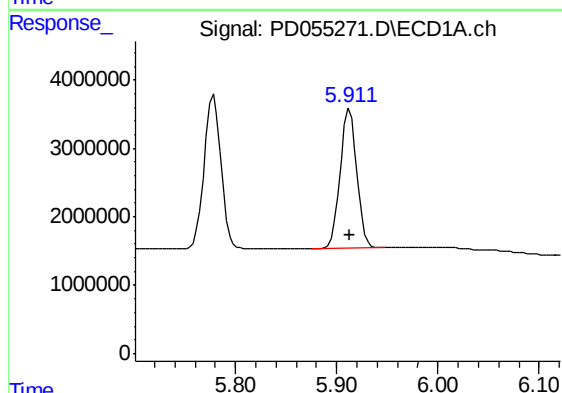


#16 4,4'-DDD

R.T.: 5.913 min
Delta R.T.: 0.000 min
Response: 22897019
Conc: 40.00 ng/ml

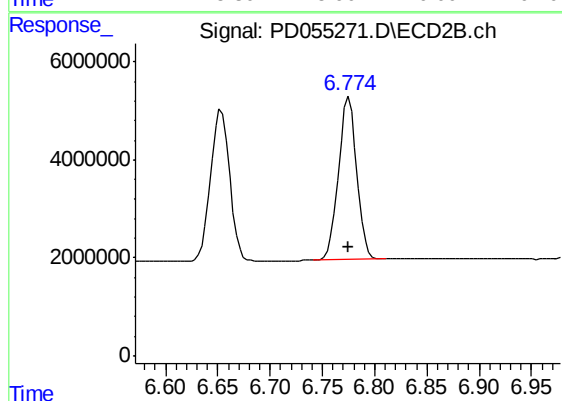

#16 4,4'-DDD


R.T.: 6.776 min
Delta R.T.: 0.000 min
Response: 40683293
Conc: 40.00 ng/ml

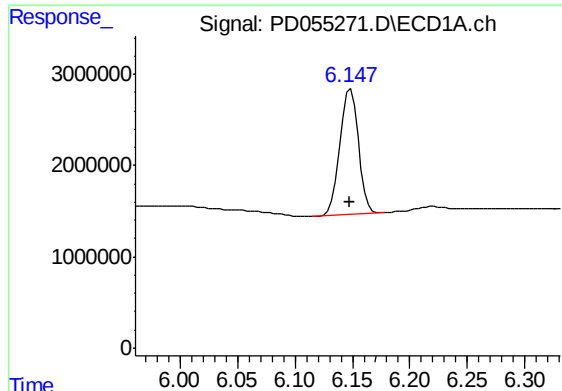

#17 4,4'-DDT


R.T.: 6.148 min
Delta R.T.: 0.000 min
Response: 16056201
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA301

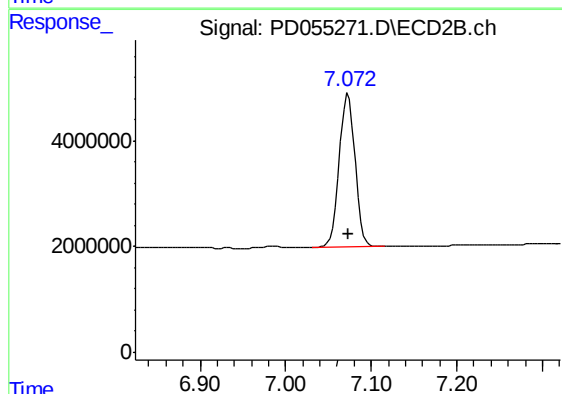


#17 4,4'-DDT

R.T.: 7.073 min
Delta R.T.: 0.000 min
Response: 37255267
Conc: 40.00 ng/ml

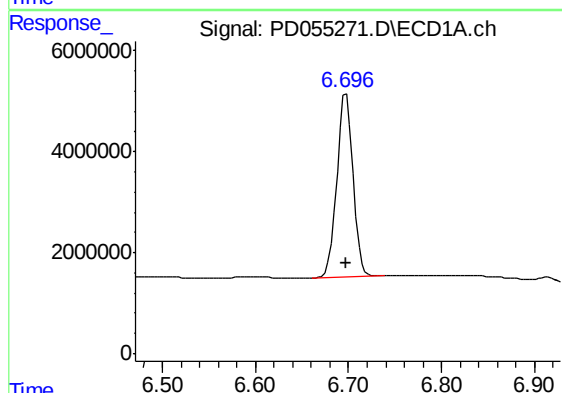


#20 Methoxychlor

R.T.: 6.698 min
Delta R.T.: 0.000 min
Response: 43724568
Conc: 200.00 ng/ml

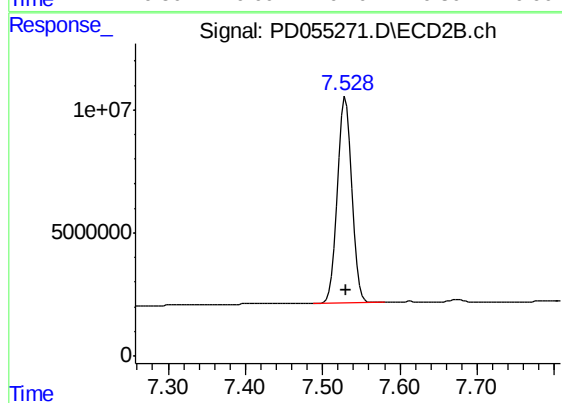

#20 Methoxychlor


R.T.: 7.530 min
Delta R.T.: 0.000 min
Response: 109750043
Conc: 200.00 ng/ml

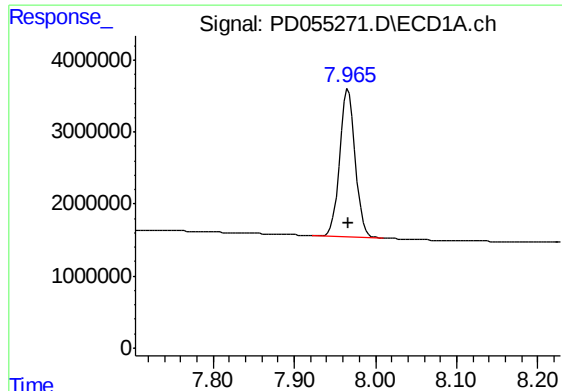

#27 Decachlorobiphenyl

R.T.: 7.966 min
Delta R.T.: 0.000 min
Response: 27449088
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA301

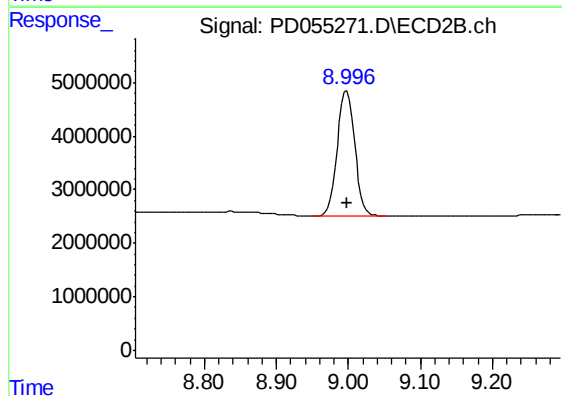

#27 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.000 min
Response: 39514433
Conc: 40.00 ng/ml