

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101519\
 Data File : PD055273.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2019 19:23
 Operator : SG\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA401

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:14:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101519CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 16 04:12:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.963	24967864	37308787	40.061	40.188
27)	SA Decachlor...	7.967	8.998	53543210	77171431	78.025	78.120
Target Compounds							
2)	A alpha-BHC	3.717	4.349	38358271	54642387	41.406	41.987
3)	MA gamma-BHC...	3.992	4.632	35113325	52610836	41.062	41.264
4)	MA Heptachlor	4.278	5.137	20420250	48444948	39.780	40.889
9)	A Endosulfan I	5.286	6.180	28770846	45569930	40.338	40.734
13)	MA Dieldrin	5.526	6.436	64851468	104.2E6	82.184	82.993
14)	MA Endrin	5.778	6.653	52089718	80655084	80.938	82.136
16)	A 4,4'-DDD	5.912	6.775	46636551	83947416	81.472	82.537
17)	MA 4,4'-DDT	6.148	7.073	34599620	78824652	86.196	84.632
20)	A Methoxychlor	6.697	7.530	87782098	220.4E6	401.523	401.613


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101519\
Data File : PD055273.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2019 19:23
Operator : SG\AJ
Sample : INDA401
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
INDA401

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:14:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101519CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 16 04:12:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

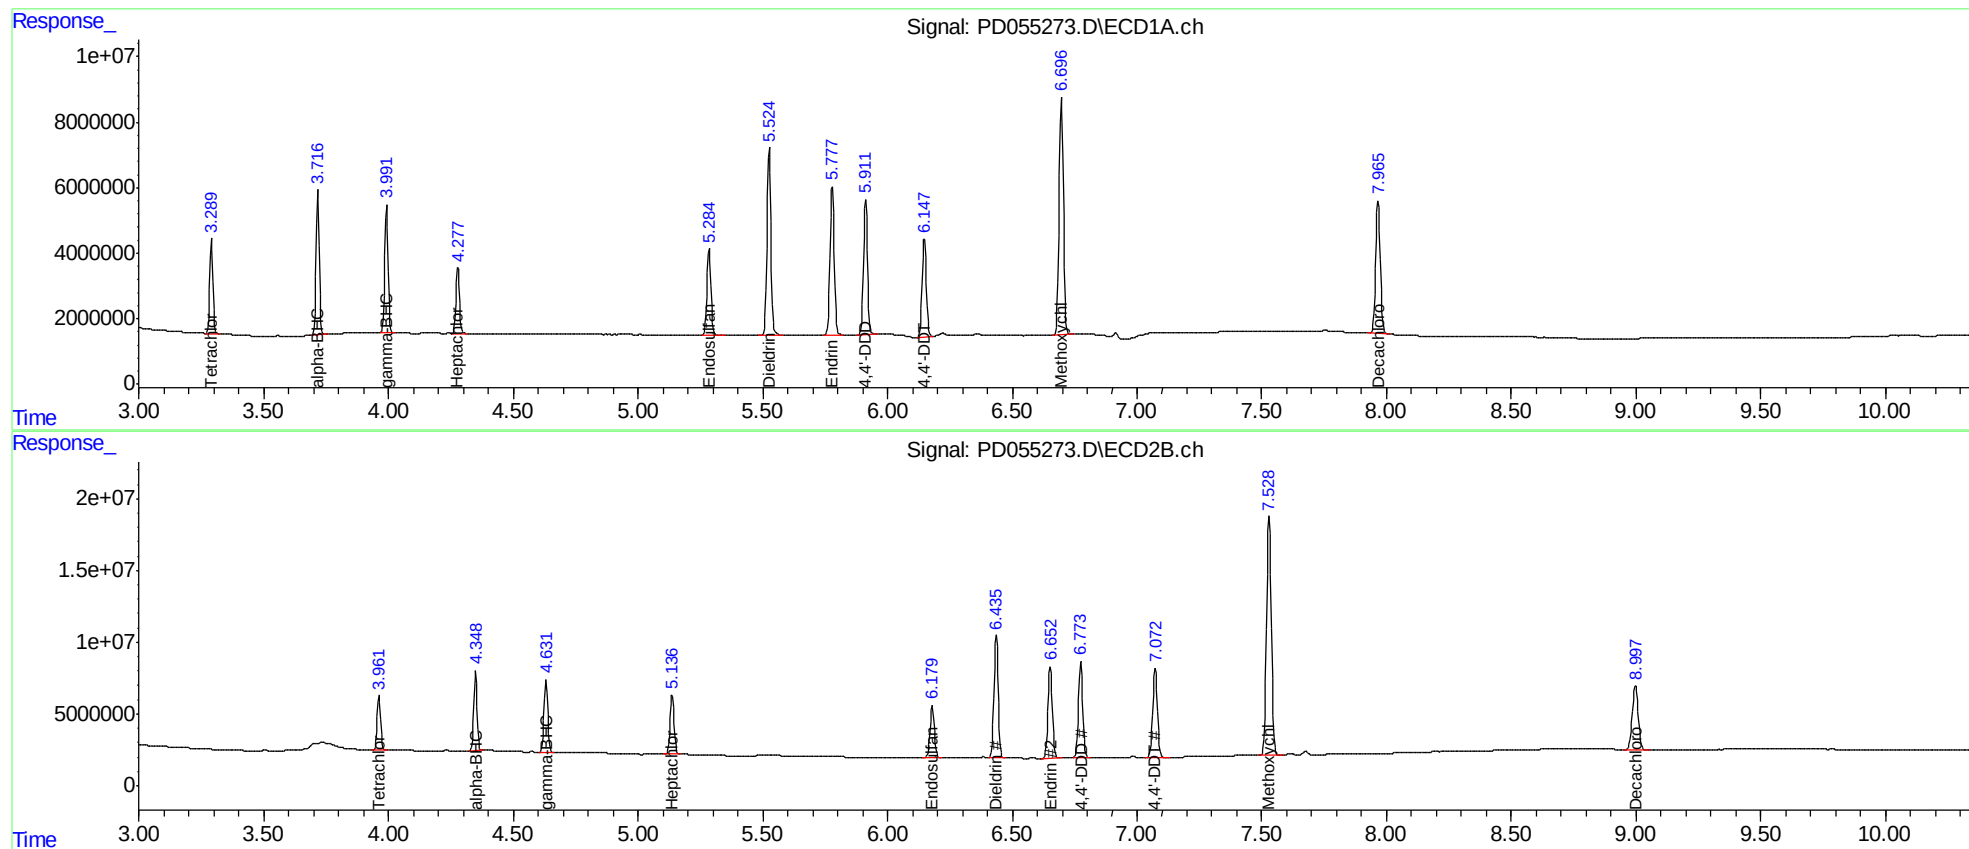


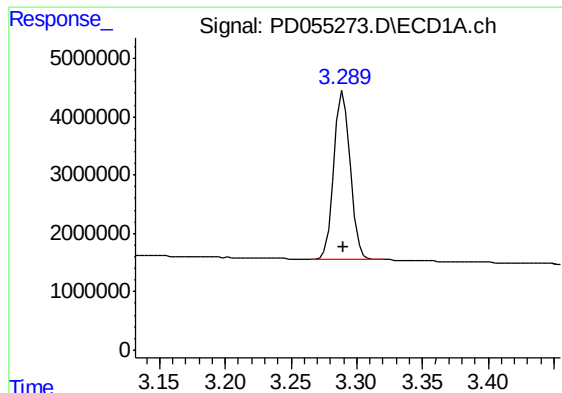

#1 Tetrachloro-m-xylene


R.T.: 3.290 min
Delta R.T.: 0.000 min
Response: 24967864
Conc: 40.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

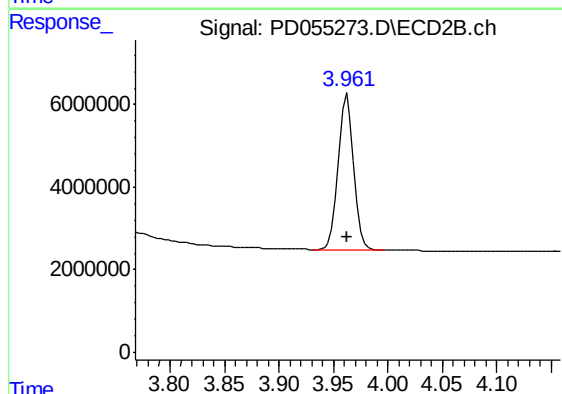


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 37308787
Conc: 40.19 ng/ml

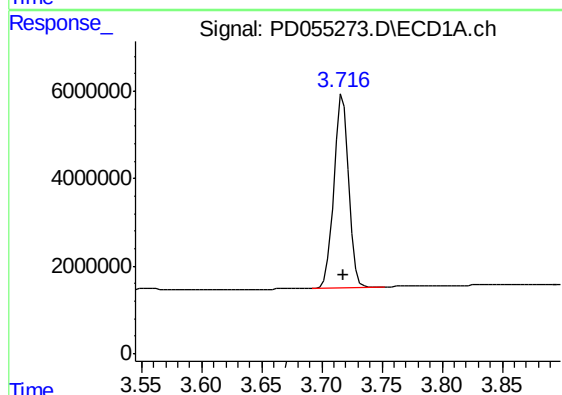


#2 alpha-BHC

R.T.: 3.717 min
Delta R.T.: 0.000 min
Response: 38358271
Conc: 41.41 ng/ml

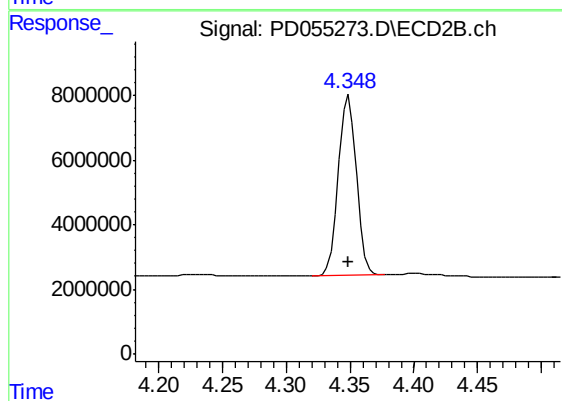

#2 alpha-BHC


R.T.: 4.349 min
Delta R.T.: 0.000 min
Response: 54642387
Conc: 41.99 ng/ml

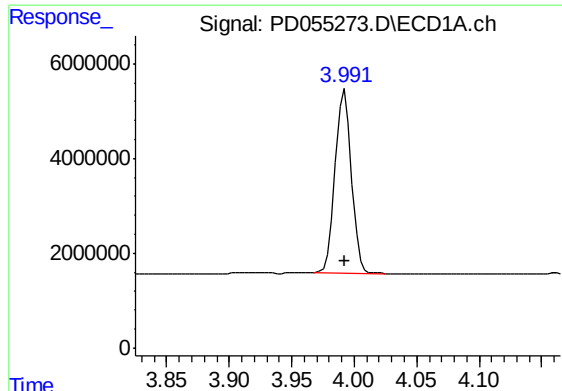

#3 gamma-BHC (Lindane)


R.T.: 3.992 min
Delta R.T.: 0.000 min
Response: 35113325
Conc: 41.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

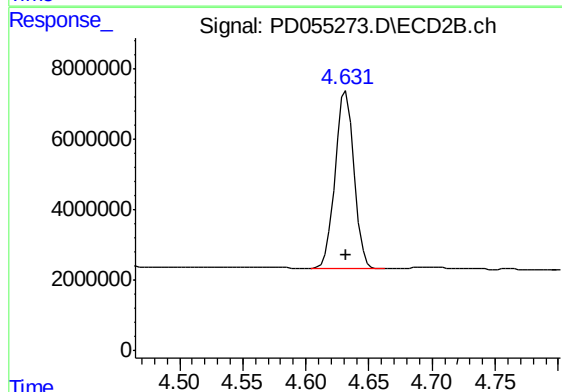


#3 gamma-BHC (Lindane)

R.T.: 4.632 min
Delta R.T.: 0.000 min
Response: 52610836
Conc: 41.26 ng/ml

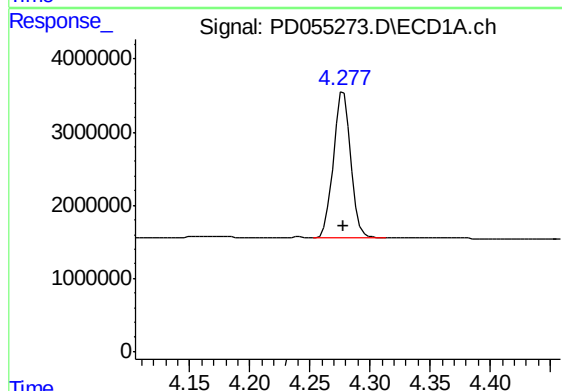


#4 Heptachlor

R.T.: 4.278 min
Delta R.T.: 0.000 min
Response: 20420250
Conc: 39.78 ng/ml

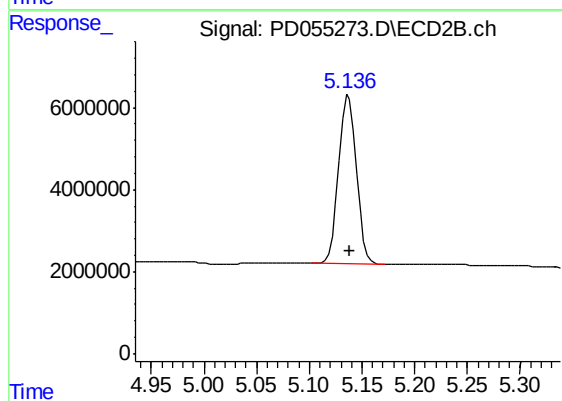

#4 Heptachlor


R.T.: 5.137 min
Delta R.T.: 0.000 min
Response: 48444948
Conc: 40.89 ng/ml

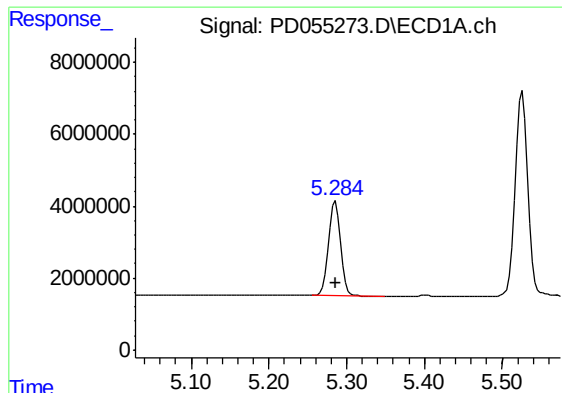

#9 Endosulfan I


R.T.: 5.286 min
Delta R.T.: 0.000 min
Response: 28770846
Conc: 40.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

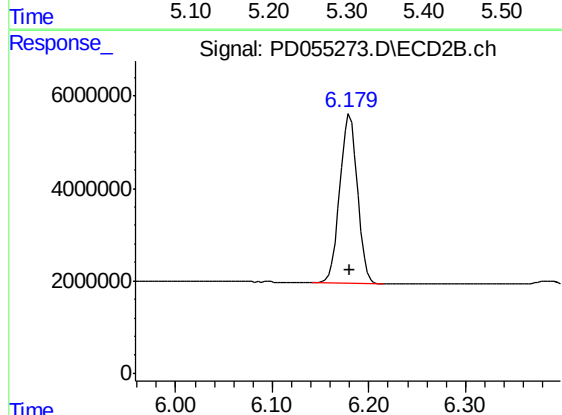


#9 Endosulfan I

R.T.: 6.180 min
Delta R.T.: 0.000 min
Response: 45569930
Conc: 40.73 ng/ml

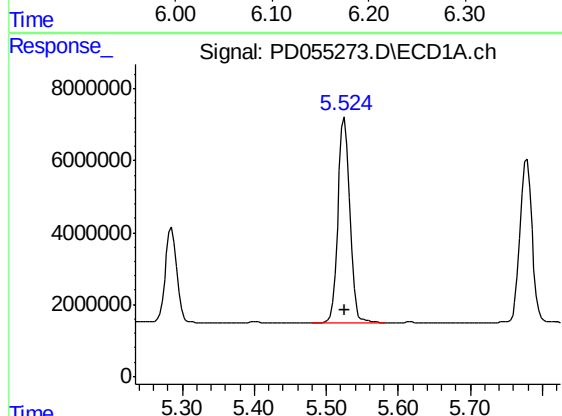


#13 Dieldrin

R.T.: 5.526 min
Delta R.T.: 0.000 min
Response: 64851468
Conc: 82.18 ng/ml

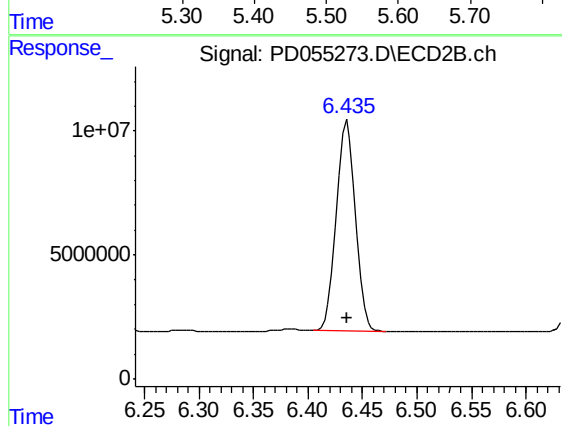

#13 Dieldrin


R.T.: 6.436 min
Delta R.T.: 0.000 min
Response: 104168936
Conc: 82.99 ng/ml

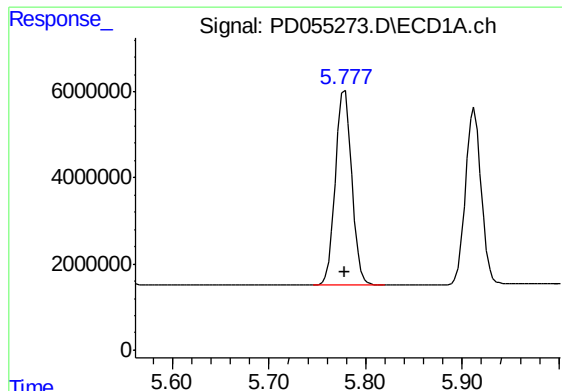

#14 Endrin


R.T.: 5.778 min
Delta R.T.: 0.000 min
Response: 52089718
Conc: 80.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

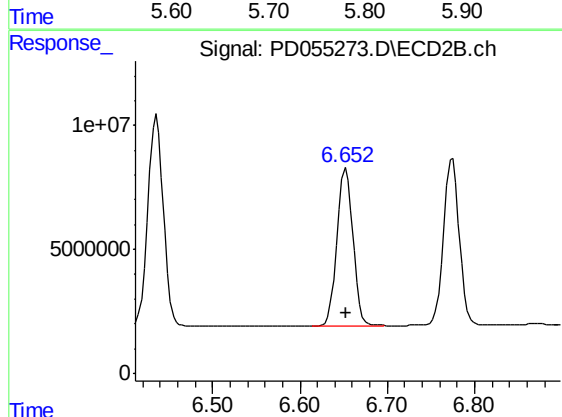


#14 Endrin

R.T.: 6.653 min
Delta R.T.: 0.000 min
Response: 80655084
Conc: 82.14 ng/ml

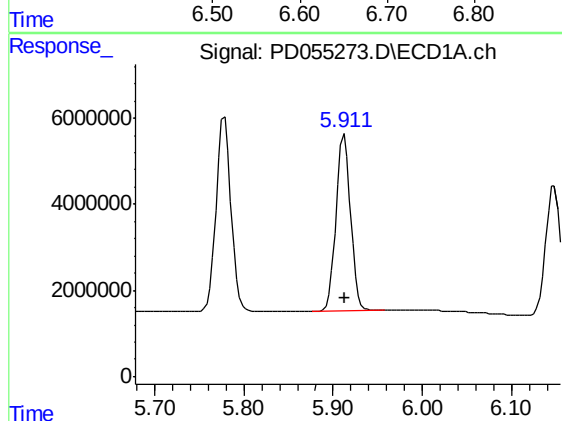


#16 4,4'-DDD

R.T.: 5.912 min
Delta R.T.: 0.000 min
Response: 46636551
Conc: 81.47 ng/ml

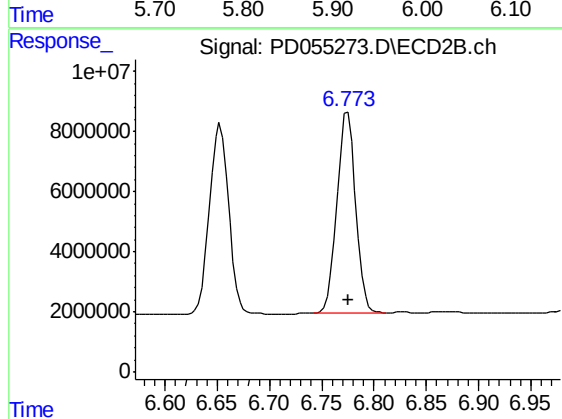

#16 4,4'-DDD


R.T.: 6.775 min
Delta R.T.: 0.000 min
Response: 83947416
Conc: 82.54 ng/ml

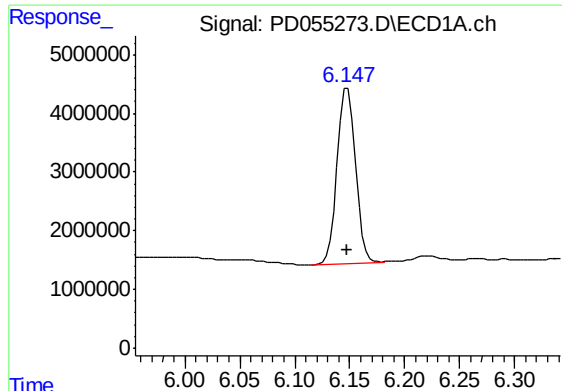

#17 4,4'-DDT


R.T.: 6.148 min
Delta R.T.: 0.000 min
Response: 34599620
Conc: 86.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

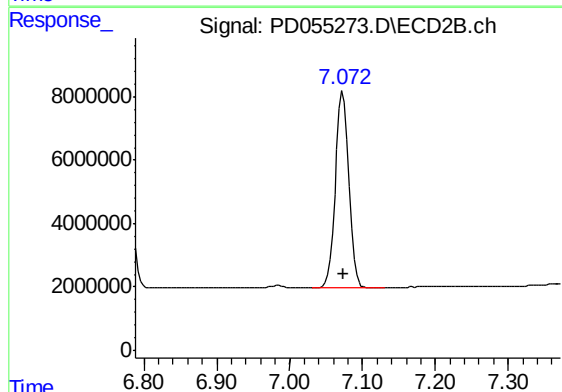


#17 4,4'-DDT

R.T.: 7.073 min
Delta R.T.: 0.000 min
Response: 78824652
Conc: 84.63 ng/ml

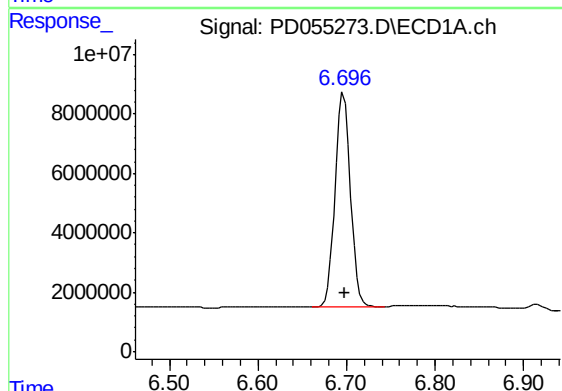


#20 Methoxychlor

R.T.: 6.697 min
Delta R.T.: 0.000 min
Response: 87782098
Conc: 401.52 ng/ml

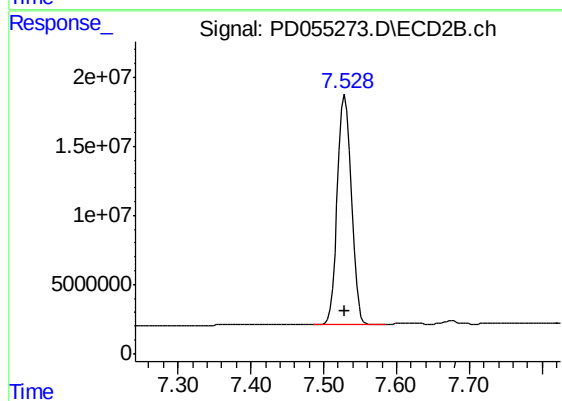

#20 Methoxychlor


R.T.: 7.530 min
Delta R.T.: 0.000 min
Response: 220385427
Conc: 401.61 ng/ml

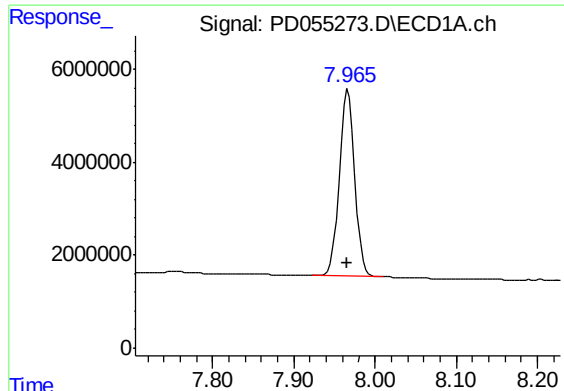

#27 Decachlorobiphenyl

R.T.: 7.967 min
Delta R.T.: 0.000 min
Response: 53543210
Conc: 78.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

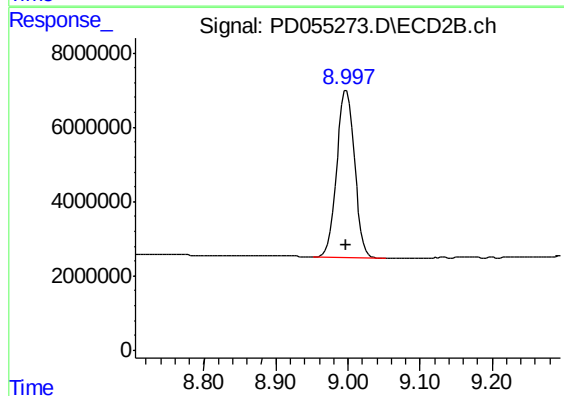

#27 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.000 min
Response: 77171431
Conc: 78.12 ng/ml