

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101519\
 Data File : PD055287.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2019 22:39
 Operator : SG\AJ
 Sample : PB123990BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E0AA5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:59:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101519CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 16 04:32:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.963	13458352	20146006	21.303	21.630
2)	SA Decachlor...	7.967	8.997	26910544	38788661	38.893	39.288
Target Compounds							
19)	B Endosulfa...	0.000	7.242f	0	2941610	N.D.	2.715

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101519\
Data File : PD055287.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2019 22:39
Operator : SG\AJ
Sample : PB123990BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:59:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101519CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 16 04:32:26 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

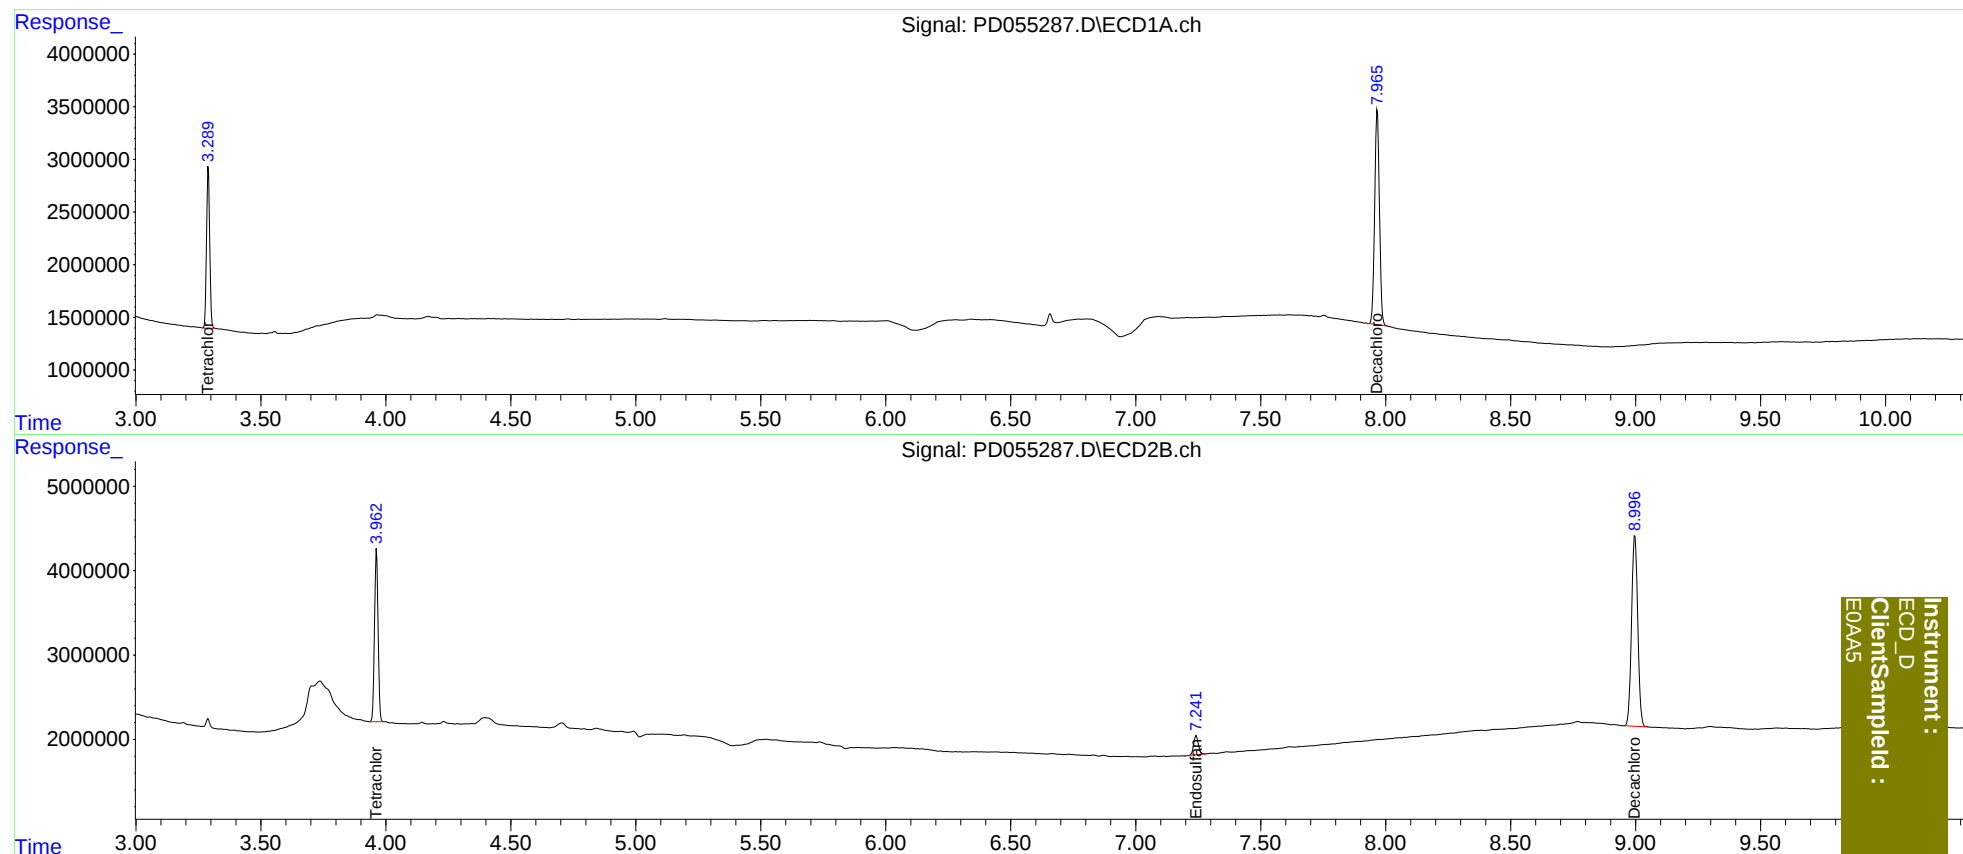


Instrument :
ECD_D
ClientSampleId :
E0AAS

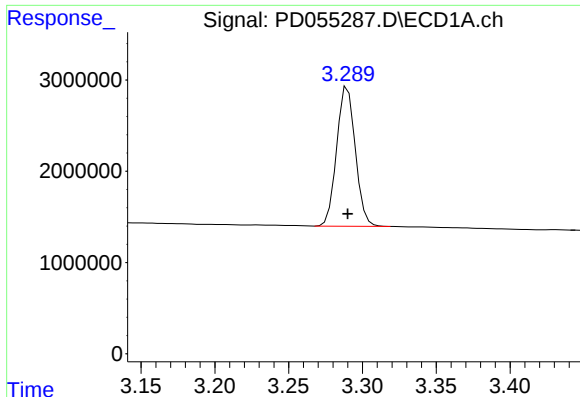

#1 Tetrachloro-m-xylene


R.T.: 3.290 min
Delta R.T.: 0.000 min
Response: 13458352
Conc: 21.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
E0AA5

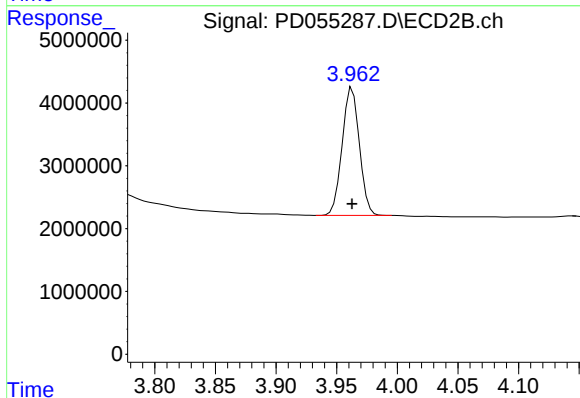


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 20146006
Conc: 21.63 ng/ml

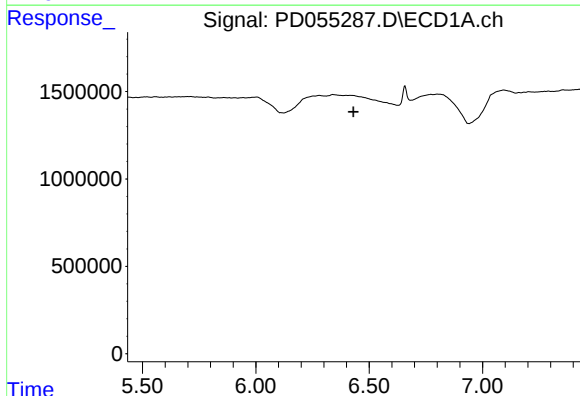


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.431 min
Response: 0
Conc: N.D.

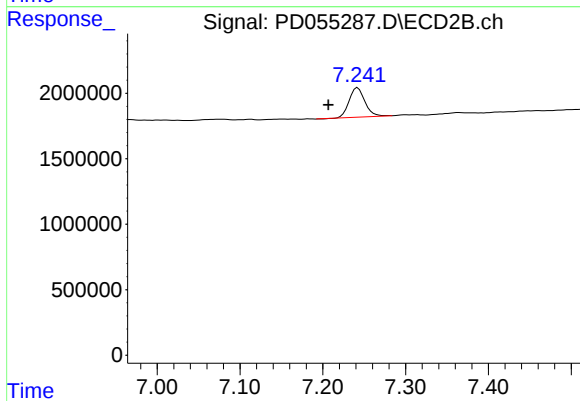

#19 Endosulfan Sulfate


R.T.: 7.242 min
Delta R.T.: 0.035 min
Response: 2941610
Conc: 2.71 ng/ml

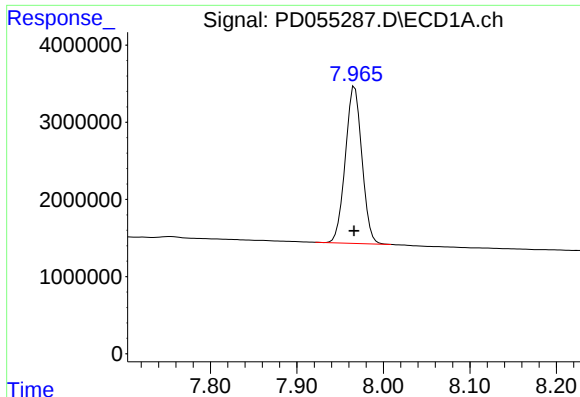

#27 Decachlorobiphenyl

R.T.: 7.967 min
Delta R.T.: 0.000 min
Response: 26910544
Conc: 38.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
E0AA5

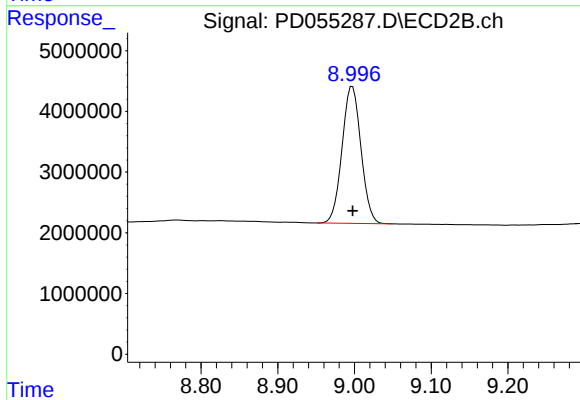

#27 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: 0.000 min
Response: 38788661
Conc: 39.29 ng/ml