

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101519\
 Data File : PD055260.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2019 16:21
 Operator : SG\AJ
 Sample : RESC06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC06

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:57:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101519CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 16 04:32:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.963	11637980	17385339	18.421	18.666
27)	SA Decachlor...	7.966	8.998	25811269	37818335	37.304	38.305
Target Compounds							
2)	A alpha-BHC	3.717	4.349	8546118	11637744	9.105	8.968
3)	MA gamma-BHC...	3.992	4.632	8070580	11780145	9.265	9.145
4)	MA Heptachlor	4.277	5.138	5073205	10936933	9.815	9.170
5)	MB Aldrin	4.517	5.442	7142191	10301712	8.806	8.545
6)	B beta-BHC	4.242	4.800	3731574	5384381	9.226	8.898
7)	B delta-BHC	4.437	5.015	7916391	10091158	8.517	7.859
8)	B Heptachlo...	4.955	5.825	6783110	10035452	8.956	8.512
9)	A Endosulfan I	5.285	6.180	6766577	10240473	9.329	9.080
10)	B trans-Chl...	5.176	6.058	6855249	10762628	8.939	8.796
11)	B cis-Chlor...	5.233	6.131	6568197	10140166	8.834	8.594
12)	B 4,4'-DDE	5.402	6.287	13523449	20766770	17.386	17.300
13)	MA Dieldrin	5.525	6.436	14972718	22971205	18.689	18.183
14)	MA Endrin	5.778	6.653	12425836	18150361	19.181	18.353
15)	B Endosulfa...	6.051	6.861	12903903	20124526	17.791	17.535
16)	A 4,4'-DDD	5.912	6.775	11154356	18620922	19.190	18.253
17)	MA 4,4'-DDT	6.148	7.073	7075061	16788489	17.647	17.963
18)	B Endrin al...	6.220	6.984	11437902	17220779	18.340	17.843
19)	B Endosulfa...	6.431	7.207	12427179	19186884	18.242	17.708
20)	A Methoxychlor	6.696	7.530	21061269	52242574	96.598	95.678
21)	B Endrin ke...	6.914	7.675	13670570	22082127	19.166	18.700


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101519\
Data File : PD055260.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2019 16:21
Operator : SG\AJ
Sample : RESC06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:57:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101519CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 16 04:32:26 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

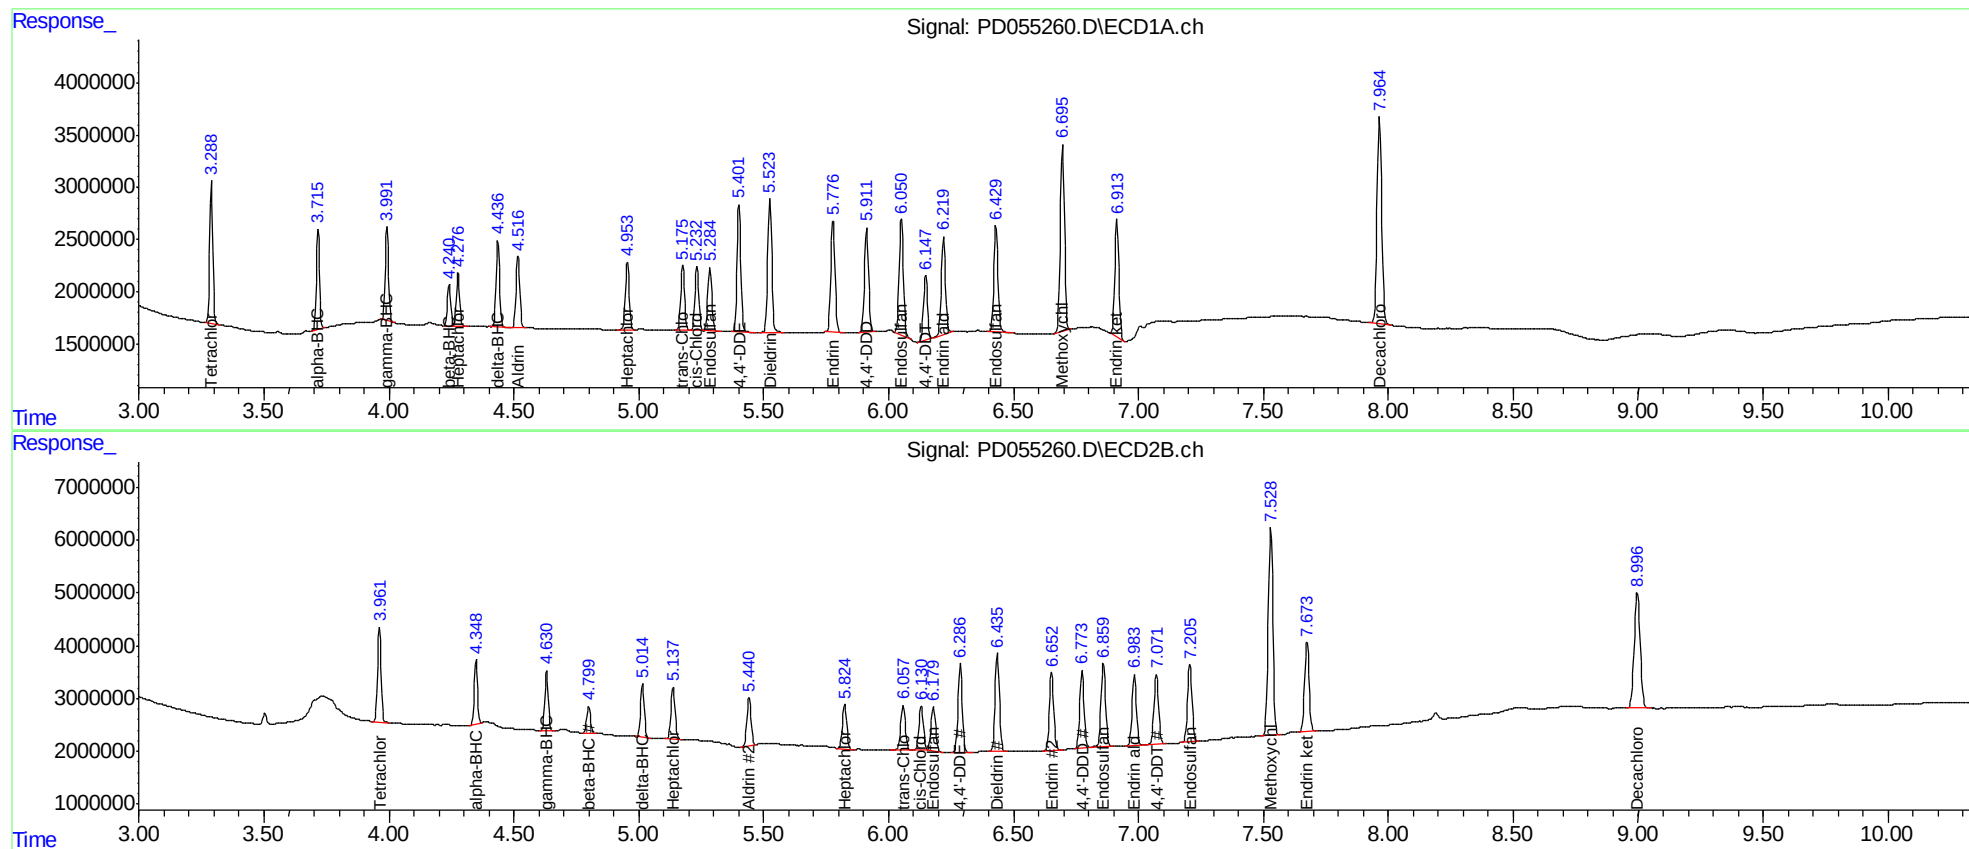

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101519\
Data File : PD055260.D
Acq On : 15 Oct 2019 16:21
Operator : SG\AJ
Sample : RESC06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101519CLP.M
Title : GC Extractables
Last Update : Wed Oct 16 04:32:26 2019
Integrator: ChemStation

RT#1	RT#2	Resolution
3.290	3.717	100.00%
3.717	3.992	100.00%
3.992	4.242	100.00%
4.242	4.277	97.21%
4.277	4.437	100.00%
4.437	4.517	100.00%
4.517	4.955	100.00%
4.955	5.176	100.00%
5.176	5.233	100.00%
5.233	5.285	100.00%
5.285	5.402	100.00%
5.402	5.525	100.00%
5.525	5.778	100.00%
5.778	5.912	100.00%
5.912	6.051	100.00%
6.051	6.148	100.00%
6.148	6.220	100.00%
6.220	6.431	100.00%
6.431	6.696	100.00%
6.696	6.914	100.00%
6.914	7.966	100.00%

Signal #2


3.963	4.349	100.00%
4.349	4.632	100.00%
4.632	4.800	100.00%
4.800	5.015	100.00%
5.015	5.138	100.00%
5.138	5.442	100.00%
5.442	5.825	100.00%
5.825	6.058	100.00%
6.058	6.131	100.00%
6.131	6.180	100.00%
6.180	6.287	100.00%
6.287	6.436	100.00%
6.436	6.653	100.00%
6.653	6.775	100.00%
6.775	6.861	100.00%
6.861	6.984	100.00%
6.984	7.073	100.00%
7.073	7.207	100.00%
7.207	7.530	100.00%
7.530	7.675	100.00%
7.675	8.998	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101519\
Data File : PD055260.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2019 16:21
Operator : SG\AJ
Sample : RESC06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:57:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101519CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 16 04:32:26 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

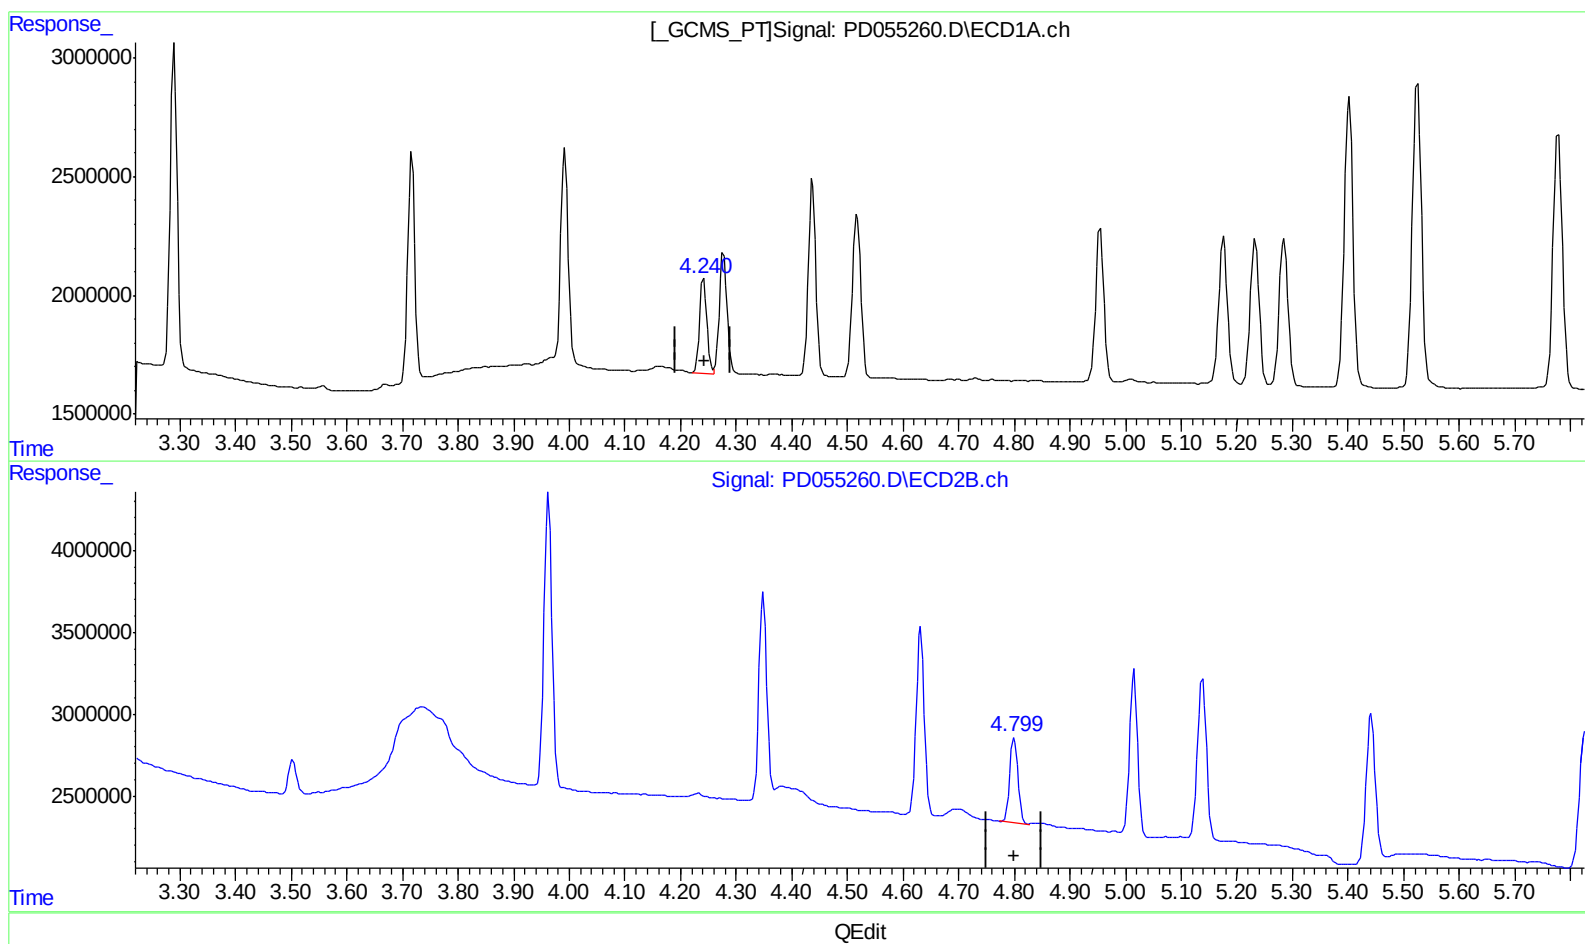

(6) beta-BHC (B)

4.242min 9.226 ng/ml

response 3731574

(6) beta-BHC #2 (B)

4.800min 8.898 ng/ml

response 5384381