

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101520\
 Data File : PD059751.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2020 09:33
 Operator : DD\AJ
 Sample : L4201-13DL 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AP3DL

Manual Integrations
 APPROVED

Ankita
 10/19/2020 10:22:52 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:12:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 02 04:21:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.509	4.024	972534	1122175	0.673	0.565
27) SA Decachlor...	8.310	9.109	3021194	4232888	2.820	2.845m
Target Compounds						
10) B trans-Chl...	5.474	6.140	32801047	66656480	20.193m	29.867m#
11) B cis-Chlor...	5.531	6.215	38373983	53127157	23.700m	24.290
12) B 4,4'-DDE	5.697	6.369	10543697	54828002	6.843	26.216 #
13) MA Dieldrin	5.822	6.512	57882922	33569795	35.293m	15.059 #
14) MA Endrin	6.086	6.730	20481426	47239162	17.338	30.491 #
16) A 4,4'-DDD	6.217	6.864	48544077	164.1E6	37.130	94.768 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101520\
Data File : PD059751.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2020 09:33
Operator : DD\AJ
Sample : L4201-13DL 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:12:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 02 04:21:20 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

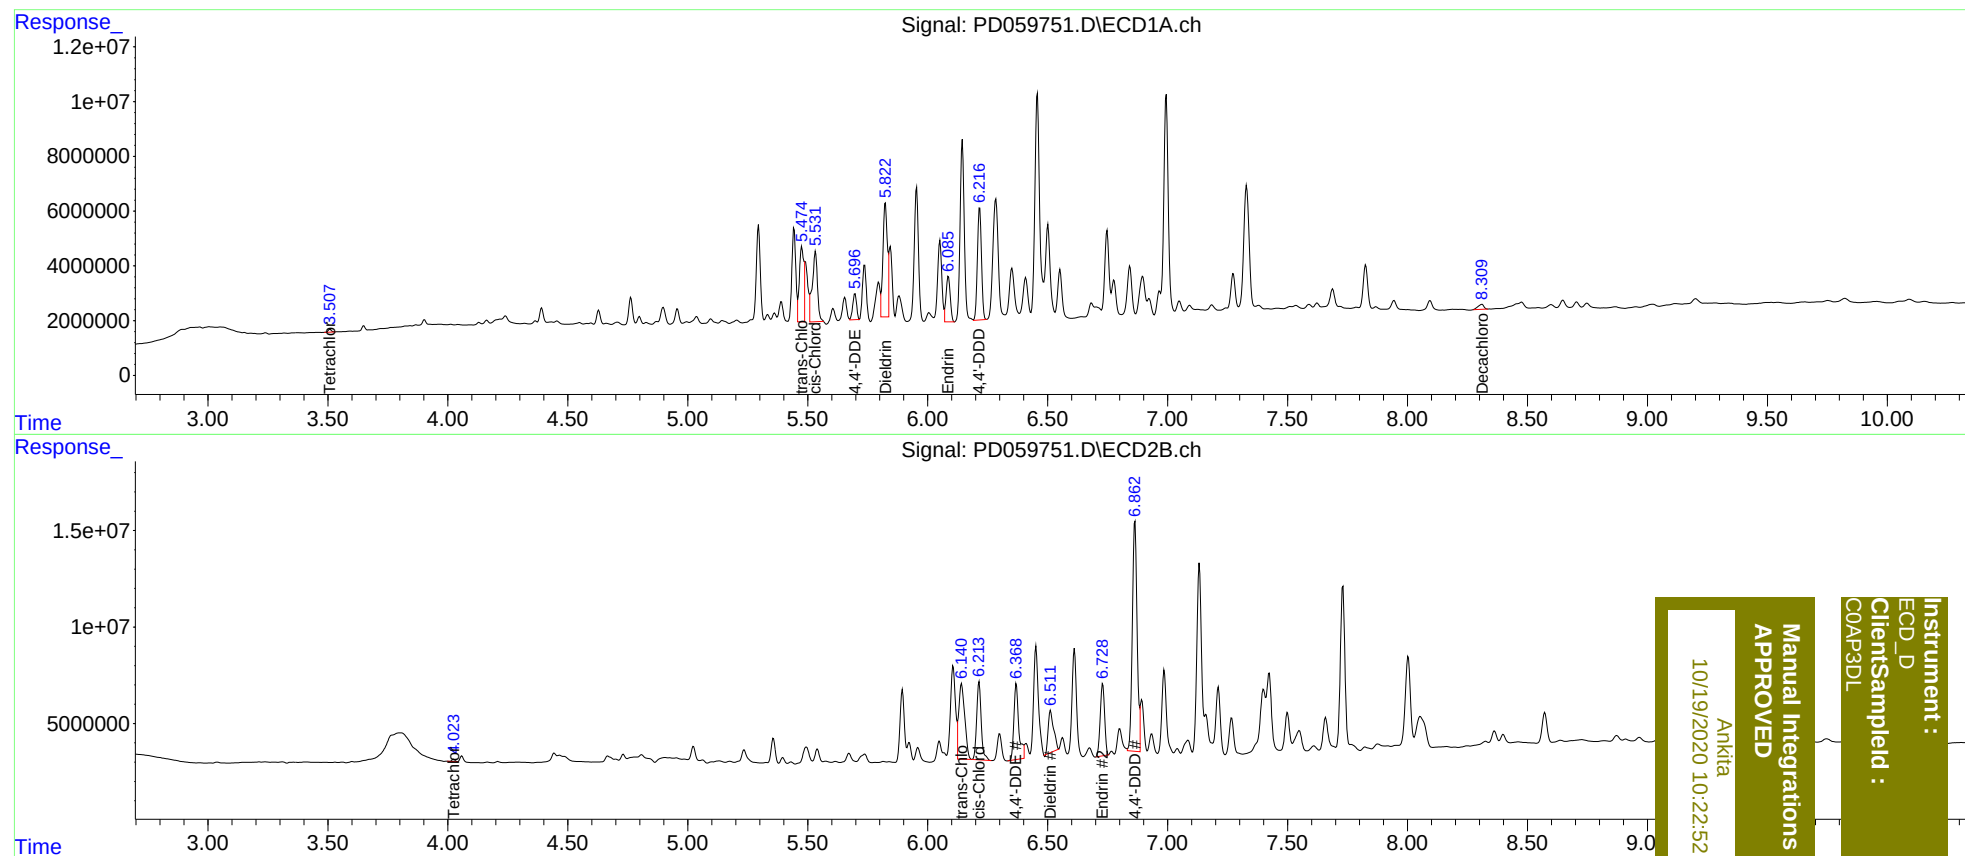

10/19/2020 10:22:52 AM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client Sampled :
COAP3DL