

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101520\
 Data File : PD059791.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2020 21:33
 Operator : DD\AJ
 Sample : L4235-15
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AQ0

Manual Integrations
 APPROVED

Ankita
 10/19/2020 10:23:25 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:29:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 02 04:21:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.508	4.025	6409366	8945117	4.437	4.504
27)	SA Decachlor...	8.308	9.111	11203656	11483179	10.456	7.718m#
Target Compounds							
3)	MA gamma-BHC...	4.241	4.682	7557681	8640411	3.870m	3.256
10)	B trans-Chl...	5.472	6.124	4797403	42642234	2.953m	19.107m#
11)	B cis-Chlor...	5.532	6.215	8511742	11646774	5.257	5.325
12)	B 4,4'-DDE	5.695	6.365	1861985	6581831	1.208m	3.147m#
13)	MA Dieldrin	5.829	6.522	17389780	4043585	10.603	1.814m#
14)	MA Endrin	6.083	6.729	2279475	2430554	1.930	1.569m
16)	A 4,4'-DDD	6.215	6.859	5242887	13540060	4.010	7.821 #
17)	MA 4,4'-DDT	6.457	7.164	3331083	2608686	2.482	1.625 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101520\
Data File : PD059791.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2020 21:33
Operator : DD\AJ
Sample : L4235-15
Misc :
ALS Vial : 42 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:29:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 02 04:21:20 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

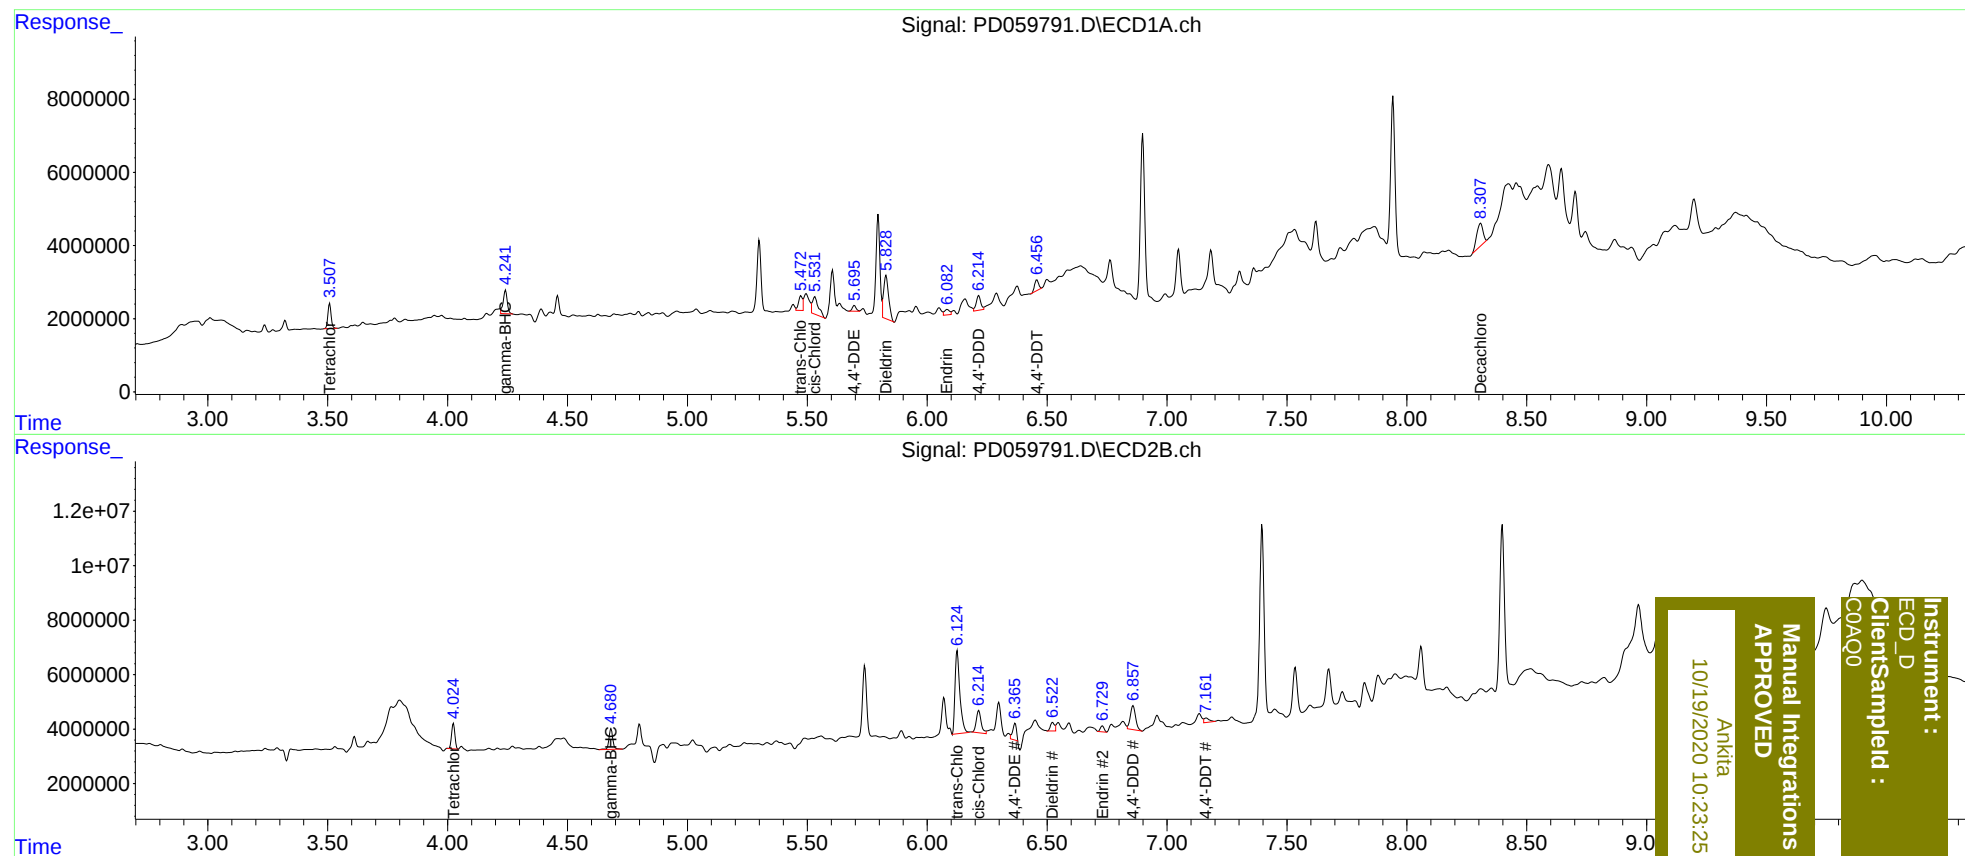

10/19/2020 10:23:25 AM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client Sampled :
COAQ0