

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101520\
Data File : PD059774.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2020 15:24
Operator : DD\AJ
Sample : PB132240BS
Misc :
ALS Vial : 27 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
PLCS40

Manual Integrations
APPROVED

Ankita
10/19/2020 10:23:12 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 05:22:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 02 04:21:20 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

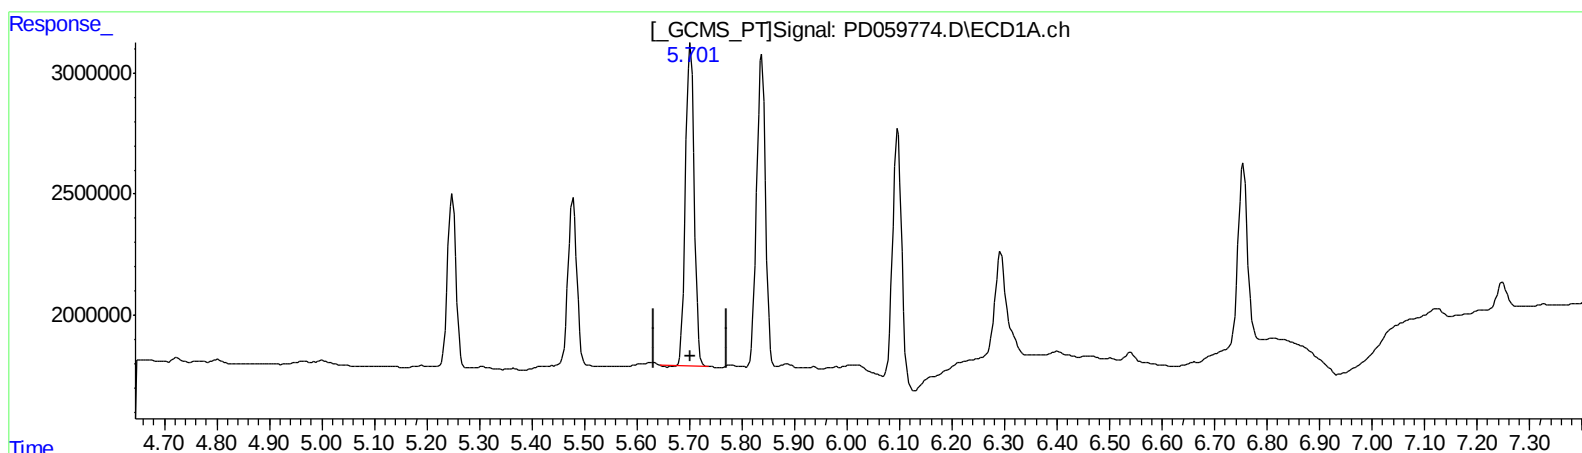

(12) 4,4'-DDE (B)
5.702min 9.830 ng/ml
response 15145444

(12) 4,4'-DDE #2 (B)
6.370min 9.902 ng/ml
response 20709485

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101520\
Data File : PD059774.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2020 15:24
Operator : DD\AJ
Sample : PB132240BS
Misc :
ALS Vial : 27 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
PLCS40

Manual Integrations
APPROVED

Ankita
10/19/2020 10:23:12 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 05:22:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 02 04:21:20 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

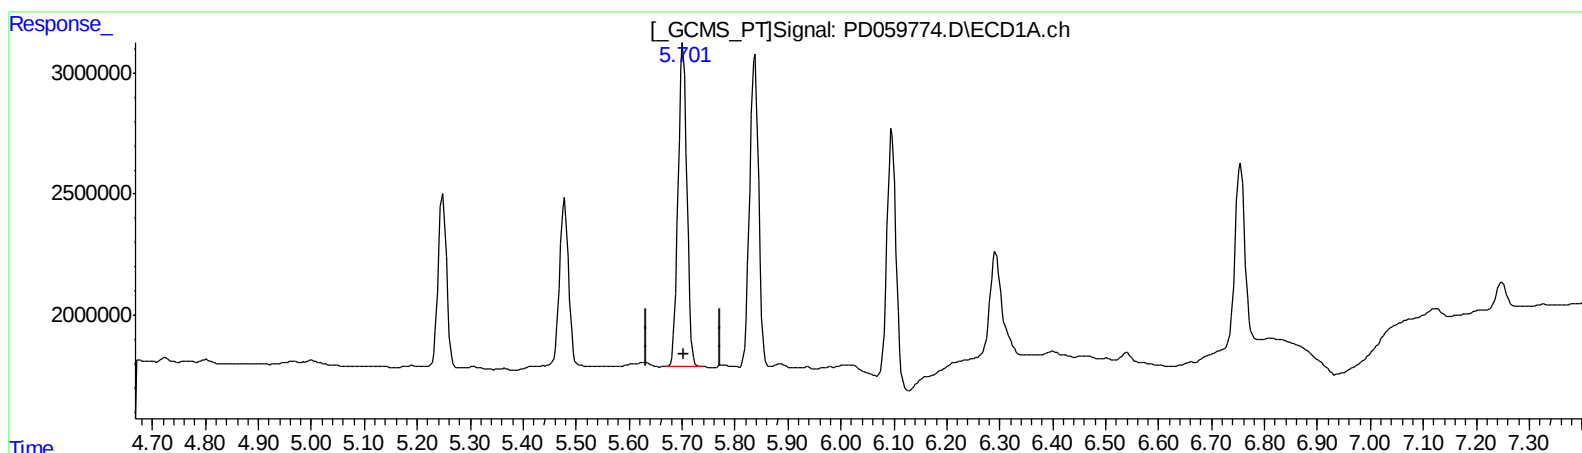

(12) 4,4'-DDE (B)
5.701min 9.947 ng/ml m
response 15325945

(12) 4,4'-DDE #2 (B)
6.370min 9.902 ng/ml
response 20709485

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101520\
 Data File : PD059774.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2020 15:24
 Operator : DD\AJ
 Sample : PB132240BS
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS40

Manual Integrations
 APPROVED

Ankita
 10/19/2020 10:23:12 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 05:22:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 02 04:21:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.513	4.025	24189823	38256957	16.746	19.262
27) SA Decachlor...	8.317	9.114	44231292	54085382	41.280	36.352
Target Compounds						
3) MA gamma-BHC...	4.241	4.701	7628885	13043099	3.906	4.915 #
8) B Heptachlo...	5.248	5.907	7969364	10610742	4.924	4.727
10) B trans-Chl...	5.478	6.141	8125780	11074393	5.002	4.962
12) B 4,4'-DDE	5.701	6.370	15325945	20709485	9.947m	9.902
13) MA Dieldrin	5.838	6.523	15282630	21735299	9.318	9.750
14) MA Endrin	6.097	6.742	13096349	16182395	11.086	10.445
19) B Endosulfa...	6.755	7.296	9649803	12994997	7.718	7.238

AJ
 10/20/20

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.