

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101520\
Data File : PD059782.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2020 17:18
Operator : DD\AJ
Sample : PB132373BS
Misc :
ALS Vial : 35 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
PLCS73

Manual Integrations
APPROVED

Ankita
10/19/2020 10:23:13 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 05:41:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 02 04:21:20 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

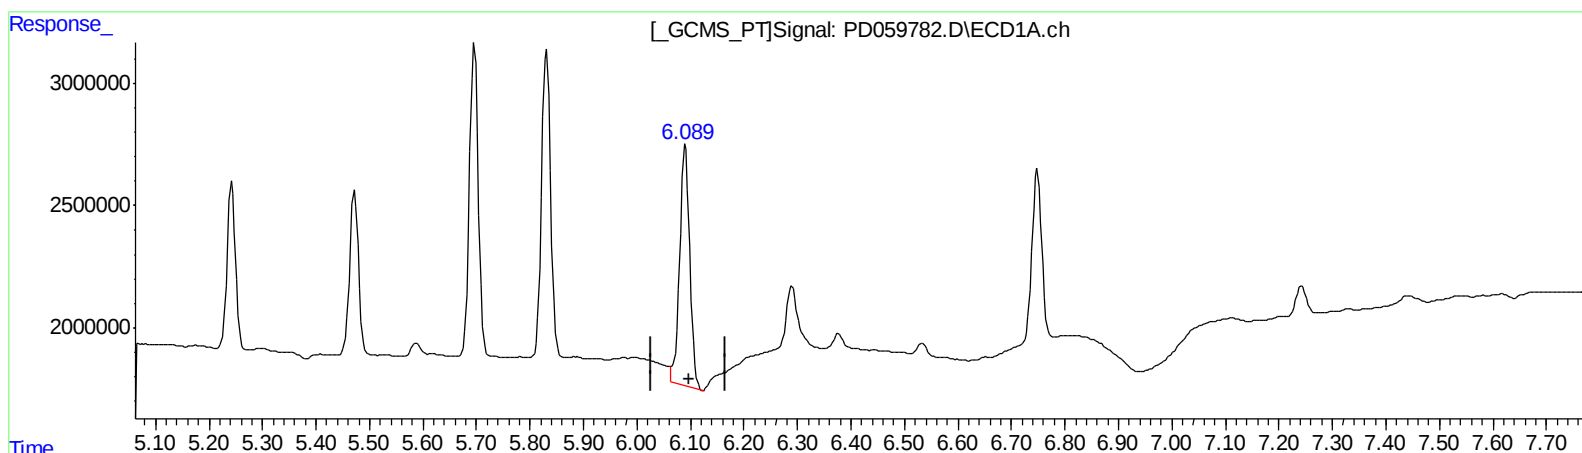

(14) Endrin (MA)
6.090min 10.943 ng/ml
response 12926544

(14) Endrin #2 (MA)
6.740min 9.628 ng/ml
response 14916115

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101520\
Data File : PD059782.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2020 17:18
Operator : DD\AJ
Sample : PB132373BS
Misc :
ALS Vial : 35 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
PLCS73

Manual Integrations
APPROVED

Ankita
10/19/2020 10:23:13 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 05:41:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 02 04:21:20 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

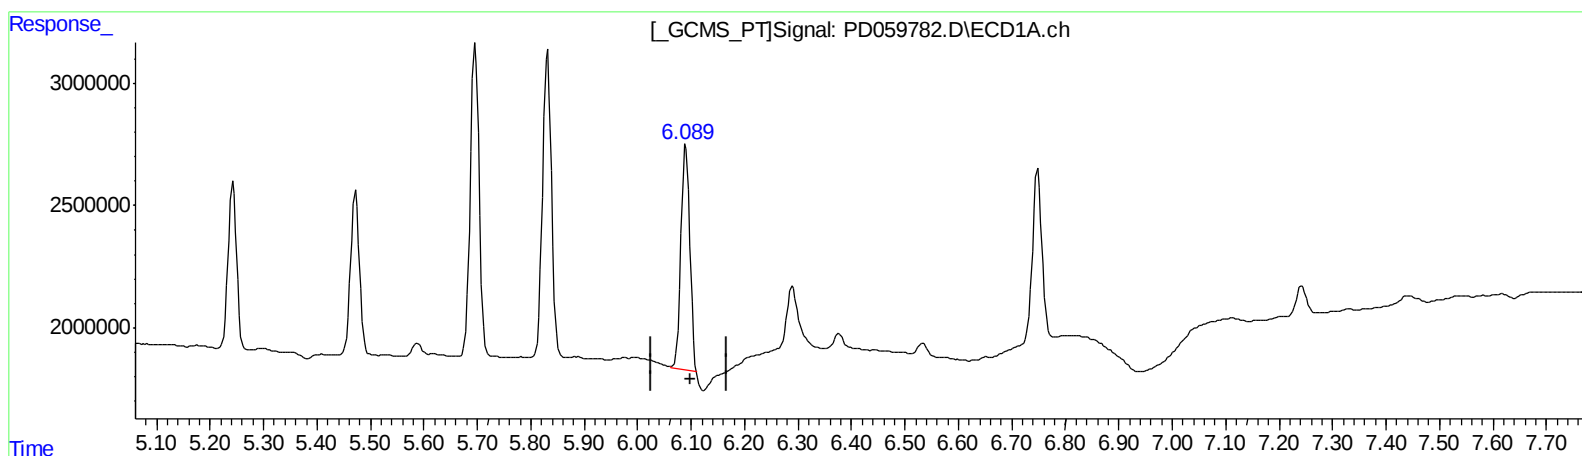

(14) Endrin (MA)
6.089min 9.181 ng/ml m
response 10845105

(14) Endrin #2 (MA)
6.740min 9.628 ng/ml
response 14916115

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101520\
 Data File : PD059782.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2020 17:18
 Operator : DD\AJ
 Sample : PB132373BS
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS73

Manual Integrations
 APPROVED

Ankita
 10/19/2020 10:23:13 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 05:41:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 02 04:21:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.508	4.025	23625955	37513631	16.356	18.887
27) SA Decachlor...	8.310	9.113	43123501	52895578	40.247	35.553
Target Compounds						
3) MA gamma-BHC...	4.236	4.702	7422022	10490715	3.800	3.953
8) B Heptachlo...	5.243	5.907	7642977	10573164	4.722	4.710
10) B trans-Chl...	5.472	6.141	7787639	10678656	4.794	4.785
12) B 4,4'-DDE	5.696	6.369	14717244	19645463	9.552	9.394
13) MA Dieldrin	5.831	6.522	14848696	20552314	9.054	9.219
14) MA Endrin	6.089	6.740	10845105	14916115	9.181m	9.628
19) B Endosulfa...	6.749	7.296	8855268	12090899	7.083	6.735

AJ
 10/20/20

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.