

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101520\
 Data File : PD059750.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2020 09:19
 Operator : DD\AJ
 Sample : L4201-11DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AL9DL

Manual Integrations
 APPROVED

Ankita
 10/19/2020 10:22:51 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:11:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 02 04:21:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.514	4.025	3149840	3983217	2.181	2.005
27)	SA Decachlor...	8.317	9.112	6465404	12346636	6.034m	8.299m#
Target Compounds							
8)	B Heptachlo...	5.246	5.894	2349141	17694663	1.451m	7.883 #
10)	B trans-Chl...	5.480	6.140	39344188	75441916	24.221m	33.803m#
11)	B cis-Chlor...	5.540	6.216	42247241	78842932	26.093	36.047 #
12)	B 4,4'-DDE	5.705	6.371	15559142	30587536	10.098	14.626 #
13)	MA Dieldrin	5.833	6.522	22007882	12134028	13.419m	5.443m#
14)	MA Endrin	6.097	6.732	5401243	8678345	4.572	5.602
16)	A 4,4'-DDD	6.225	6.862	26882949	56745957	20.562	32.778 #
17)	MA 4,4'-DDT	6.468	7.161	80369995	105.7E6	59.891	65.844

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101520\
Data File : PD059750.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2020 09:19
Operator : DD\AJ
Sample : L4201-11DL 5X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:11:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 02 04:21:20 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

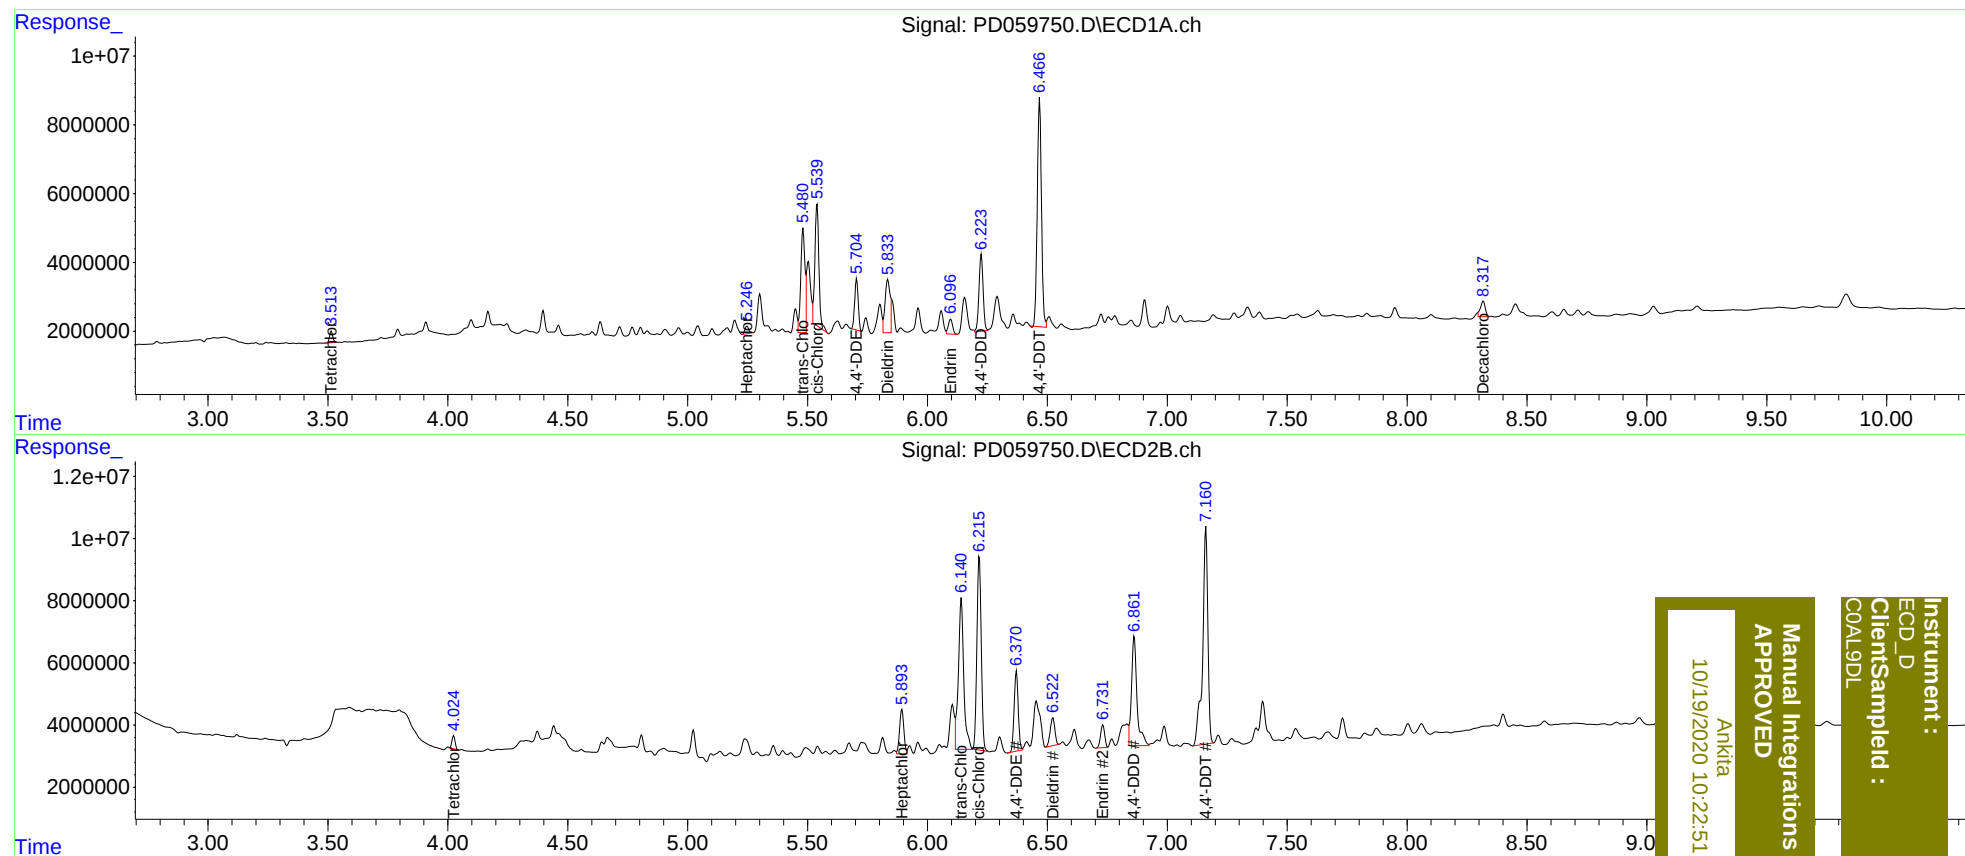

10/19/2020 10:22:51 AM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client Sampled :
COAL9DL