

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101520\
 Data File : PD059776.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2020 15:53
 Operator : DD\AJ
 Sample : L4235-12
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COANO

Manual Integrations
 APPROVED

Ankita
 10/19/2020 1:53:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 05:50:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 02 04:21:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.508	4.024	21333687	33513700	14.769	16.873
27)	SA Decachlor...	8.310	9.111	33304313	41405030	31.082	27.830
Target Compounds							
8)	B Heptachlo...	5.237	5.892	830092	2618736	0.513m	1.167 #
10)	B trans-Chl...	5.488	6.146	5136030	12039060	3.162m	5.394 #
11)	B cis-Chlor...	5.529	6.214	1653346	1453956	1.021m	0.665 #
12)	B 4,4'-DDE	5.696	6.369	1640606	3640269	1.065	1.741 #
14)	MA Endrin	6.084	6.729	1048145	1067049	0.887m	0.689

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101520\
Data File : PD059776.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2020 15:53
Operator : DD\AJ
Sample : L4235-12
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 05:50:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 02 04:21:20 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

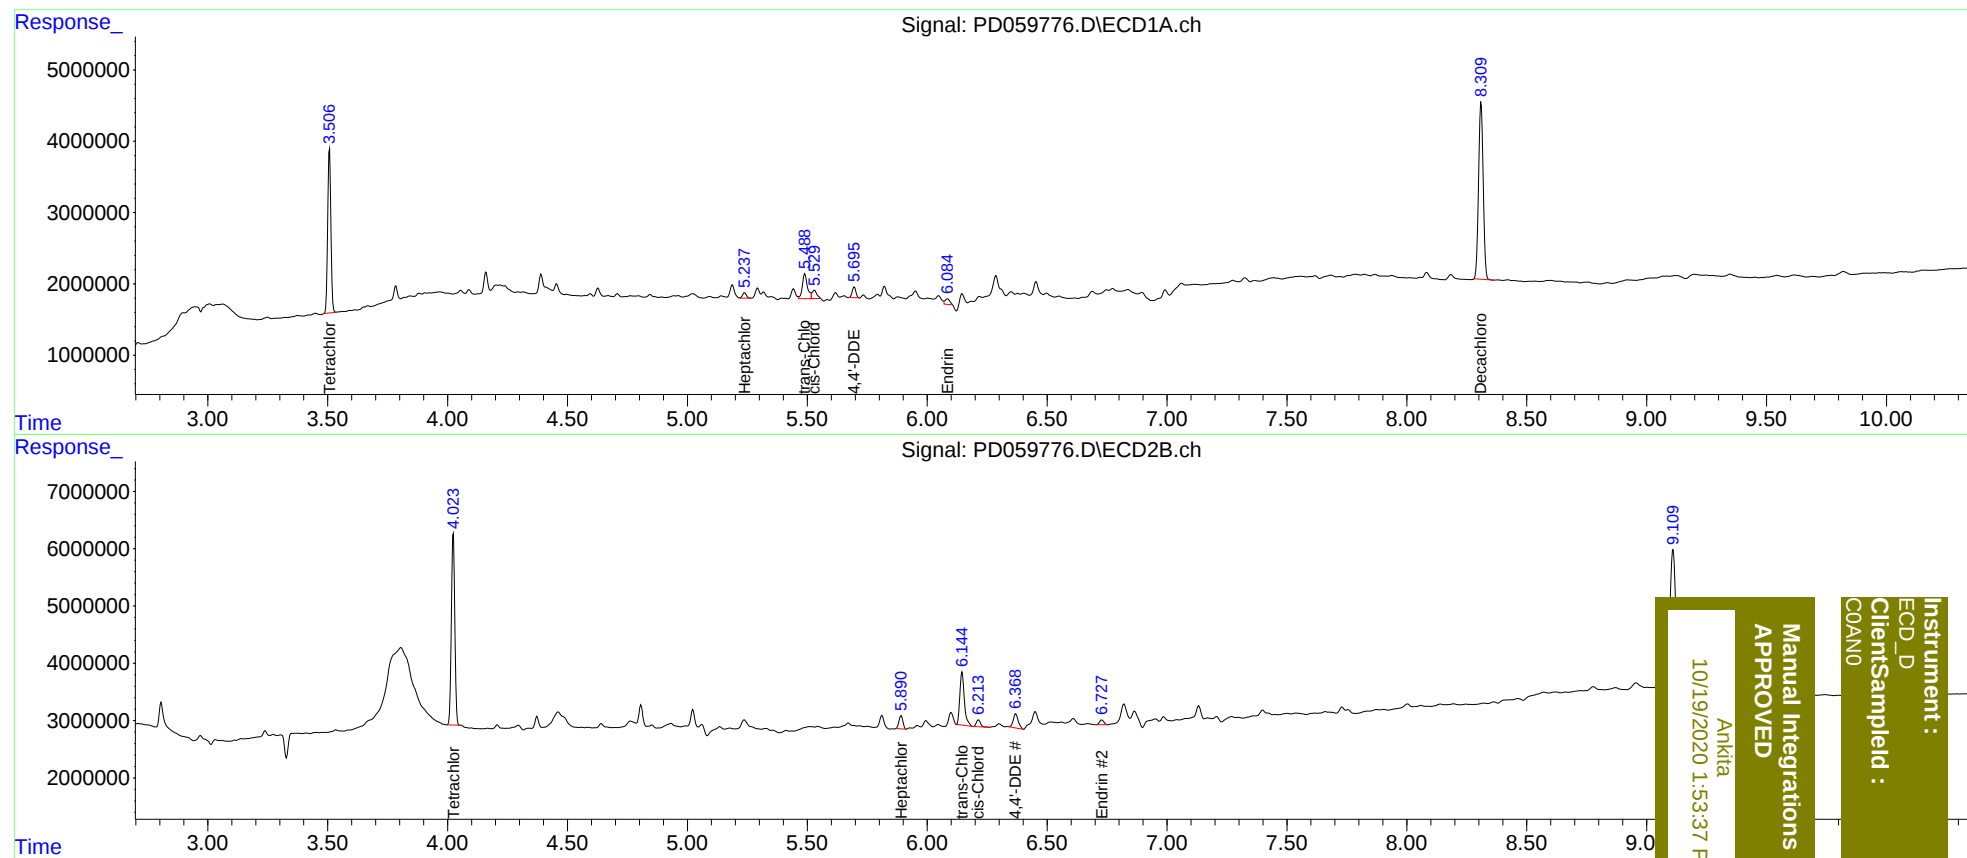

10/19/2020 1:53:37 PM
Ankita

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
COANO