

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101521\
 Data File : PD066260.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2021 13:59
 Operator : AR\AJ
 Sample : M4030-03MSD
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C00Q5MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 10:18:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101321CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 13 06:25:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.971	33323449	120.3E6	17.501	17.817
2)	SA Decachlor...	8.167	9.019	49771673	189.0E6	24.605	38.961 #
Target Compounds							
2)	A alpha-BHC	3.878	4.364	153.2E6	467.3E6	51.644	43.916
3)	MA gamma-BHC...	4.159	4.648	148.4E6	444.4E6	48.852	45.725
4)	MA Heptachlor	4.453	5.148	145.7E6	410.8E6	58.841	45.471
5)	MB Aldrin	4.699	5.452	136.5E6	413.8E6	47.507	43.348
6)	B beta-BHC	4.407	4.824	59144695	192.4E6	37.785	41.851
7)	B delta-BHC	4.609	5.040	142.8E6	428.0E6	54.150	40.999
8)	B Heptachlo...	5.140	5.840	131.6E6	387.2E6	51.535	54.102
9)	A Endosulfan I	5.476	6.197	119.9E6	378.9E6	51.698	41.964
10)	B trans-Chl...	5.364	6.073	131.8E6	400.0E6	50.332	40.796
11)	B cis-Chlor...	5.422	6.145	127.6E6	394.8E6	49.247	41.040
12)	B 4,4'-DDE	5.586	6.305	265.8E6	752.7E6	111.679	79.990 #
13)	MA Dieldrin	5.718	6.454	279.2E6	810.2E6	108.633	85.290
14)	MA Endrin	5.975	6.672	238.6E6	571.9E6	121.919	71.973 #
15)	B Endosulfa...	6.247	6.886	224.7E6	679.7E6	100.236	82.336
16)	A 4,4'-DDD	6.100	6.798	216.1E6	656.0E6	108.180	87.055
17)	MA 4,4'-DDT	6.339	7.095	217.7E6	683.1E6	122.529	89.989 #
18)	B Endrin al...	6.416	7.011	180.1E6	570.5E6	113.259	97.877
19)	B Endosulfa...	6.627	7.233	204.9E6	659.6E6	101.030	86.883
20)	A Methoxychlor	6.886	7.555	564.5E6	1512.8E6	546.615	446.557
21)	B Endrin ke...	7.119	7.705	254.8E6	729.5E6	99.833	91.490

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101521\
Data File : PD066260.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2021 13:59
Operator : AR\AJ
Sample : M4030-03MSD
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 10:18:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101321CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 13 06:25:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

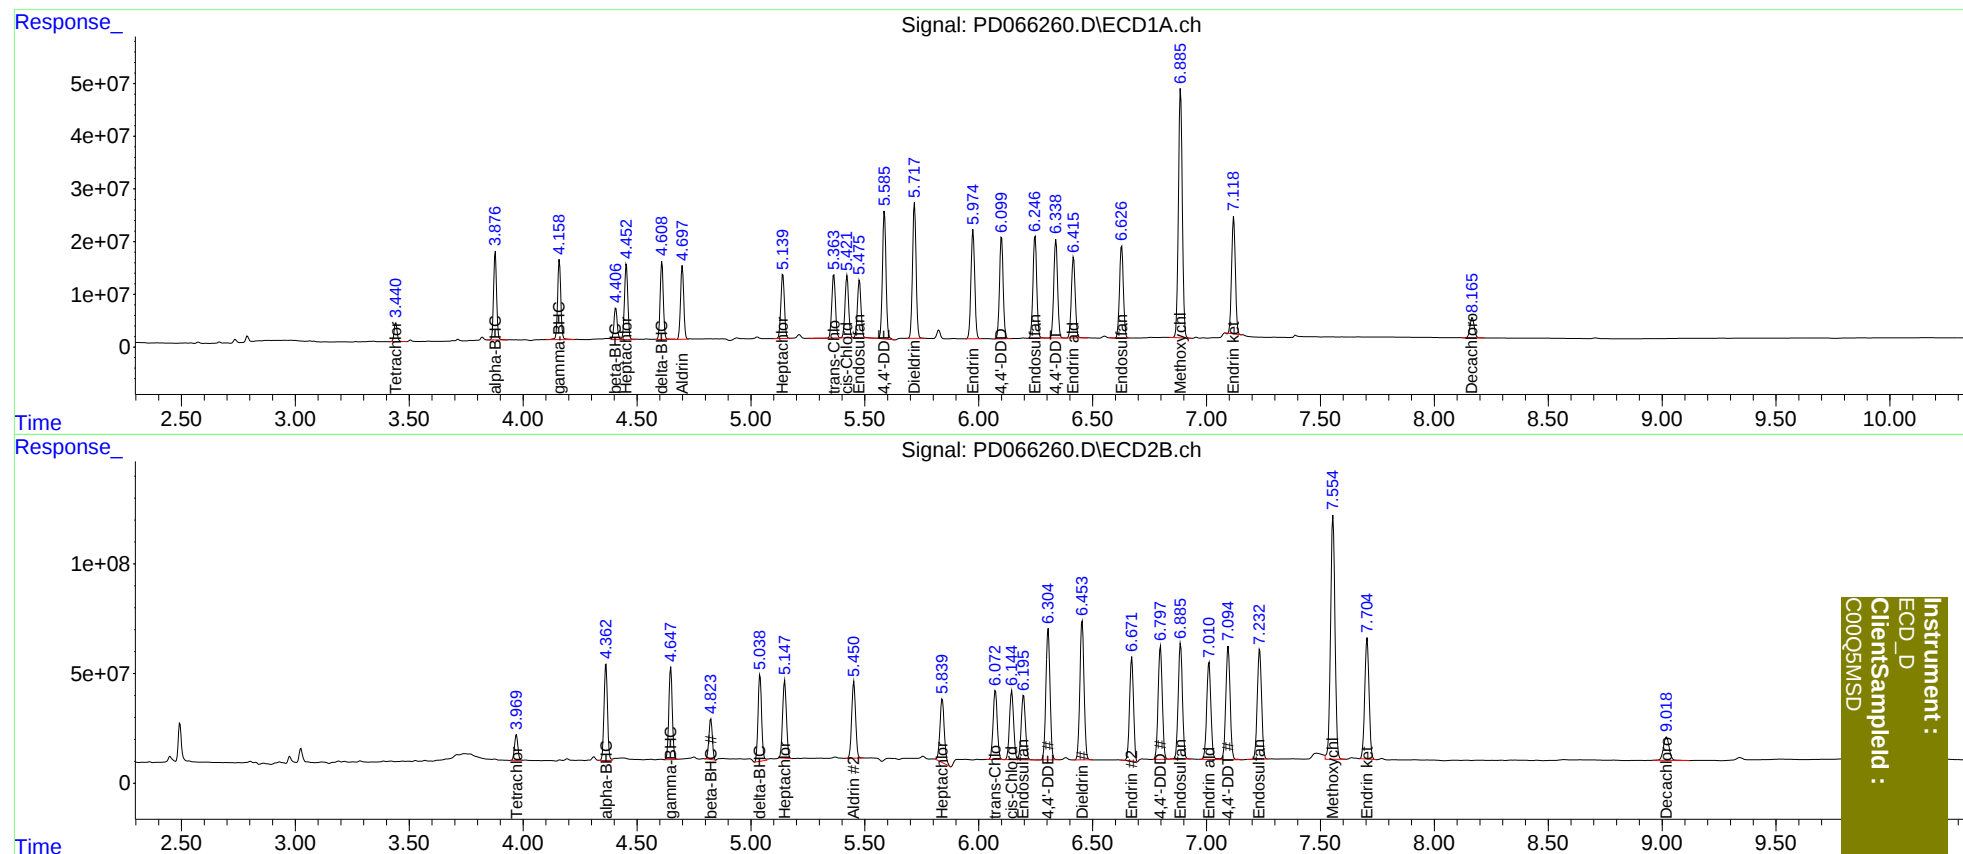

Instrument :
ECD_D
ClientSample :
C0009MSD