

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101521\
 Data File : PD066259.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2021 13:46
 Operator : AR\AJ
 Sample : M4030-02MS
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C00Q5MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 10:18:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101321CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 13 06:25:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.970	35490629	127.0E6	18.639	18.797
27)	SA Decachlor...	8.167	9.020	53096052	195.4E6	26.248	40.274 #
Target Compounds							
2)	A alpha-BHC	3.878	4.363	156.2E6	475.6E6	52.663	44.702
3)	MA gamma-BHC...	4.159	4.648	150.6E6	453.3E6	49.566	46.642
4)	MA Heptachlor	4.454	5.148	149.9E6	415.1E6	60.543	45.946
5)	MB Aldrin	4.699	5.451	138.2E6	419.5E6	48.122	43.948
6)	B beta-BHC	4.407	4.824	60349053	195.2E6	38.554	42.462
7)	B delta-BHC	4.610	5.039	145.9E6	409.9E6	55.301	39.266 #
8)	B Heptachlo...	5.140	5.839	133.8E6	354.4E6	52.402	49.519
9)	A Endosulfan I	5.476	6.196	121.5E6	383.9E6	52.410	42.520
10)	B trans-Chl...	5.364	6.073	135.5E6	405.0E6	51.723	41.311
11)	B cis-Chlor...	5.422	6.145	129.9E6	401.2E6	50.138	41.704
12)	B 4,4'-DDE	5.586	6.304	268.8E6	760.5E6	112.938	80.819 #
13)	MA Dieldrin	5.718	6.454	283.8E6	820.4E6	110.454	86.369
14)	MA Endrin	5.975	6.672	242.5E6	596.4E6	123.910	75.056 #
15)	B Endosulfa...	6.248	6.885	228.8E6	688.2E6	102.077	83.357
16)	A 4,4'-DDD	6.100	6.797	219.8E6	664.0E6	110.028	88.125
17)	MA 4,4'-DDT	6.339	7.094	221.7E6	688.9E6	124.776	90.751 #
18)	B Endrin al...	6.416	7.010	184.0E6	575.5E6	115.708	98.724
19)	B Endosulfa...	6.628	7.233	210.7E6	665.7E6	103.878	87.678
20)	A Methoxychlor	6.886	7.555	571.2E6	1515.7E6	553.122	447.422
21)	B Endrin ke...	7.119	7.705	260.0E6	734.7E6	101.866	92.146

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101521\
Data File : PD066259.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2021 13:46
Operator : AR\AJ
Sample : M4030-02MS
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 10:18:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101321CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 13 06:25:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

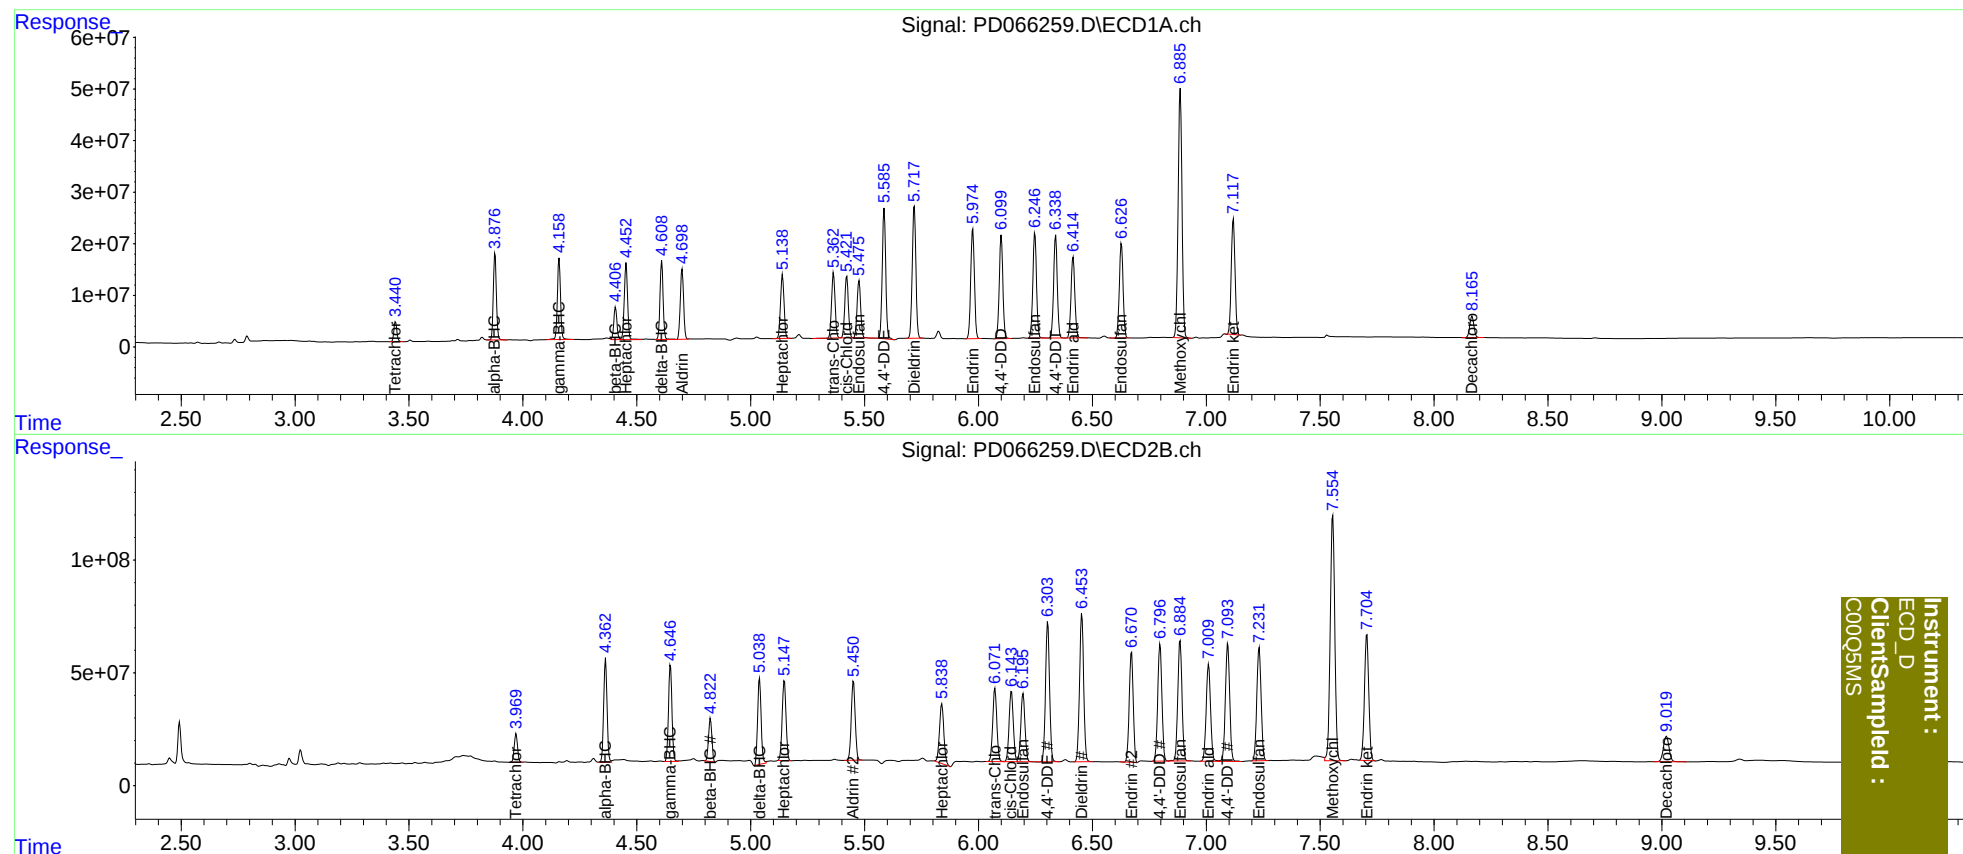

Instrument :
ECD_D
ClientSample :
C00095MS