

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101521\
 Data File : PD066262.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2021 14:27
 Operator : AR\AJ
 Sample : M4030-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C00U0

Manual Integrations
 APPROVED

mohammad
 10/15/2021 4:02:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 10:19:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101321CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 13 06:25:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.971	23314447	81015164	12.244	11.995
27)	SA Decachlor...	8.167	9.020	26210188	123.7E6	12.957	25.496 #
Target Compounds							
3)	MA gamma-BHC...	4.163	4.631	2382240	5771929	0.784m	0.594
14)	MA Endrin	5.968	6.665	2421597	4834777	1.237	0.608 #
16)	A 4,4'-DDD	6.105	6.797	917120	48840210	0.459	6.482m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101521\
Data File : PD066262.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2021 14:27
Operator : AR\AJ
Sample : M4030-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 10:19:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101321CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 13 06:25:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

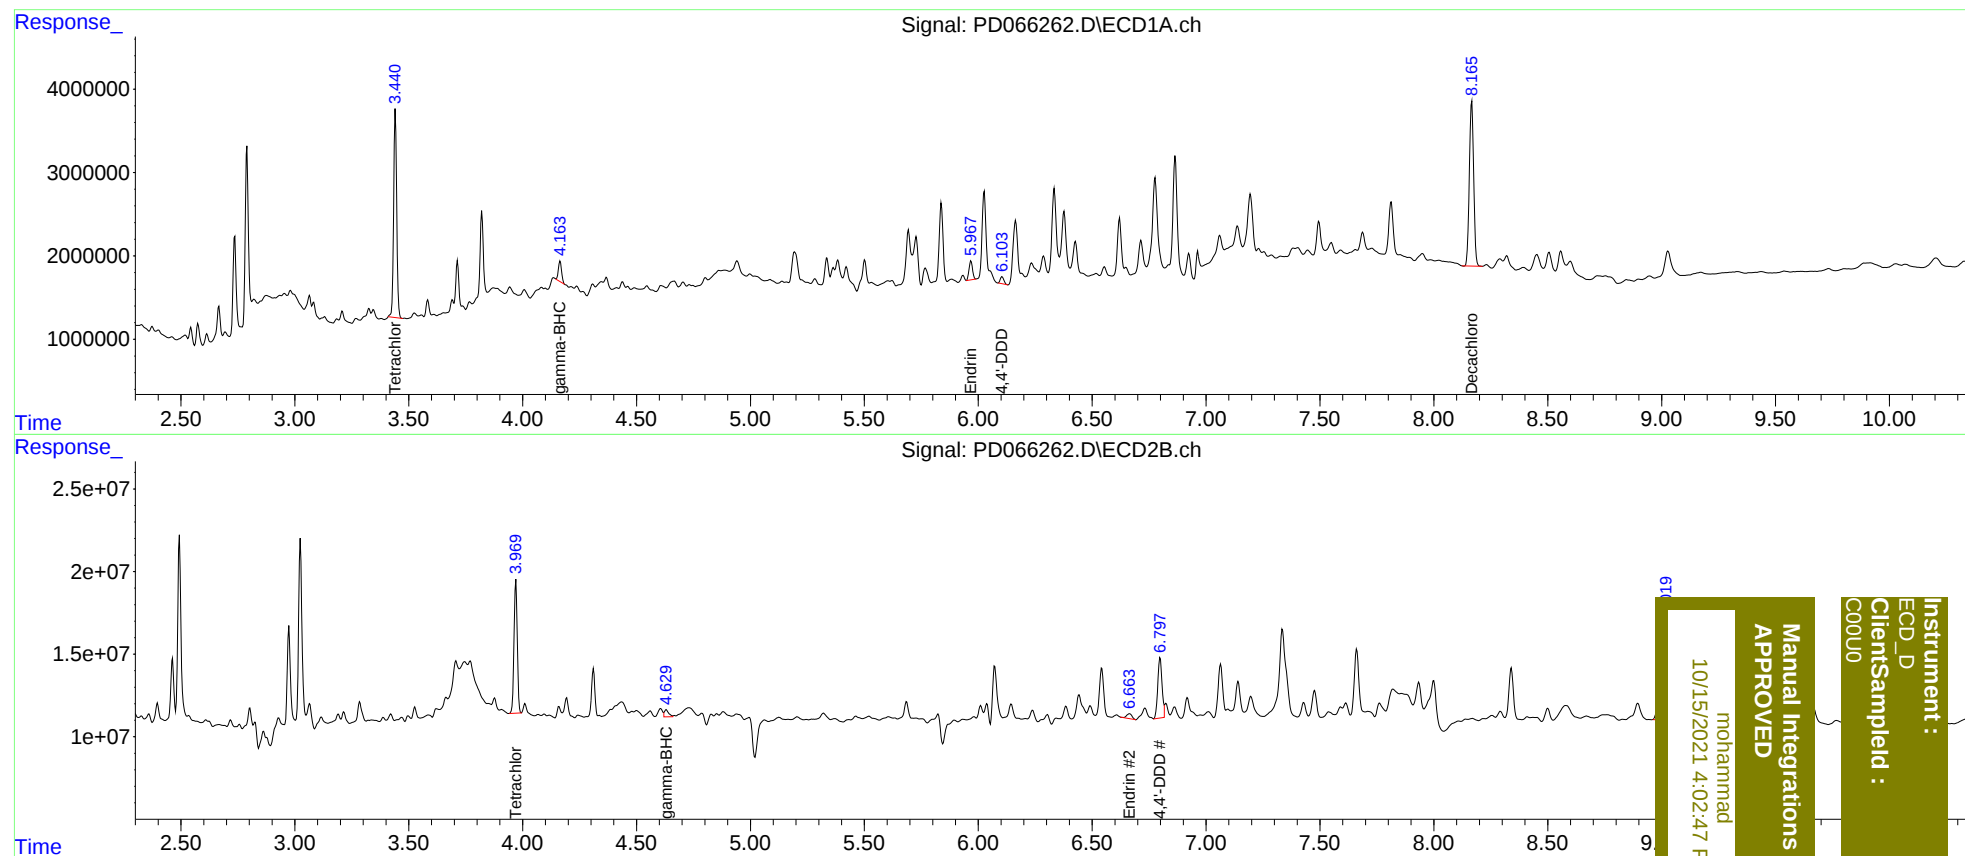

Manual Integrations
APPROVED

10/15/2021 4:02:47 PM
mohammad

Instrument :
ECD_D
ClientSampled :
C00U0