

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101523\
 Data File : PD078859.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2023 13:40
 Operator : AR\AJ
 Sample : TOXAPH201
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 16:04:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101523CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 13 15:57:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.807	18512008	26589169	9.815	10.289
27)	SA Decachlor...	9.122	7.963	36231998	48824393	19.320	20.848
Target Compounds							
22)	Toxaphene-1	5.892	5.370	7042097	15989344	1037.055	1024.377
23)	Toxaphene-2	6.482	5.730	19548253	15449101	999.782	978.832
24)	Toxaphene-3	6.682	6.011	14146196	17997925	1002.554	998.314
25)	Toxaphene-4	7.194	6.770	41194706	66771086	979.477	969.609
26)	Toxaphene-5	7.614	7.087	31098159	28945259	963.104	942.434

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101523\
Data File : PD078859.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2023 13:40
Operator : AR\AJ
Sample : TOXAPH201
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 16:04:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101523CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 13 15:57:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

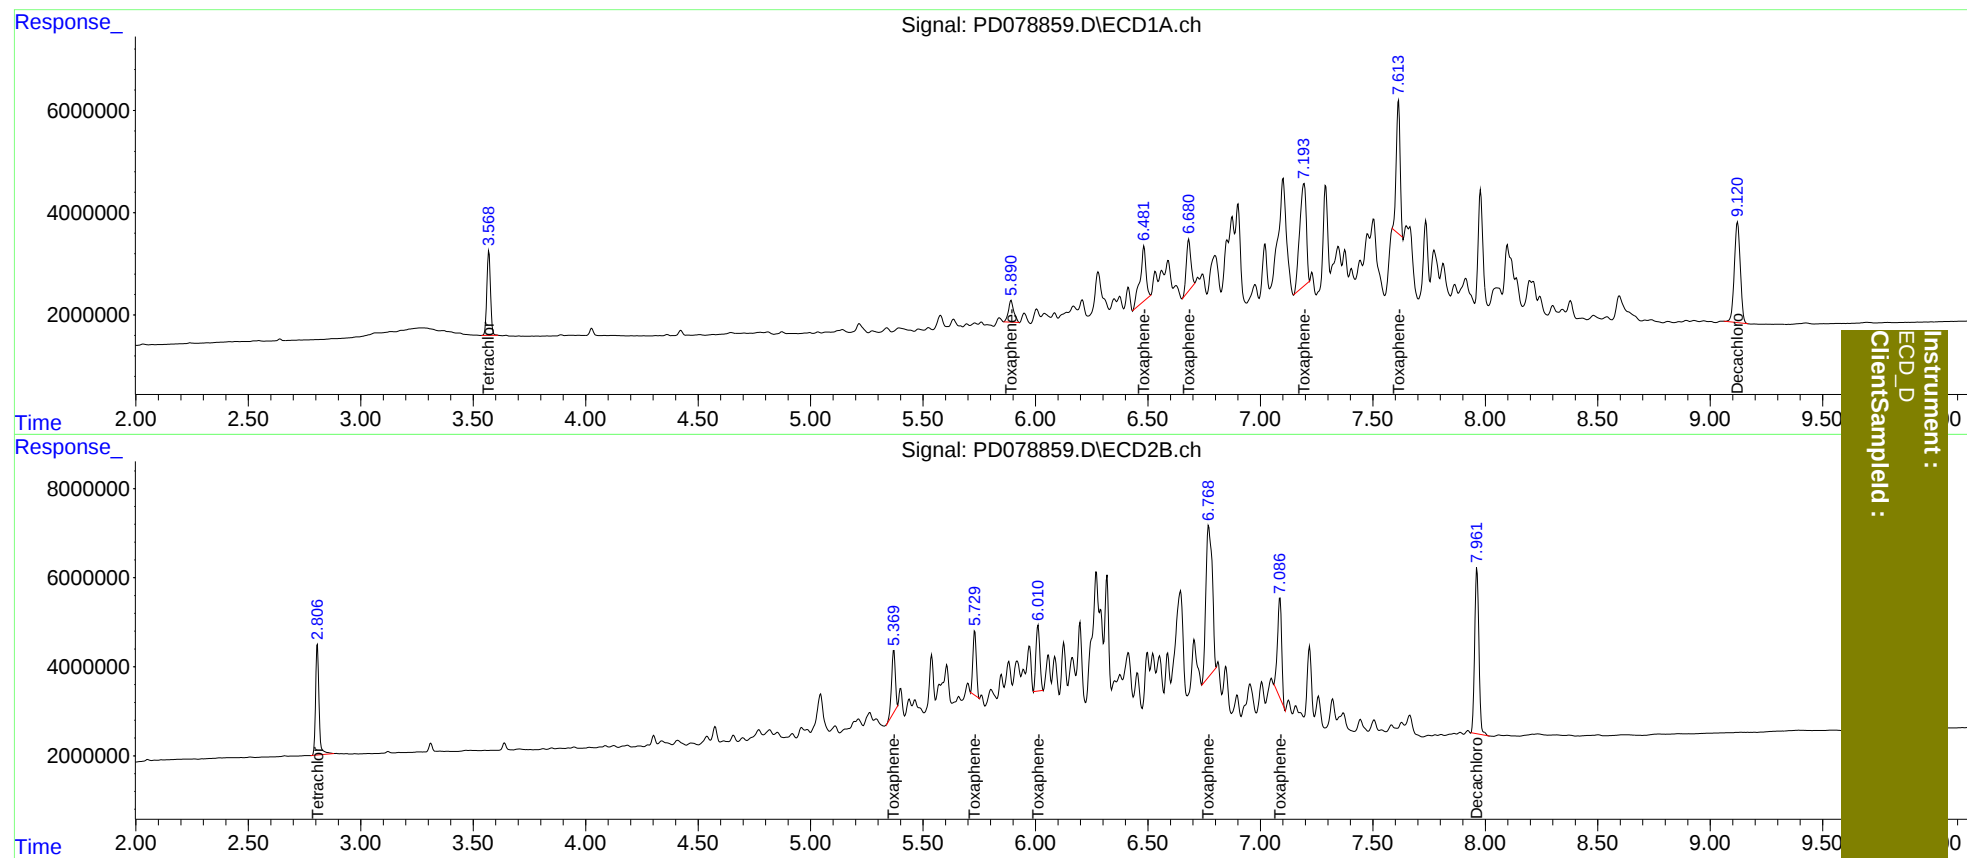

Instrument :
ECD_D
ClientSampled :
0