

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101523\
 Data File : PD078861.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2023 14:07
 Operator : AR\AJ
 Sample : TOXAPH401
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 16:02:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101523CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 13 15:57:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.808	78474861	102.0E6	41.355	39.872
27)	SA Decachlor...	9.120	7.963	151.9E6	185.9E6	80.091	80.520
Target Compounds							
22)	Toxaphene-1	5.892	5.371	26540840	61987161	3957.418	4003.815
23)	Toxaphene-2	6.482	5.731	78526058	64093071	4015.869	4032.386
24)	Toxaphene-3	6.682	6.012	56827524	72085018	4030.848	3996.184
25)	Toxaphene-4	7.193	6.770	169.7E6	277.7E6	4007.468	3992.462
26)	Toxaphene-5	7.614	7.087	130.0E6	125.8E6	3977.583	4019.709

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101523\
Data File : PD078861.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2023 14:07
Operator : AR\AJ
Sample : TOXAPH401
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 16:02:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101523CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 13 15:57:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

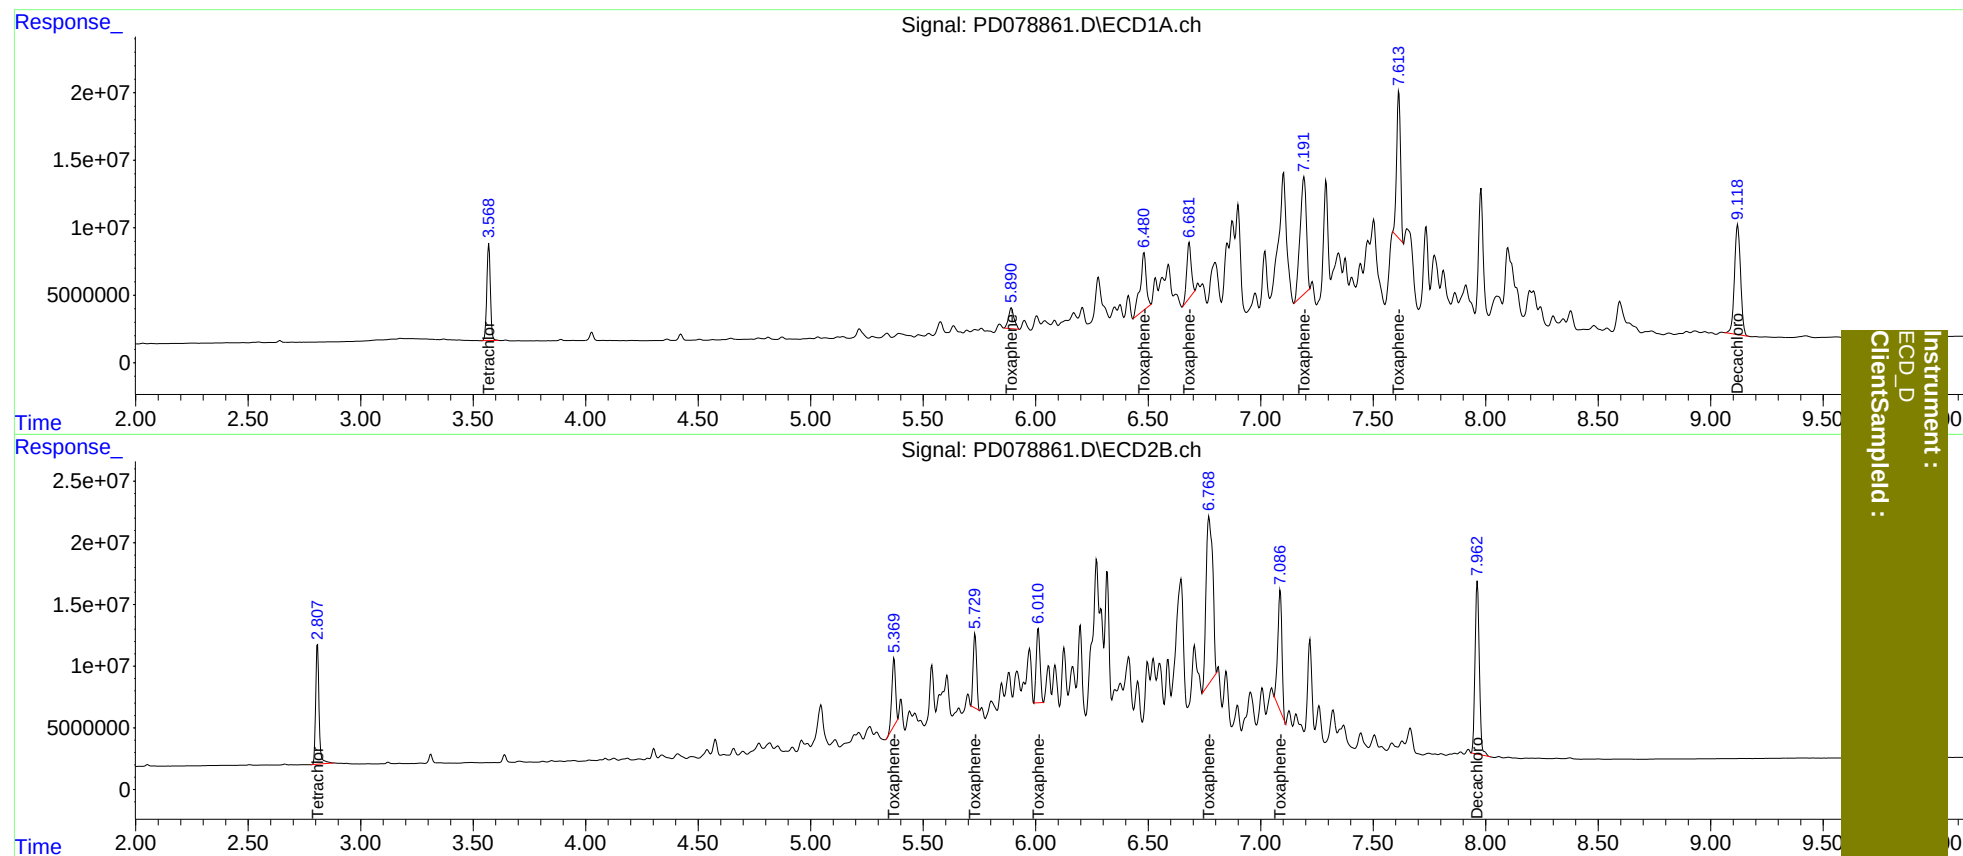

Instrument :
ECD_D
ClientSampled :
0