

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101524\
 Data File : PD086066.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 18:41
 Operator : AR\AJ
 Sample : P4349-22MSD
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EOAG2MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/16/2024
 Supervised By : Ankita Jodhani 10/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:46:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 09 17:21:49 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	2.877	24735477	127.8E6	21.625	20.573
27)	SA Decachlor...	8.901	8.058	39941692	124.8E6	20.710	25.662m
Target Compounds							
2)	A alpha-BHC	3.887	3.387	122.7E6	494.6E6	61.225	53.594
3)	MA gamma-BHC...	4.214	3.721	119.8E6	465.7E6	60.081	54.037
4)	MA Heptachlor	4.807	4.073	119.1E6	442.7E6	61.757	60.211
5)	MB Aldrin	5.146	4.357	121.4E6	451.1E6	50.438	46.642m
6)	B beta-BHC	4.400	4.016	46826276	192.1E6	44.445	42.586
7)	B delta-BHC	4.644	4.252	118.7E6	450.0E6	53.945m	48.571
8)	B Heptachlo...	5.565	4.861	110.3E6	390.6E6	49.511	44.835
9)	A Endosulfan I	5.947	5.235	104.4E6	347.9E6	57.242	50.187
10)	B trans-Chl...	5.820	5.113	109.0E6	418.5E6	48.519	46.517
11)	B cis-Chlor...	5.901	5.177	110.7E6	413.0E6	48.517	46.008
12)	B 4,4'-DDE	6.072	5.360	203.3E6	745.9E6	106.612	99.236m
13)	MA Dieldrin	6.219	5.499	234.6E6	792.6E6	119.212	107.069m
14)	MA Endrin	6.445	5.778	200.6E6	714.6E6	129.863	121.166
15)	B Endosulfa...	6.657	6.070	196.0E6	667.4E6	98.709	95.436
16)	A 4,4'-DDD	6.581	5.917	159.7E6	591.9E6	128.036	124.055
17)	MA 4,4'-DDT	6.895	6.171	173.3E6	638.5E6	128.420	128.192
18)	B Endrin al...	6.786	6.248	148.6E6	500.2E6	96.894	96.561
19)	B Endosulfa...	7.021	6.473	188.5E6	601.3E6	102.937	99.264
20)	A Methoxychlor	7.369	6.742	474.2E6	1326.8E6	593.093	632.879
21)	B Endrin ke...	7.497	6.982	207.4E6	711.3E6	101.996m	97.663

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101524\
Data File : PD086066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 18:41
Operator : AR\AJ
Sample : P4349-22MSD
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:46:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 09 17:21:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

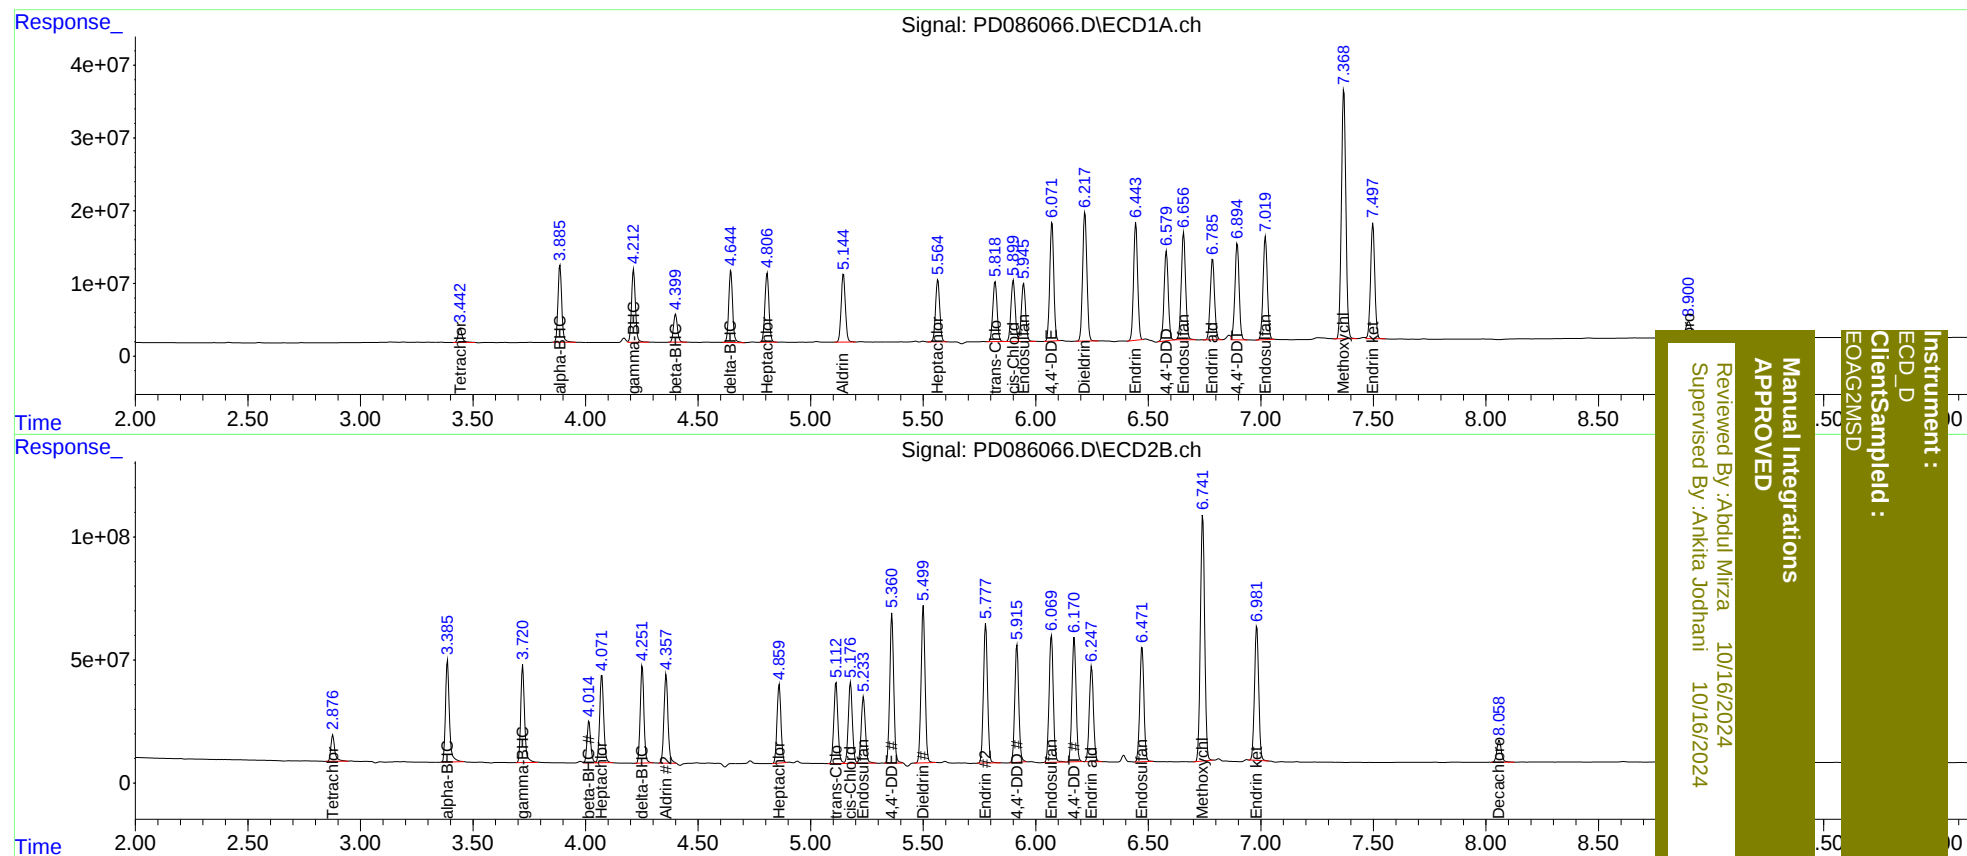

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/16/2024
Supervised By: Ankita Jodhani 10/16/2024

Instrument :
ECD_D
Client Sampled :
EOAG2MSD