

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101524\
 Data File : PD086048.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 13:43
 Operator : AR\AJ
 Sample : P4349-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EOAG9

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/18/2024
 Supervised By : Ankita Jodhani 10/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:41:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 09 17:21:49 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	2.877	27357953	136.9E6	23.917m	22.042
27)	SA Decachlor...	8.900	8.058	37716247	111.6E6	19.556	22.950
Target Compounds							
10)	B trans-Chl...	5.819	5.111	569217	3650213	0.253m	0.406m#
11)	B cis-Chlor...	5.904	5.172	2342217	4131346	1.027m	0.460m#
12)	B 4,4'-DDE	6.070	5.358	1055468	9175450	0.554m	1.221m#
16)	A 4,4'-DDD	6.578	5.915	462954	4467848	0.371m	0.936m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101524\
Data File : PD086048.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 13:43
Operator : AR\AJ
Sample : P4349-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:41:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 09 17:21:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

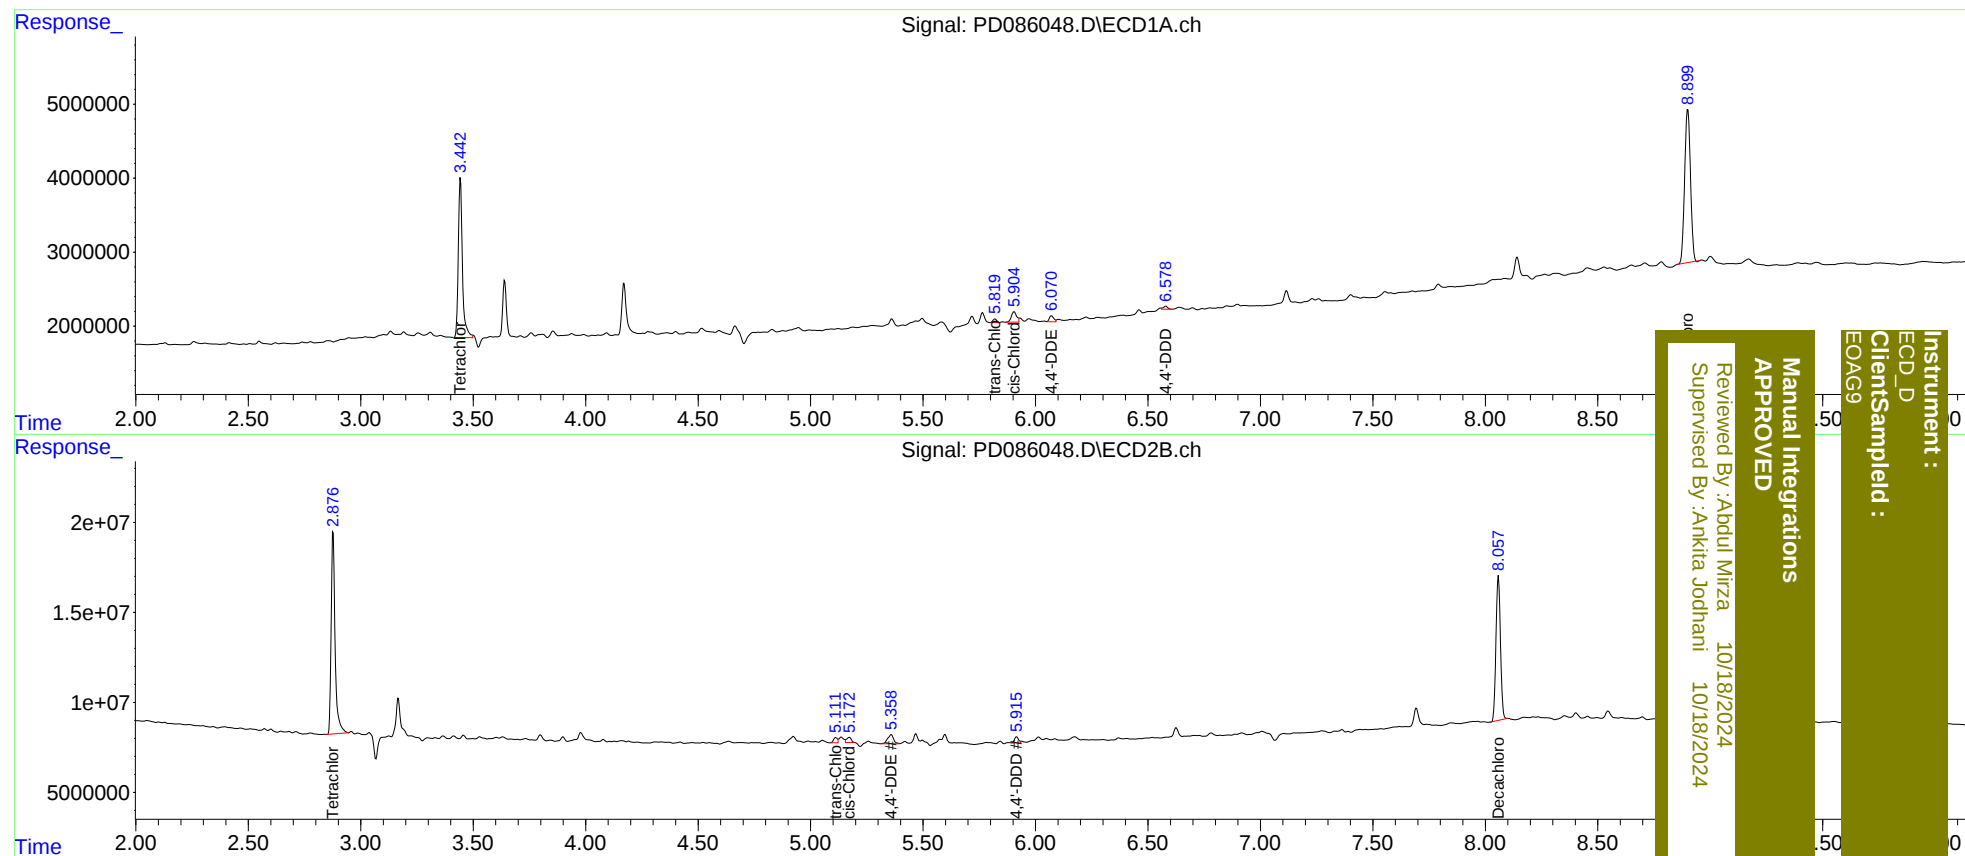

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/18/2024
Supervised By: Ankita Jodhani 10/18/2024

Instrument :
ECD_D
Client Sampled :
EOAG9