

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101524\
 Data File : PD086054.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 15:04
 Operator : AR\AJ
 Sample : P4349-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EOAG4

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/16/2024
 Supervised By :Ankita Jodhani 10/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 03:56:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 09 17:21:49 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.442	2.877	28687630	138.2E6	25.080m	22.262
2) SA Decachlor...	8.901	8.059	36583887	109.9E6	18.969	22.607
Target Compounds						
6) B beta-BHC	4.390	4.029	444864	5888466	0.422m	1.306 #
14) MA Endrin	6.459	5.783	661851	17374095	0.428m	2.946 #
15) B Endosulfa...	6.649	6.087	787339	3625415	0.397	0.518 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101524\
Data File : PD086054.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 15:04
Operator : AR\AJ
Sample : P4349-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 03:56:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 09 17:21:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

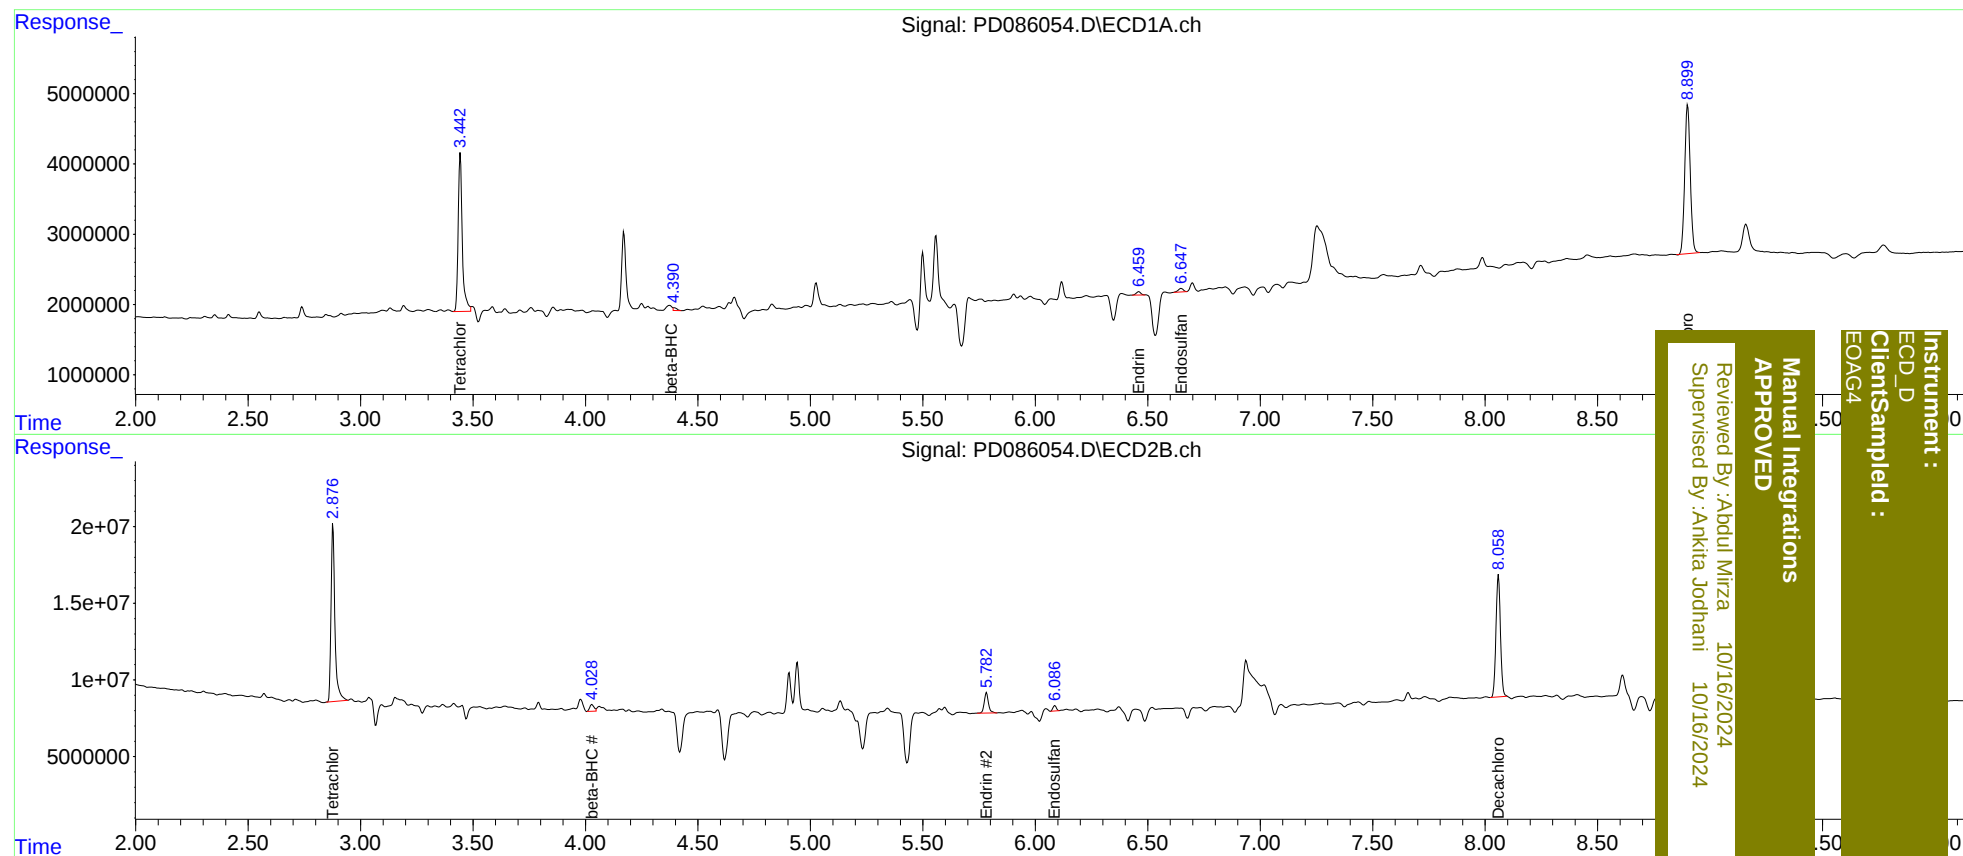

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/16/2024
Supervised By: Ankita Jodhani 10/16/2024

Instrument :
ECD_D
Client Sampled :
EOAG4