

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101524\
 Data File : PD086065.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 18:27
 Operator : AR\AJ
 Sample : P4349-21MS
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EOAG2MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/16/2024
 Supervised By : Ankita Jodhani 10/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:45:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 09 17:21:49 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	2.877	24826241	127.2E6	21.704	20.490
27)	SA Decachlor...	8.901	8.060	39716152	120.1E6	20.593	24.702
Target Compounds							
2)	A alpha-BHC	3.887	3.387	122.0E6	492.2E6	60.836	53.335
3)	MA gamma-BHC...	4.214	3.722	118.8E6	466.9E6	59.587	54.185
4)	MA Heptachlor	4.807	4.073	118.0E6	438.8E6	61.203	59.680
5)	MB Aldrin	5.146	4.357	120.3E6	444.6E6	49.980	45.979m
6)	B beta-BHC	4.401	4.016	46734064	192.0E6	44.357	42.577
7)	B delta-BHC	4.644	4.252	117.5E6	446.9E6	53.418m	48.234
8)	B Heptachlo...	5.565	4.861	112.7E6	386.9E6	50.605	44.411
9)	A Endosulfan I	5.947	5.235	103.9E6	300.9E6	56.928	43.405
10)	B trans-Chl...	5.820	5.113	108.2E6	414.8E6	48.150	46.108
11)	B cis-Chlor...	5.900	5.178	110.1E6	406.9E6	48.271	45.319
12)	B 4,4'-DDE	6.072	5.360	200.9E6	739.0E6	105.361	98.322m
13)	MA Dieldrin	6.219	5.499	233.1E6	785.5E6	118.421	106.117m
14)	MA Endrin	6.445	5.778	198.6E6	713.4E6	128.572	120.963
15)	B Endosulfa...	6.657	6.070	194.2E6	656.3E6	97.824	93.852
16)	A 4,4'-DDD	6.581	5.917	160.8E6	589.7E6	128.913	123.593
17)	MA 4,4'-DDT	6.895	6.171	169.6E6	633.1E6	125.651	127.119
18)	B Endrin al...	6.787	6.248	147.8E6	494.8E6	96.394	95.505
19)	B Endosulfa...	7.021	6.472	187.0E6	571.4E6	102.112	94.342
20)	A Methoxychlor	7.370	6.742	469.1E6	1313.7E6	586.749	626.668
21)	B Endrin ke...	7.498	6.983	207.4E6	698.9E6	102.009	95.964

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101524\
Data File : PD086065.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 18:27
Operator : AR\AJ
Sample : P4349-21MS
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:45:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 09 17:21:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

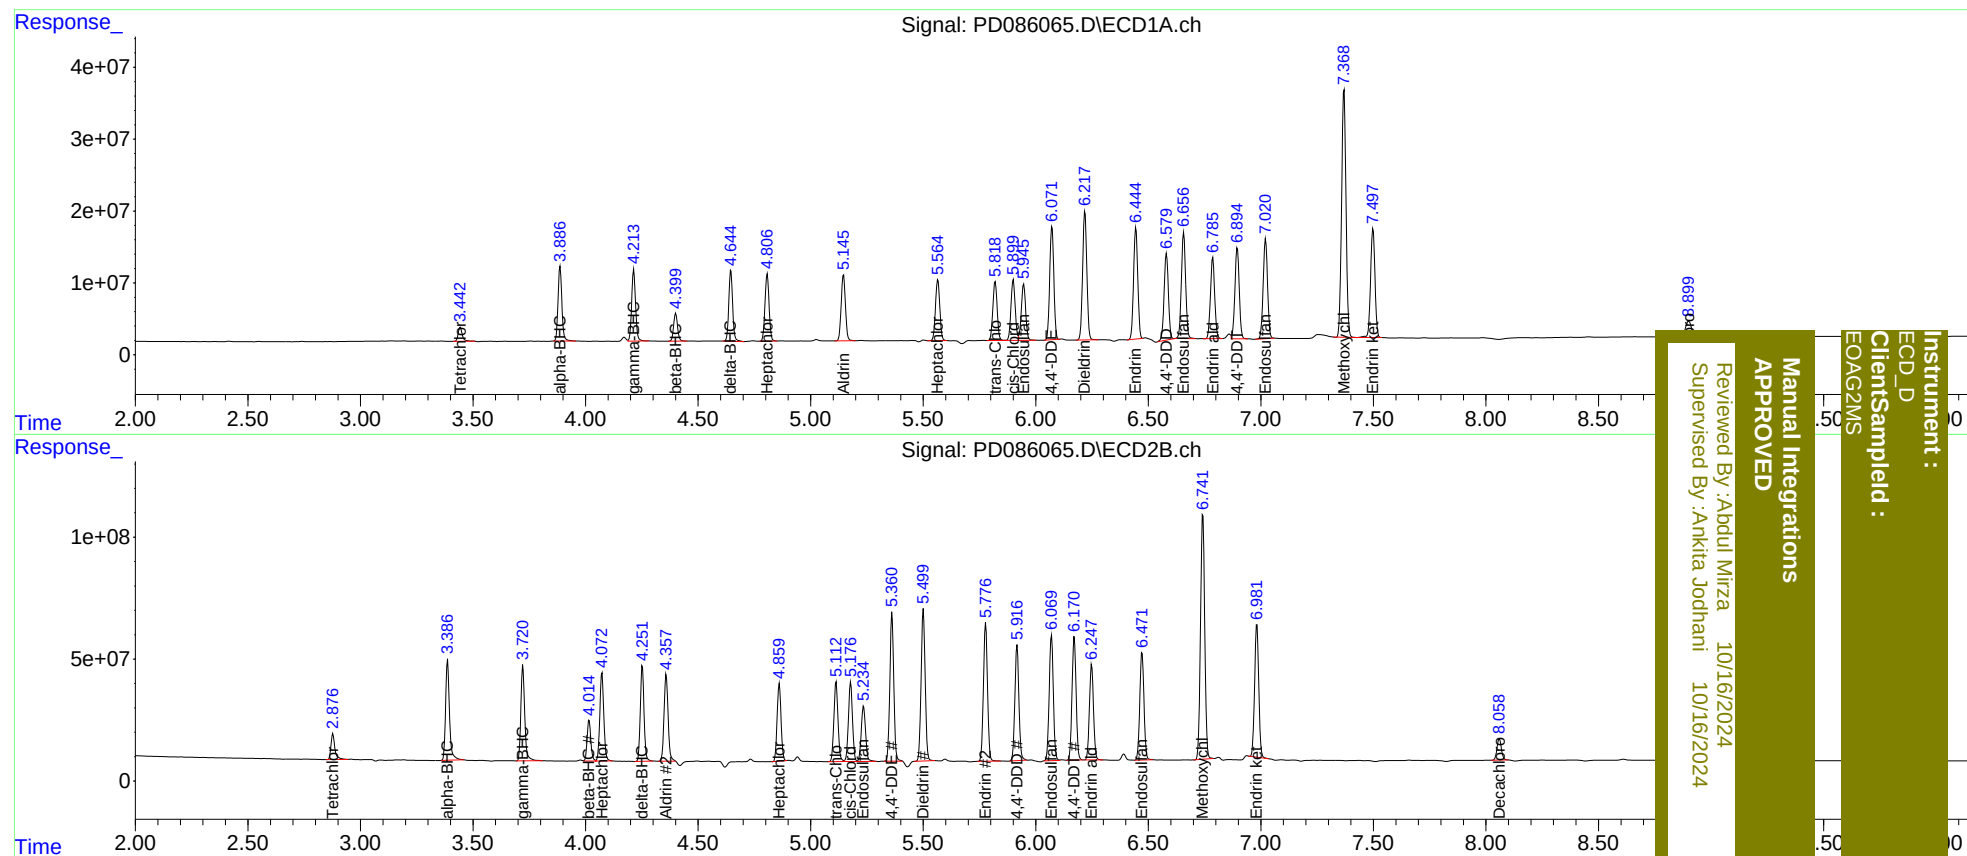

Manual Integrations
APPROVED
Reviewed By: Abul Mirza 10/16/2024
Supervised By: Ankita Jodhani 10/16/2024

Instrument :
ECD_D
Client Sampled :
EOAGZMS