

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101619\
Data File : PD055316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2019 14:07
Operator : SG\AJ
Sample : INDA322
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
ECD_D
LabSampleId :
INDA322

Manual Integrations
APPROVED

Ankita
10/18/2019 12:17:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 03:37:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101519CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 16 04:32:26 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

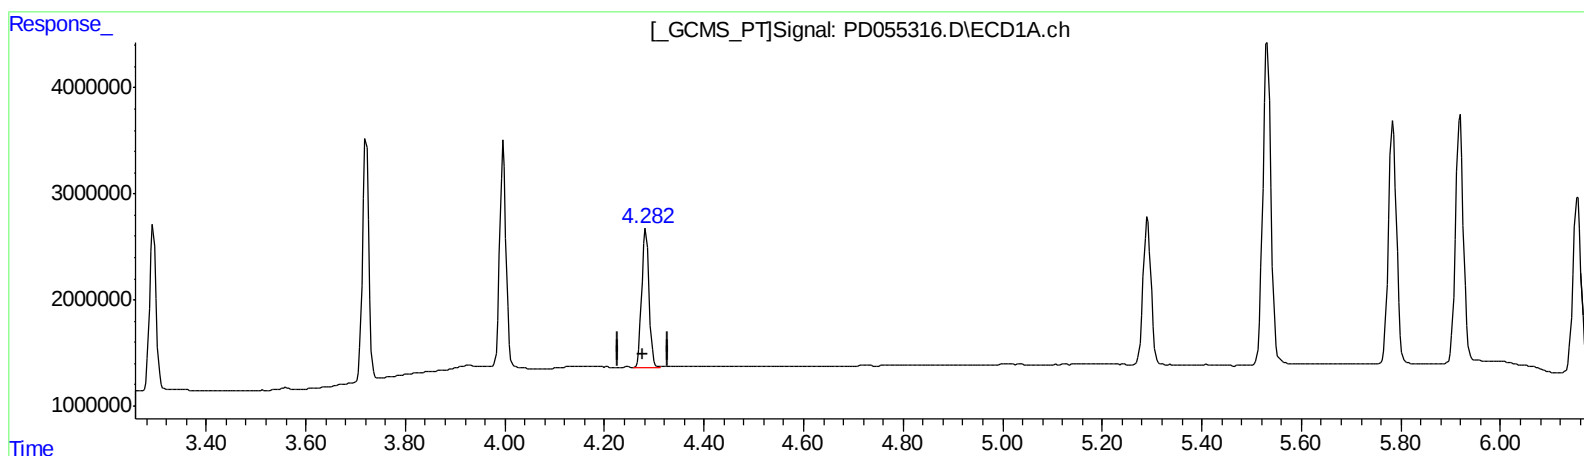

(4) Heptachlor (MA)
4.283min 25.057 ng/ml
response 12951618

(4) Heptachlor #2 (MA)
5.139min 23.363 ng/ml
response 27865885

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101619\
Data File : PD055316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2019 14:07
Operator : SG\AJ
Sample : INDA322
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
ECD_D
LabSampleId :
INDA322

Manual Integrations
APPROVED

Ankita
10/18/2019 12:17:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 03:37:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101519CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 16 04:32:26 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

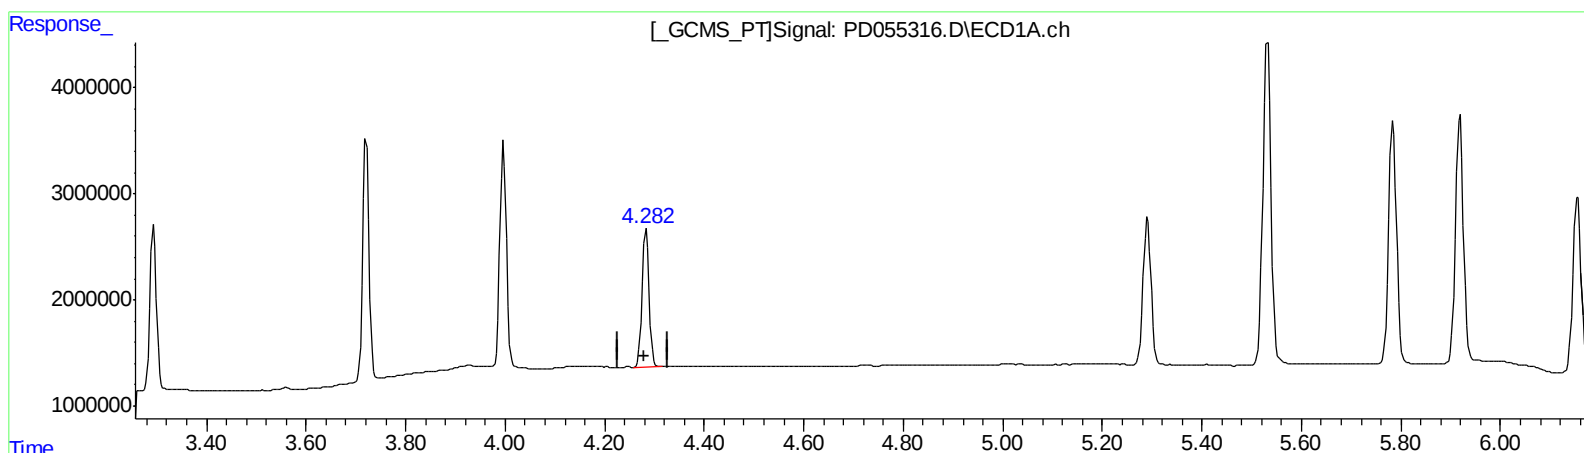

(4) Heptachlor (MA)
4.282min 24.851 ng/ml m
response 12845377

(4) Heptachlor #2 (MA)
5.139min 23.363 ng/ml
response 27865885

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101619\
 Data File : PD055316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2019 14:07
 Operator : SG\AJ
 Sample : INDA322
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 LabSampleId :
 INDA322

Manual Integrations
 APPROVED

Ankita
 10/18/2019 12:17:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 03:37:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101519CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 16 04:32:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.294	3.962	13699905	21076597	21.685	22.629
27) SA Decachlor...	7.973	9.001	30267024	43320229	43.744	43.878
Target Compounds						
2) A alpha-BHC	3.721	4.349	20428279	30329839	21.764	23.372
3) MA gamma-BHC...	3.997	4.632	19090010	28659538	21.915	22.248
4) MA Heptachlor	4.282	5.139	12845377	27865885	24.851m	23.363
9) A Endosulfan I	5.291	6.182	15696541	25504284	21.640	22.614
13) MA Dieldrin	5.532	6.438	35248945	56727353	43.999	44.904
14) MA Endrin	5.784	6.655	25482067	38595845	39.335	39.027
16) A 4,4'-DDD	5.919	6.778	26144279	46577537	44.979	45.658
17) MA 4,4'-DDT	6.155	7.076	18834093	39624763	46.976	42.398
20) A Methoxychlor	6.703	7.532	52507945	117.9E6	240.828	215.854

AJ
 10/24/19

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.