

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101619\
Data File : PD055338.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2019 01:40
Operator : SG\AJ
Sample : INDA323
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
ECD_D
LabSampleId :
INDA323

Manual Integrations
APPROVED

Ankita
10/18/2019 12:18:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 03:45:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101519CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 16 04:32:26 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

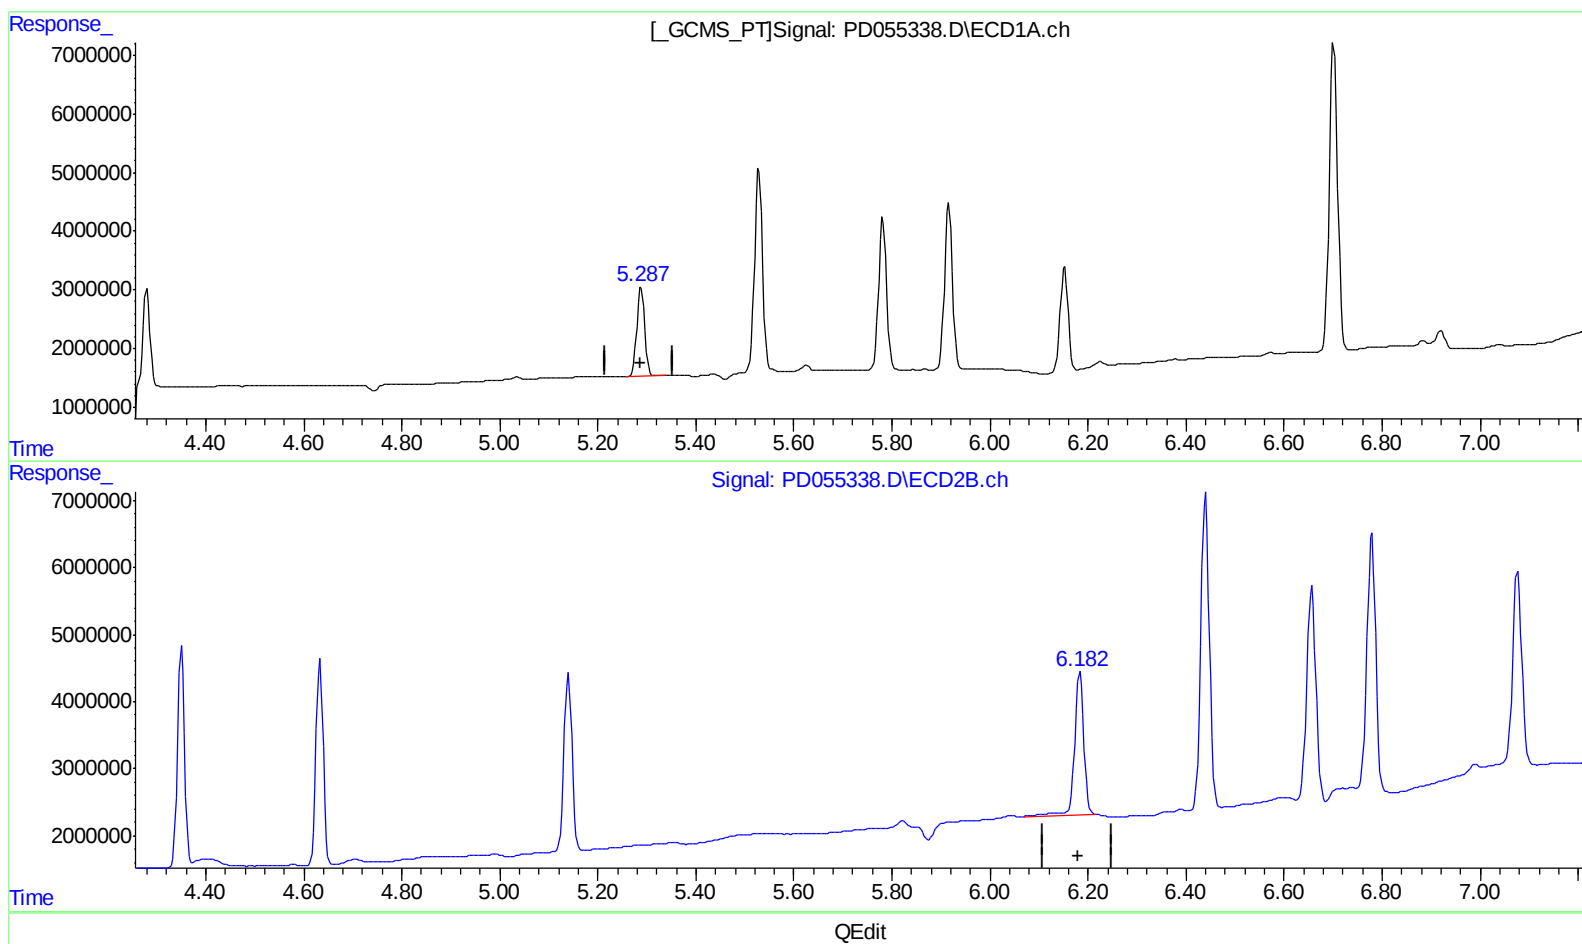

(9) Endosulfan I (A)
5.289min 23.728 ng/ml
response 17211067

(9) Endosulfan I #2 (A)
6.184min 24.619 ng/ml
response 27765570

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101619\
Data File : PD055338.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2019 01:40
Operator : SG\AJ
Sample : INDA323
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
ECD_D
LabSampleId :
INDA323

Manual Integrations
APPROVED

Ankita
10/18/2019 12:18:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 03:45:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101519CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 16 04:32:26 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

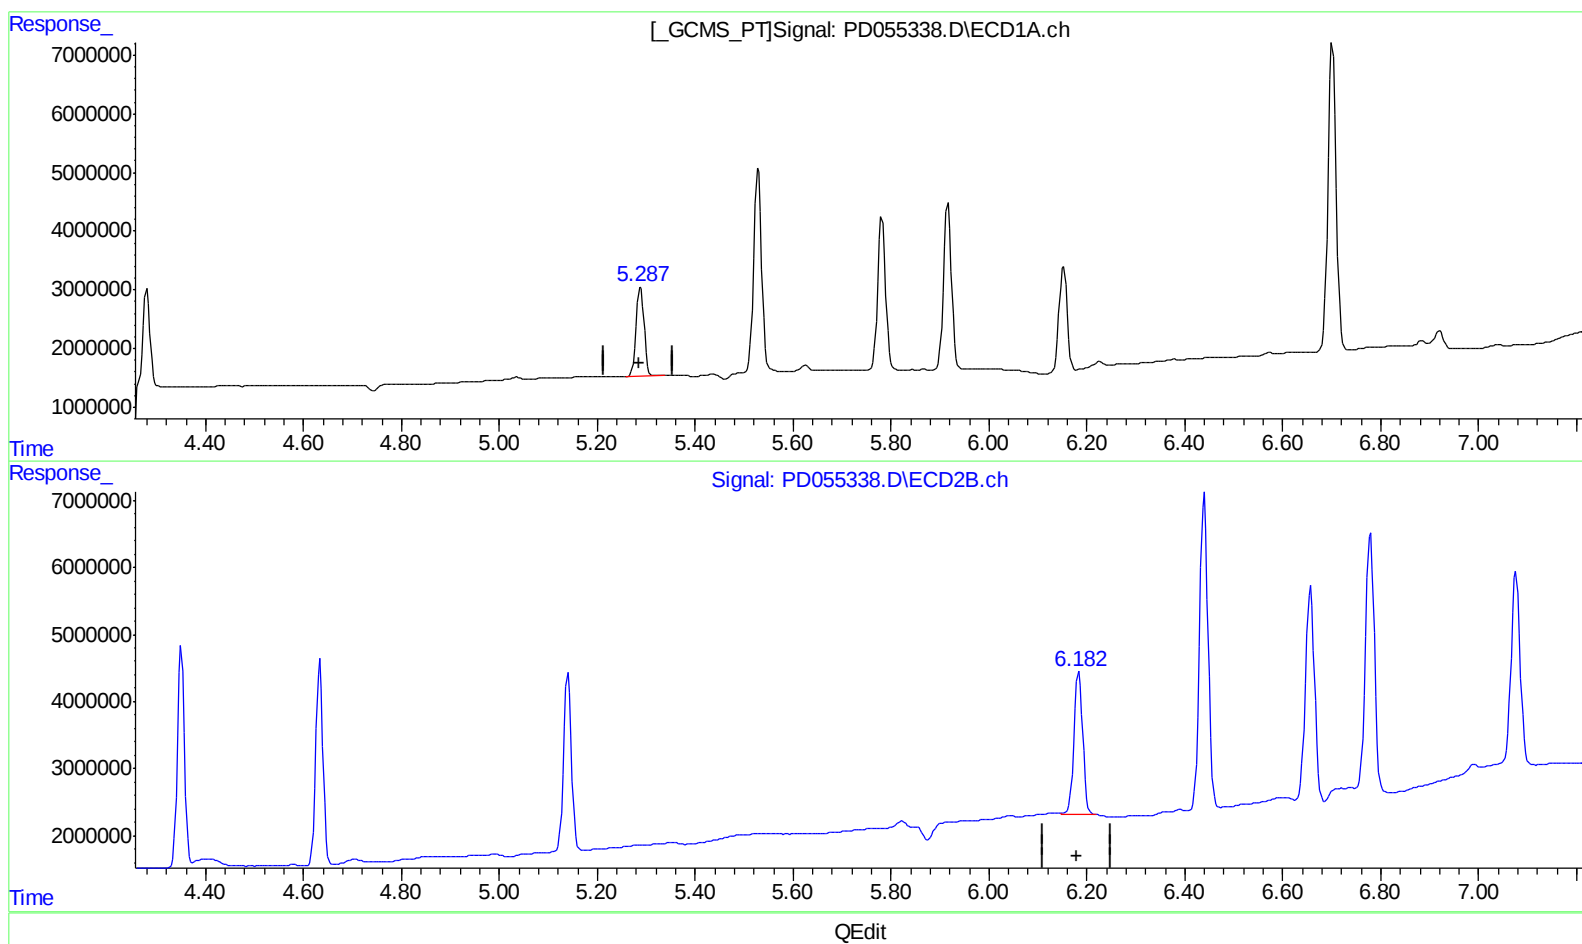

(9) Endosulfan I (A)

5.289min 23.728 ng/ml

response 17211067

(9) Endosulfan I #2 (A)

6.182min 23.434 ng/ml m

response 26428726

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101619\
 Data File : PD055338.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2019 01:40
 Operator : SG\AJ
 Sample : INDA323
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 LabSampleId :
 INDA323

Manual Integrations
 APPROVED

Ankita
 10/18/2019 12:18:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 03:45:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101519CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 16 04:32:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.291	3.964	15461658	22914175	24.474	24.602
27) SA Decachlor...	7.972	9.004	31555681	34418446	45.606	34.861
Target Compounds						
2) A alpha-BHC	3.718	4.351	22503149	31977268	23.975	24.641
3) MA gamma-BHC...	3.994	4.633	21347447	31252829	24.507	24.261
4) MA Heptachlor	4.280	5.140	16408301	30077609	31.745	25.217
9) A Endosulfan I	5.289	6.182	17211067	26428726	23.728	23.434m
13) MA Dieldrin	5.529	6.440	39917467	57486963	49.826	45.505
14) MA Endrin	5.782	6.657	29308064	40463591	45.241	40.916
16) A 4,4'-DDD	5.916	6.779	31631345	47787161	54.419	46.844
17) MA 4,4'-DDT	6.152	7.076	20598106	37158786	51.376	39.759
20) A Methoxychlor	6.701	7.534	62191306	108.7E6	285.241	198.998 #

AJ
 10/24/19

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.