

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
 Data File : PD066281.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2021 09:26
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 23:28:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 18 23:27:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	10704041	50394099	5.213	5.584
27)	SA Decachlor...	8.167	9.021	14700299	50687437	10.670	10.360
Target Compounds							
2)	A alpha-BHC	3.877	4.364	15385042	63798378	4.900	5.442
3)	MA gamma-BHC...	4.159	4.648	16717328	61317195	5.482	5.503
4)	MA Heptachlor	4.453	5.148	14372363	54911923	4.850	5.310
9)	A Endosulfan I	5.476	6.197	13035647	46451150	5.179	5.420
13)	MA Dieldrin	5.718	6.455	26025699	90749434	9.557	10.620
14)	MA Endrin	5.975	6.671	23992020	64621297	10.102	11.491
16)	A 4,4'-DDD	6.100	6.799	20058604	71389675	9.510	10.571
17)	MA 4,4'-DDT	6.338	7.096	18276785	70788555	8.990	10.762
20)	A Methoxychlor	6.886	7.557	53022954	181.5E6	50.011	55.861

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
Data File : PD066281.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2021 09:26
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 23:28:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
Quant Title : GC Extractables
QLast Update : Mon Oct 18 23:27:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

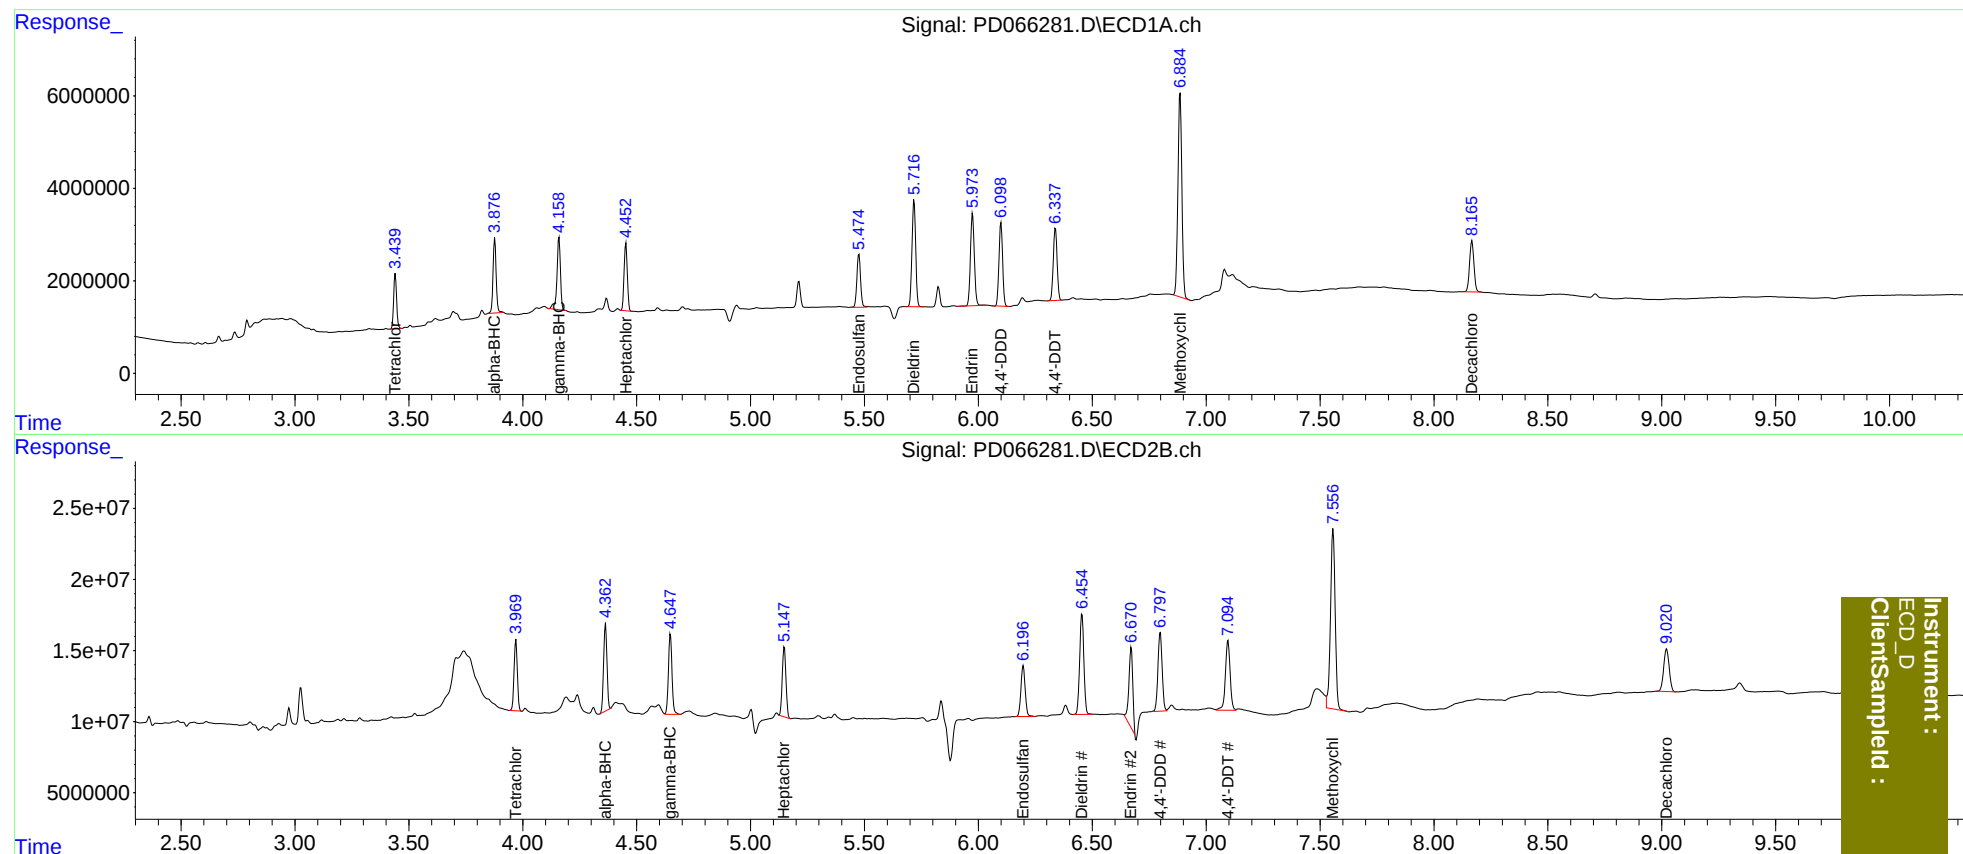


Instrument :
ECD_D
ClientSampled :

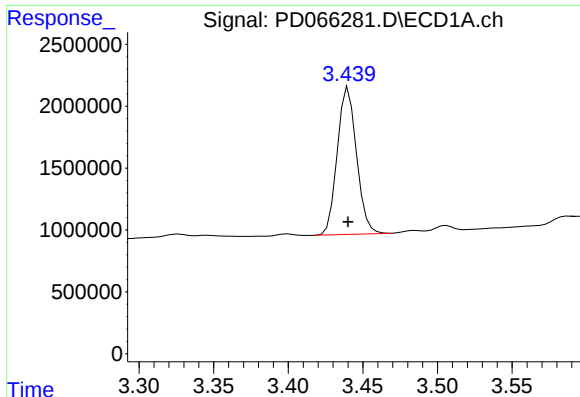

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 10704041
Conc: 5.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

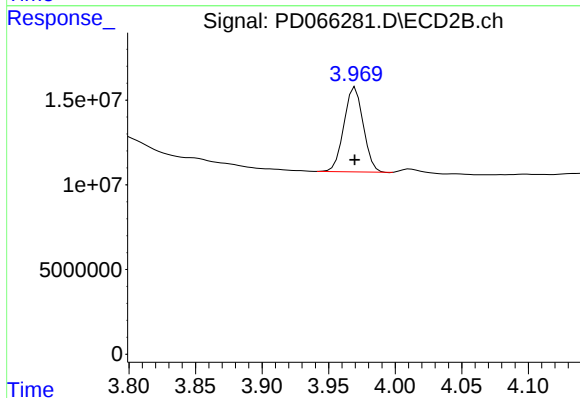


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 50394099
Conc: 5.58 ng/ml

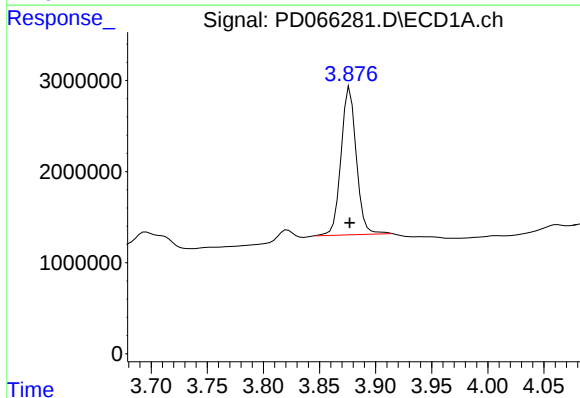


#2 alpha-BHC

R.T.: 3.877 min
Delta R.T.: 0.000 min
Response: 15385042
Conc: 4.90 ng/ml

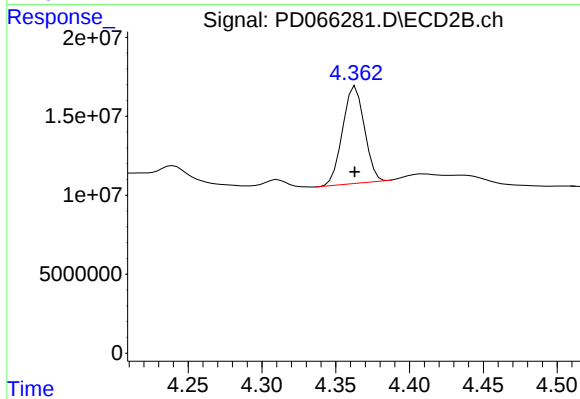

#2 alpha-BHC


R.T.: 4.364 min
Delta R.T.: 0.000 min
Response: 63798378
Conc: 5.44 ng/ml

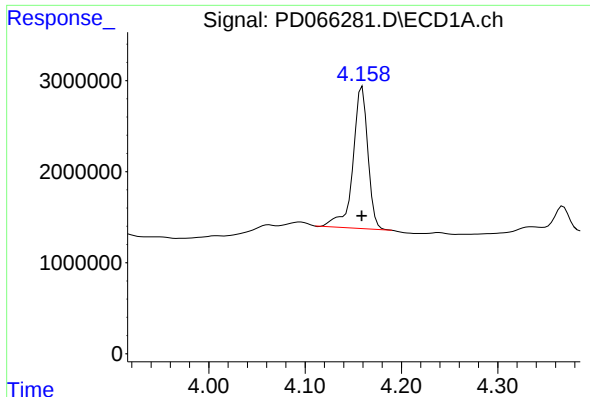

#3 gamma-BHC (Lindane)


R.T.: 4.159 min
Delta R.T.: 0.000 min
Response: 16717328
Conc: 5.48 ng/ml

Instrument :
ECD_D
ClientSampleId :

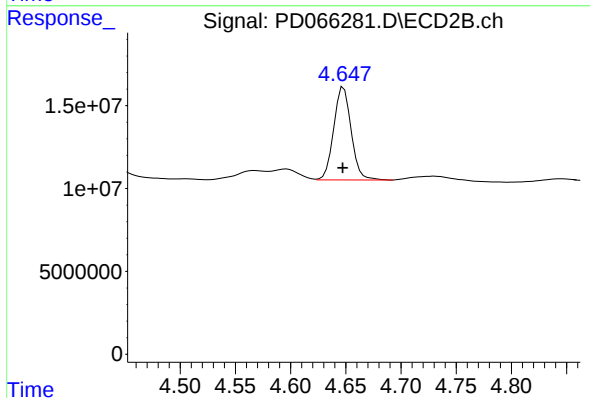


#3 gamma-BHC (Lindane)

R.T.: 4.648 min
Delta R.T.: 0.000 min
Response: 61317195
Conc: 5.50 ng/ml

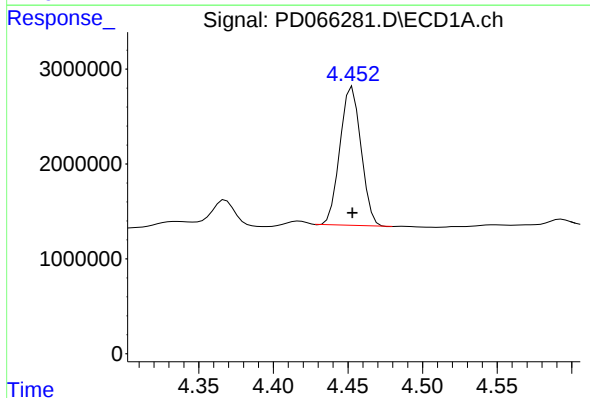


#4 Heptachlor

R.T.: 4.453 min
Delta R.T.: 0.000 min
Response: 14372363
Conc: 4.85 ng/ml

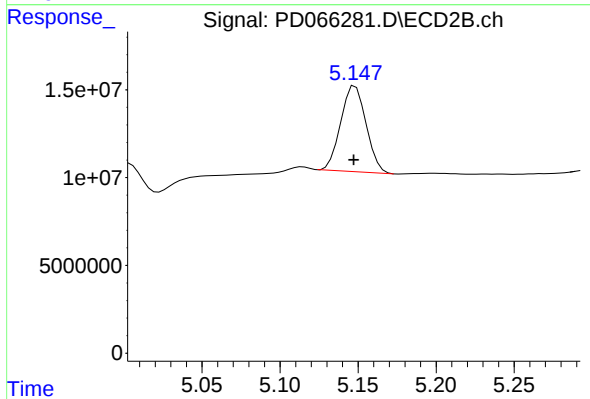

#4 Heptachlor


R.T.: 5.148 min
Delta R.T.: 0.000 min
Response: 54911923
Conc: 5.31 ng/ml

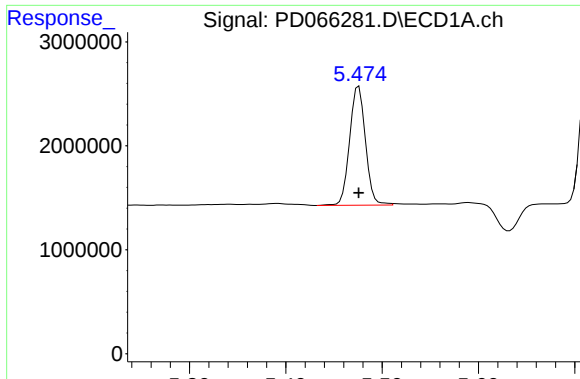

#9 Endosulfan I


R.T.: 5.476 min
Delta R.T.: 0.000 min
Response: 13035647
Conc: 5.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

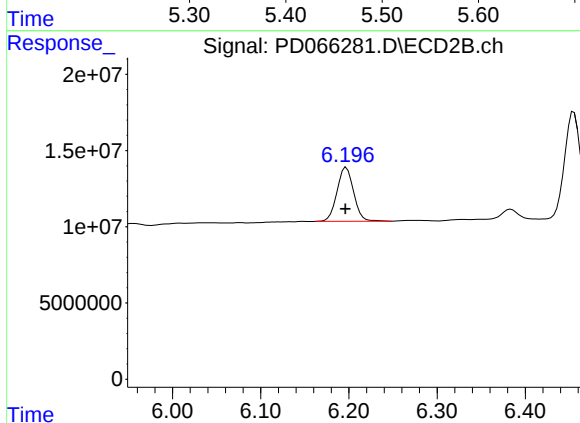


#9 Endosulfan I

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 46451150
Conc: 5.42 ng/ml

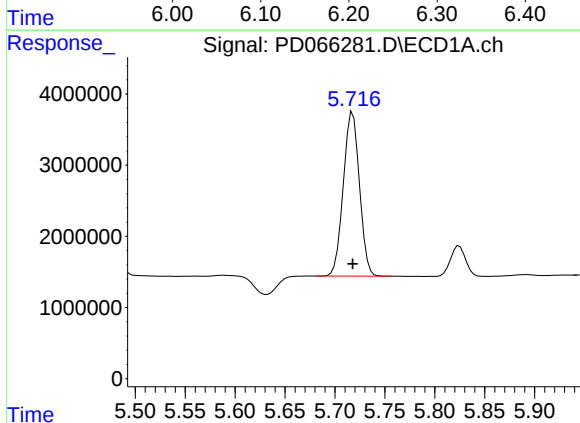


#13 Dieldrin

R.T.: 5.718 min
Delta R.T.: 0.000 min
Response: 26025699
Conc: 9.56 ng/ml

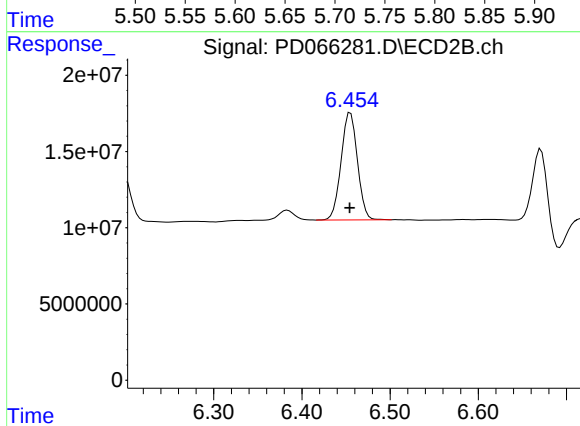

#13 Dieldrin


R.T.: 6.455 min
Delta R.T.: 0.000 min
Response: 90749434
Conc: 10.62 ng/ml

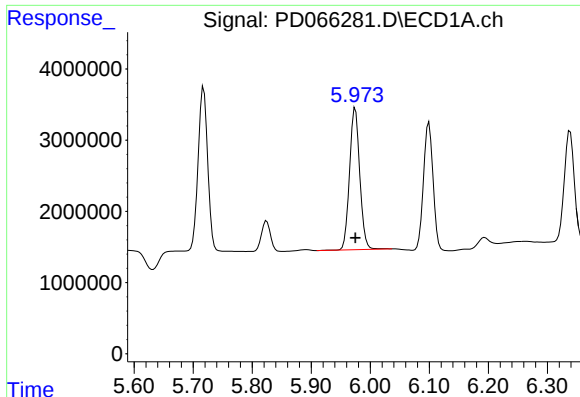

#14 Endrin


R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 23992020
Conc: 10.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

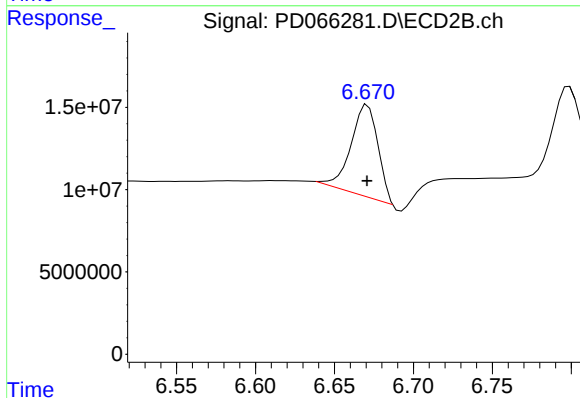


#14 Endrin

R.T.: 6.671 min
Delta R.T.: 0.000 min
Response: 64621297
Conc: 11.49 ng/ml

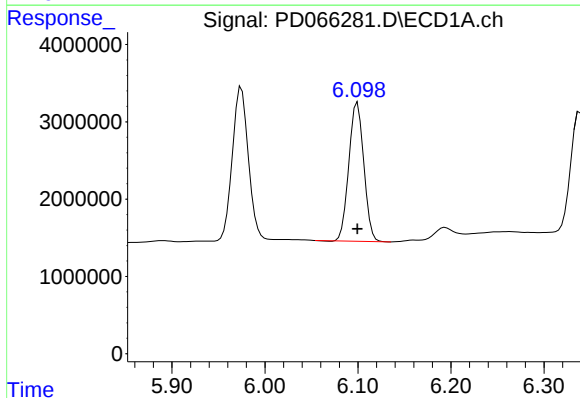


#16 4,4'-DDD

R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 20058604
Conc: 9.51 ng/ml

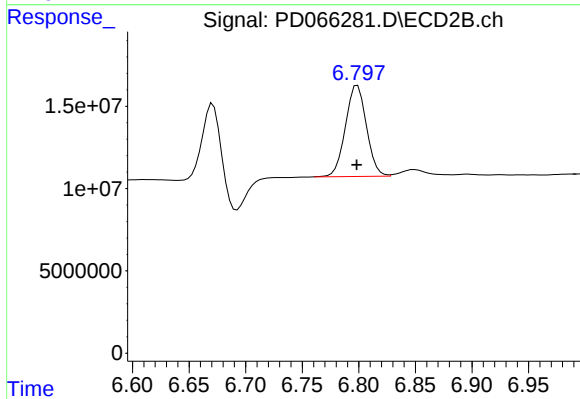

#16 4,4'-DDD


R.T.: 6.799 min
Delta R.T.: 0.000 min
Response: 71389675
Conc: 10.57 ng/ml

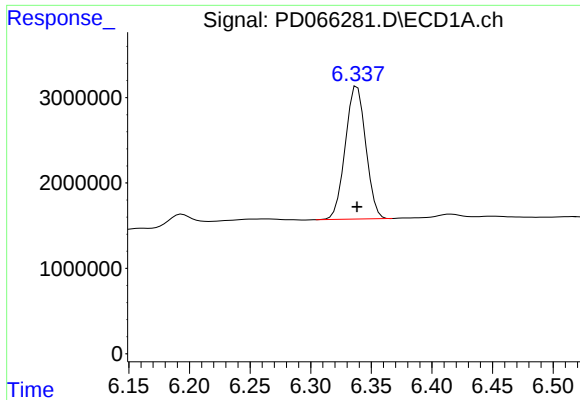

#17 4,4'-DDT


R.T.: 6.338 min
Delta R.T.: 0.000 min
Response: 18276785
Conc: 8.99 ng/ml

Instrument :
ECD_D
ClientSampleId :

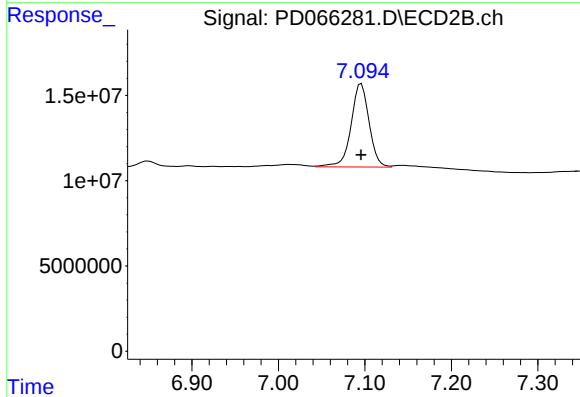


#17 4,4'-DDT

R.T.: 7.096 min
Delta R.T.: 0.000 min
Response: 70788555
Conc: 10.76 ng/ml

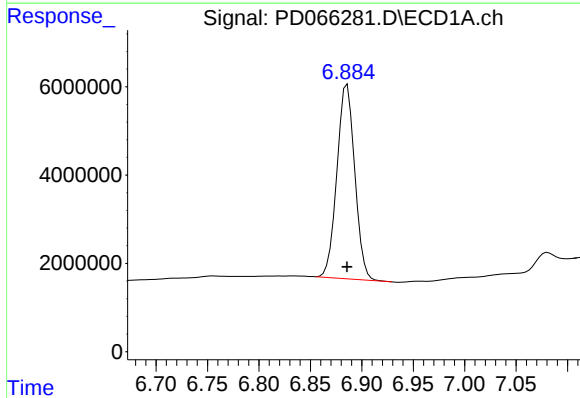


#20 Methoxychlor

R.T.: 6.886 min
Delta R.T.: 0.000 min
Response: 53022954
Conc: 50.01 ng/ml

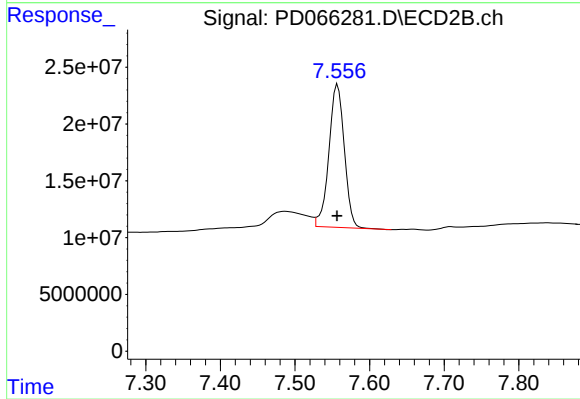

#20 Methoxychlor


R.T.: 7.557 min
Delta R.T.: 0.000 min
Response: 181468705
Conc: 55.86 ng/ml

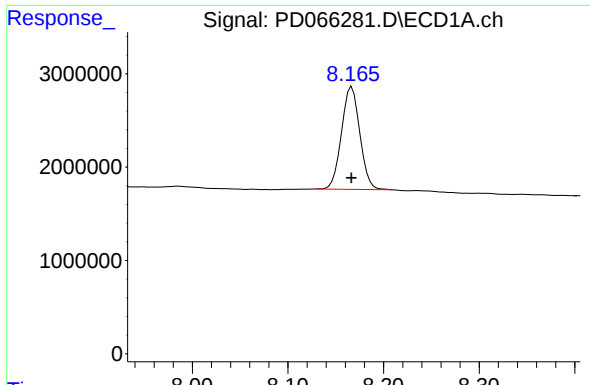

#27 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: 0.000 min
Response: 14700299
Conc: 10.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

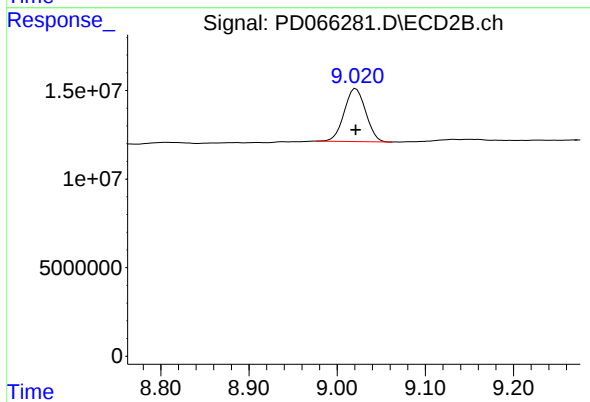

#27 Decachlorobiphenyl

R.T.: 9.021 min
Delta R.T.: 0.000 min
Response: 50687437
Conc: 10.36 ng/ml