

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
 Data File : PD066283.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2021 09:54
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 23:28:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 18 23:27:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	21064735	95932198	10.258	10.630
27)	SA Decachlor...	8.167	9.021	27940352	99909347	20.279	20.420
Target Compounds							
2)	A alpha-BHC	3.877	4.363	31154682	122.7E6	9.921	10.463
3)	MA gamma-BHC...	4.159	4.648	31704143	117.5E6	10.396	10.550
4)	MA Heptachlor	4.453	5.148	29293112	107.1E6	9.886	10.359
9)	A Endosulfan I	5.475	6.196	26758448	91277614	10.631	10.651
13)	MA Dieldrin	5.717	6.454	52837347	177.8E6	19.402	20.806
14)	MA Endrin	5.975	6.669	51687086	113.6E6	21.763	20.195
16)	A 4,4'-DDD	6.100	6.798	41643666	138.8E6	19.743	20.556
17)	MA 4,4'-DDT	6.339	7.096	38682542	140.6E6	19.026	21.374
20)	A Methoxychlor	6.886	7.557	105.6E6	426.4E6	99.642	131.252 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
Data File : PD066283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2021 09:54
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 23:28:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
Quant Title : GC Extractables
QLast Update : Mon Oct 18 23:27:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

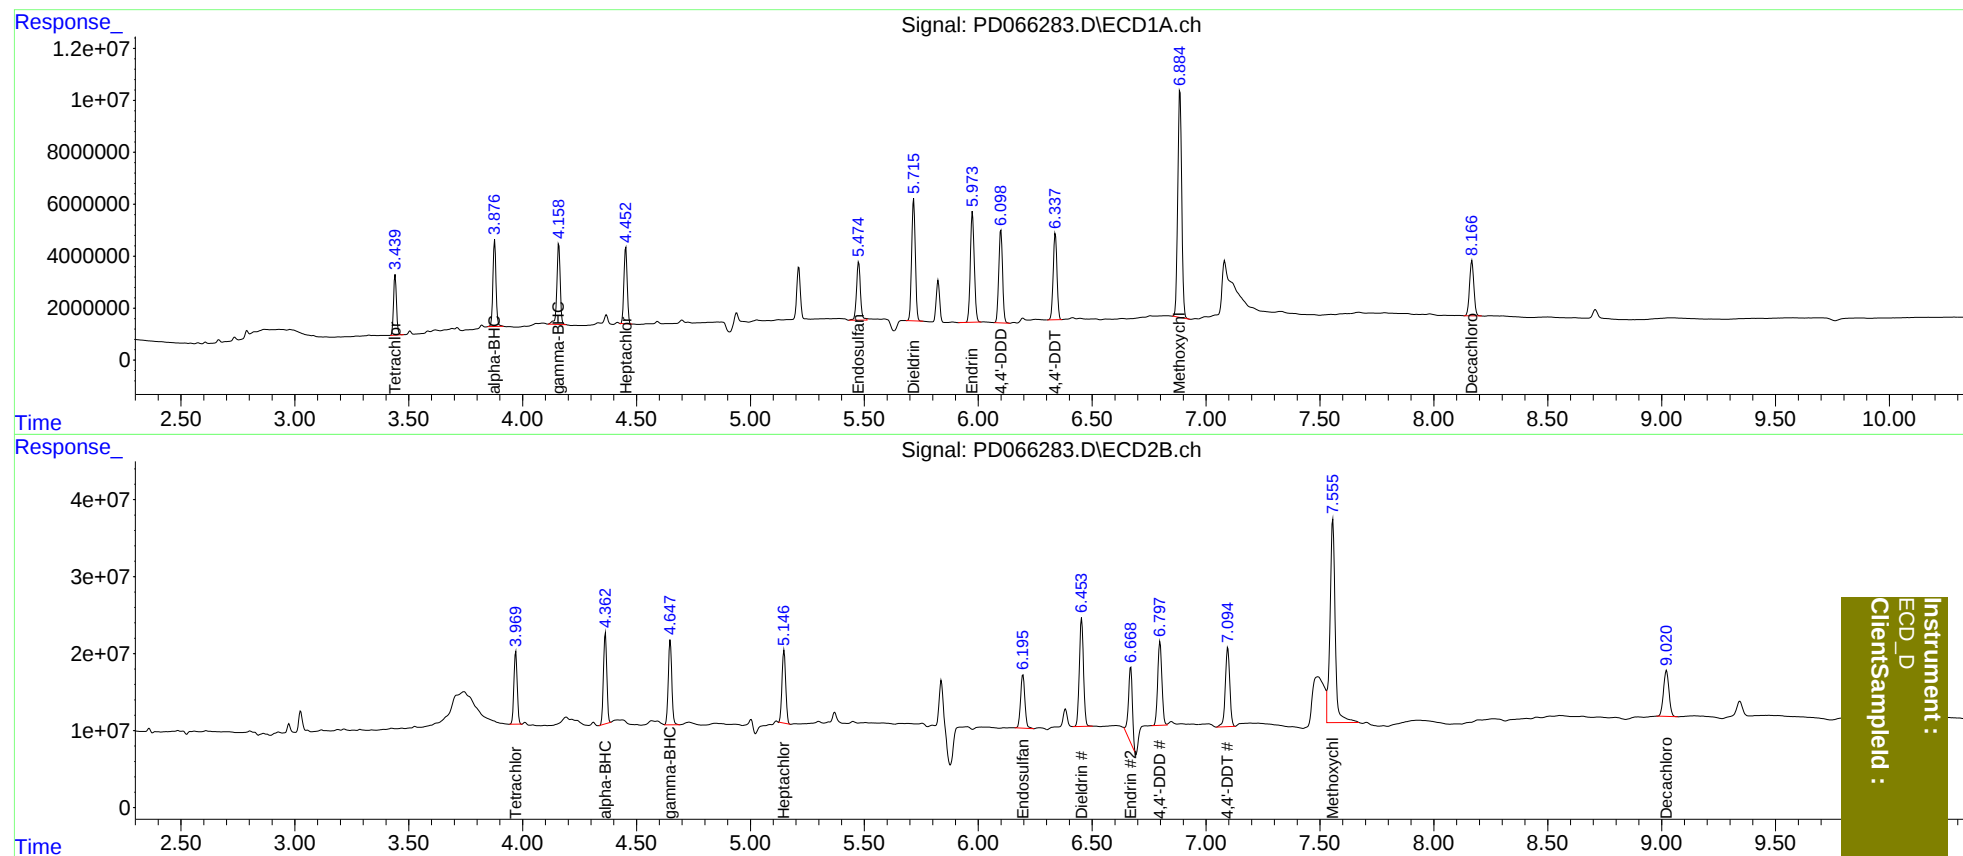


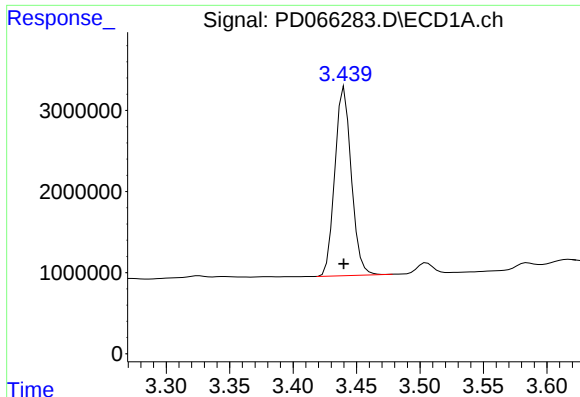

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 21064735
Conc: 10.26 ng/ml

Instrument :
ECD_D
ClientSampleId :

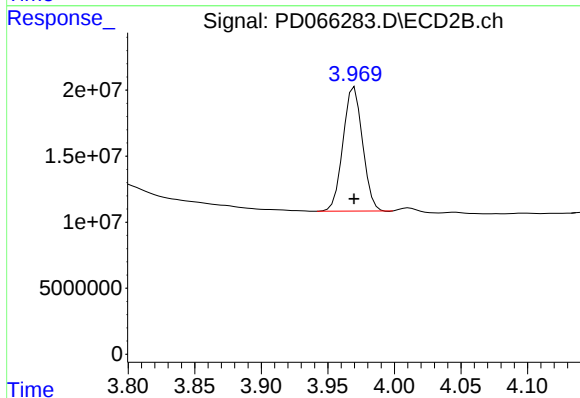


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 95932198
Conc: 10.63 ng/ml

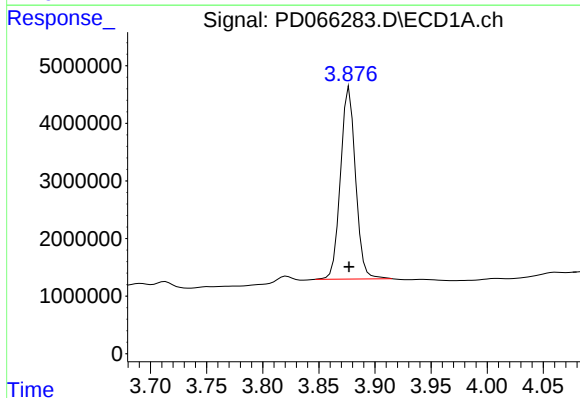


#2 alpha-BHC

R.T.: 3.877 min
Delta R.T.: 0.000 min
Response: 31154682
Conc: 9.92 ng/ml

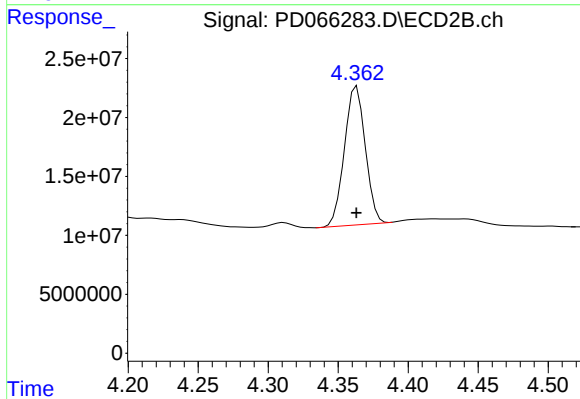

#2 alpha-BHC


R.T.: 4.363 min
Delta R.T.: 0.000 min
Response: 122666663
Conc: 10.46 ng/ml

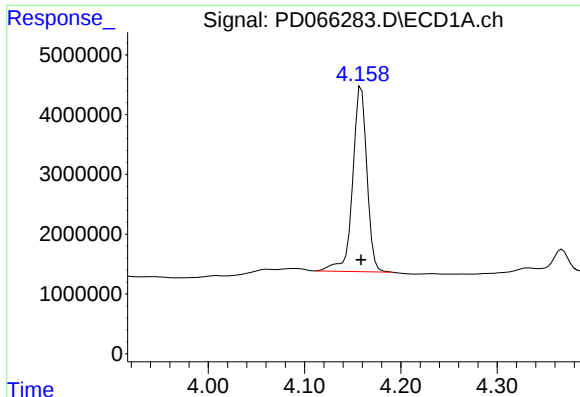

#3 gamma-BHC (Lindane)


R.T.: 4.159 min
Delta R.T.: 0.000 min
Response: 31704143
Conc: 10.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

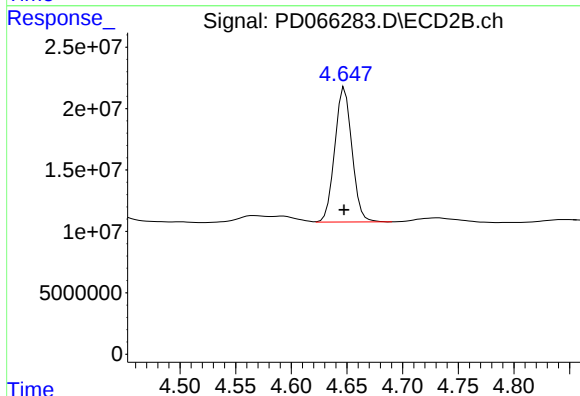


#3 gamma-BHC (Lindane)

R.T.: 4.648 min
Delta R.T.: 0.000 min
Response: 117545947
Conc: 10.55 ng/ml

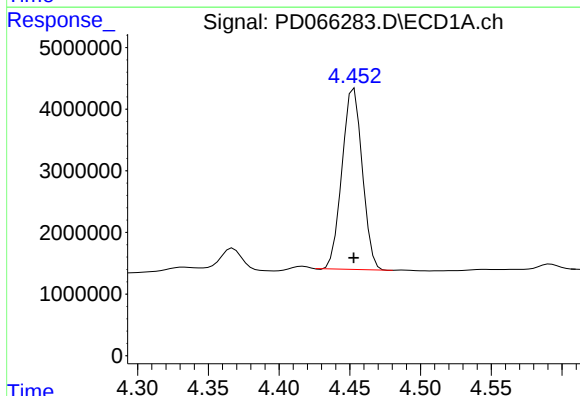


#4 Heptachlor

R.T.: 4.453 min
Delta R.T.: 0.000 min
Response: 29293112
Conc: 9.89 ng/ml

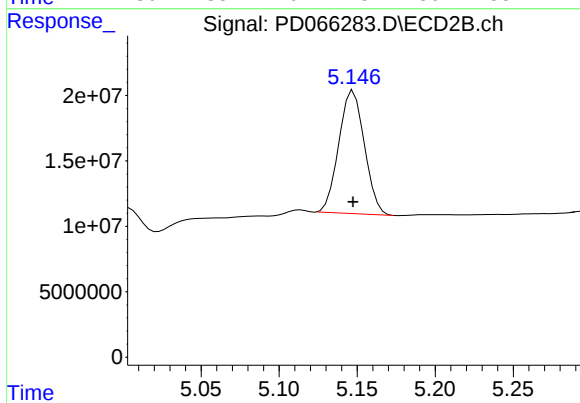

#4 Heptachlor


R.T.: 5.148 min
Delta R.T.: 0.000 min
Response: 107117501
Conc: 10.36 ng/ml

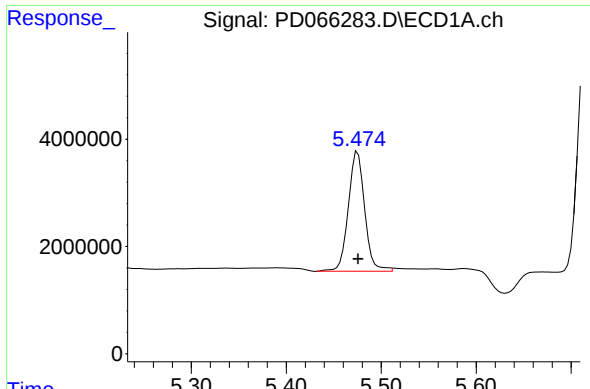

#9 Endosulfan I


R.T.: 5.475 min
Delta R.T.: 0.000 min
Response: 26758448
Conc: 10.63 ng/ml

Instrument :
ECD_D
ClientSampleId :

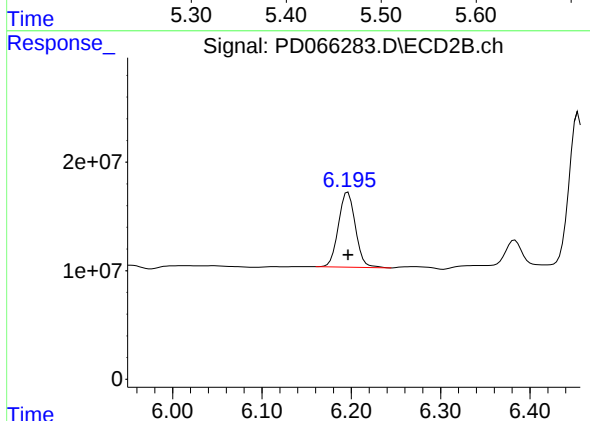


#9 Endosulfan I

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 91277614
Conc: 10.65 ng/ml

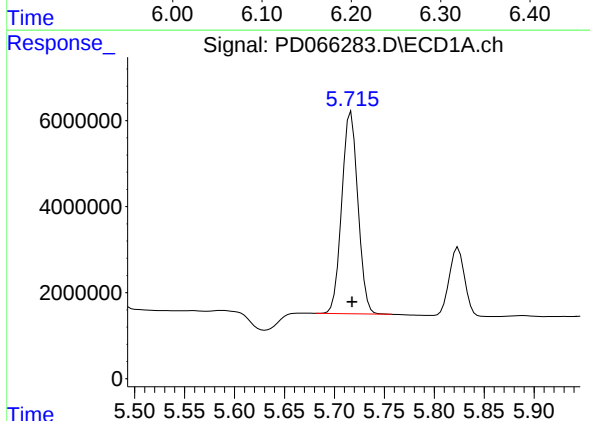


#13 Dieldrin

R.T.: 5.717 min
Delta R.T.: 0.000 min
Response: 52837347
Conc: 19.40 ng/ml

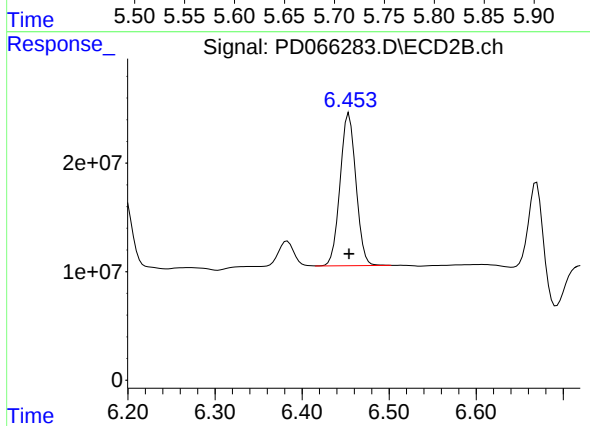

#13 Dieldrin


R.T.: 6.454 min
Delta R.T.: 0.000 min
Response: 177781647
Conc: 20.81 ng/ml

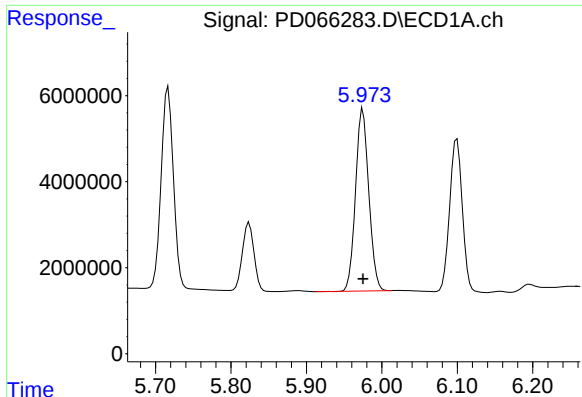

#14 Endrin


R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 51687086
Conc: 21.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

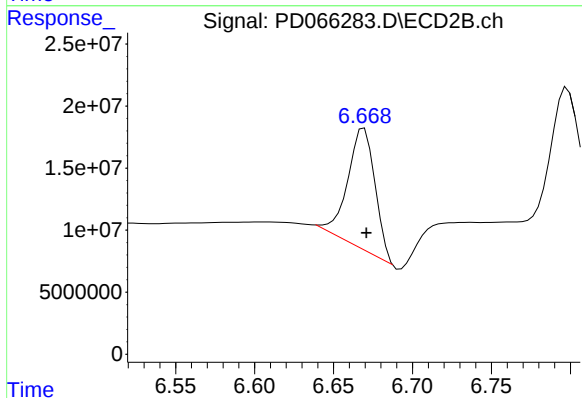


#14 Endrin

R.T.: 6.669 min
Delta R.T.: -0.001 min
Response: 113568301
Conc: 20.20 ng/ml

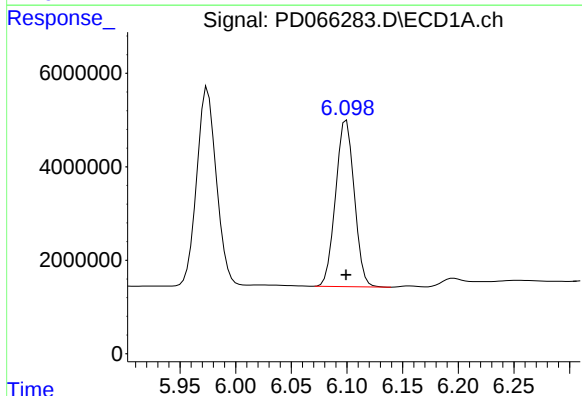


#16 4,4'-DDD

R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 41643666
Conc: 19.74 ng/ml

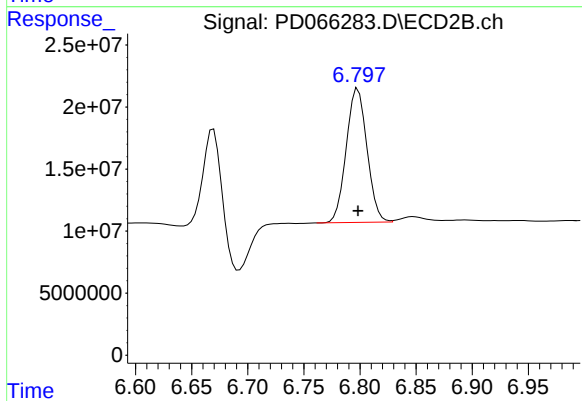

#16 4,4'-DDD


R.T.: 6.798 min
Delta R.T.: 0.000 min
Response: 138822314
Conc: 20.56 ng/ml

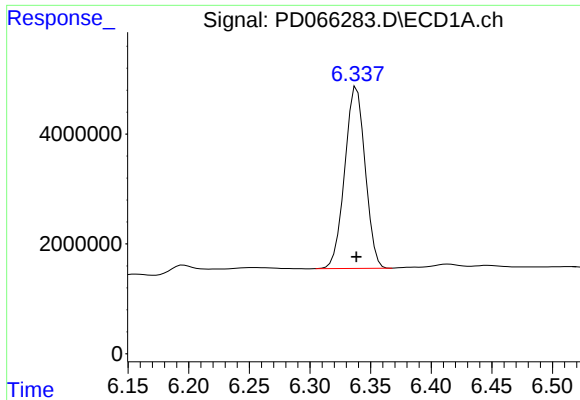

#17 4,4'-DDT


R.T.: 6.339 min
Delta R.T.: 0.000 min
Response: 38682542
Conc: 19.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

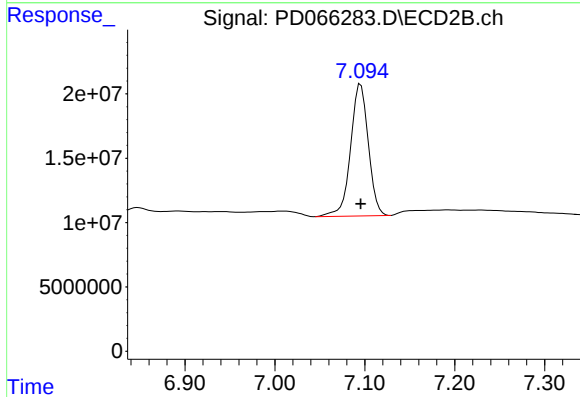


#17 4,4'-DDT

R.T.: 7.096 min
Delta R.T.: 0.000 min
Response: 140581191
Conc: 21.37 ng/ml

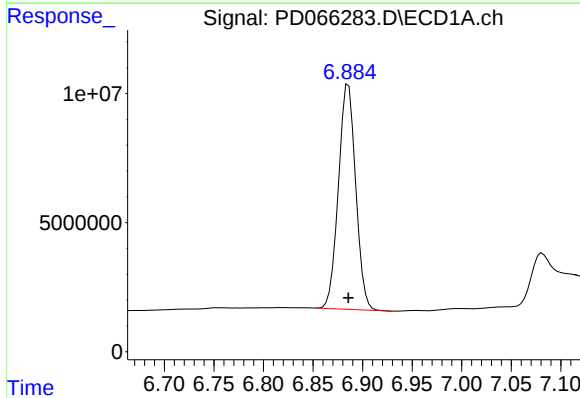


#20 Methoxychlor

R.T.: 6.886 min
Delta R.T.: 0.000 min
Response: 105642892
Conc: 99.64 ng/ml

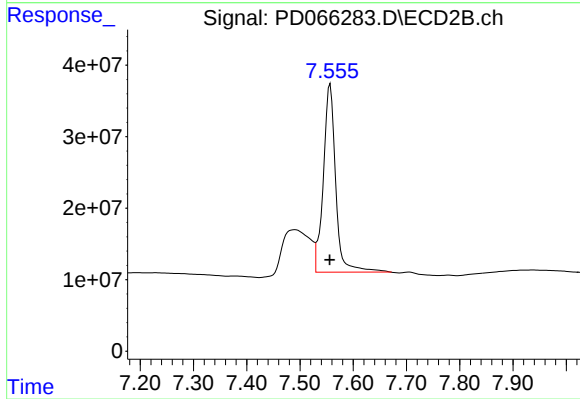

#20 Methoxychlor


R.T.: 7.557 min
Delta R.T.: 0.000 min
Response: 426378262
Conc: 131.25 ng/ml

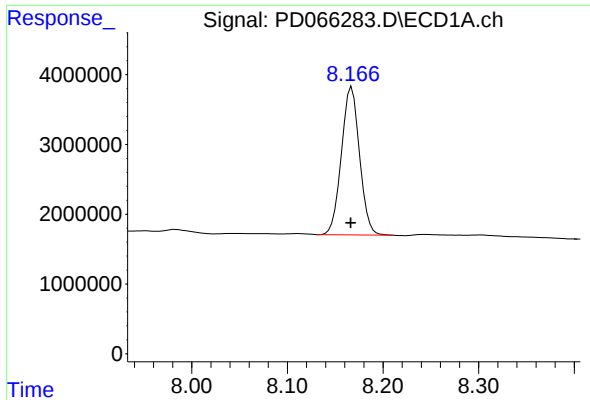

#27 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: 0.000 min
Response: 27940352
Conc: 20.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

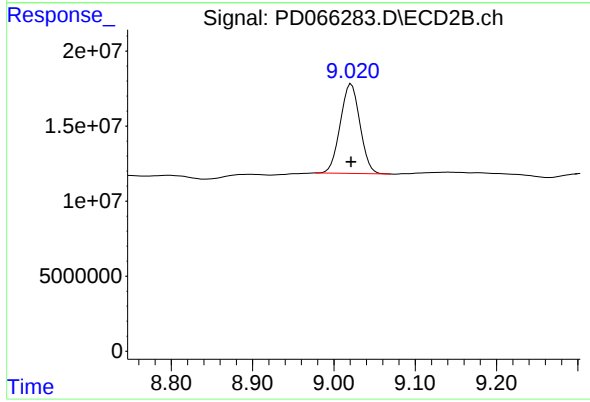

#27 Decachlorobiphenyl

R.T.: 9.021 min
Delta R.T.: 0.000 min
Response: 99909347
Conc: 20.42 ng/ml