

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
 Data File : PD066285.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2021 10:22
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 23:28:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 18 23:27:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	41067945	180.5E6	20.000	20.000
27)	SA Decachlor...	8.166	9.021	55111141	195.7E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.877	4.363	62802491	234.5E6	20.000	20.000
3)	MA gamma-BHC...	4.159	4.647	60991154	222.8E6	20.000	20.000
4)	MA Heptachlor	4.453	5.147	59263052	206.8E6	20.000	20.000
9)	A Endosulfan I	5.476	6.196	50338986	171.4E6	20.000	20.000
13)	MA Dieldrin	5.718	6.454	108.9E6	341.8E6	40.000	40.000
14)	MA Endrin	5.975	6.671	95001732	224.9E6	40.000	40.000
16)	A 4,4'-DDD	6.099	6.798	84369586	270.1E6	40.000	40.000
17)	MA 4,4'-DDT	6.338	7.095	81323984	263.1E6	40.000	40.000
20)	A Methoxychlor	6.886	7.556	212.0E6	649.7E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
Data File : PD066285.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2021 10:22
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 23:28:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
Quant Title : GC Extractables
QLast Update : Mon Oct 18 23:27:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

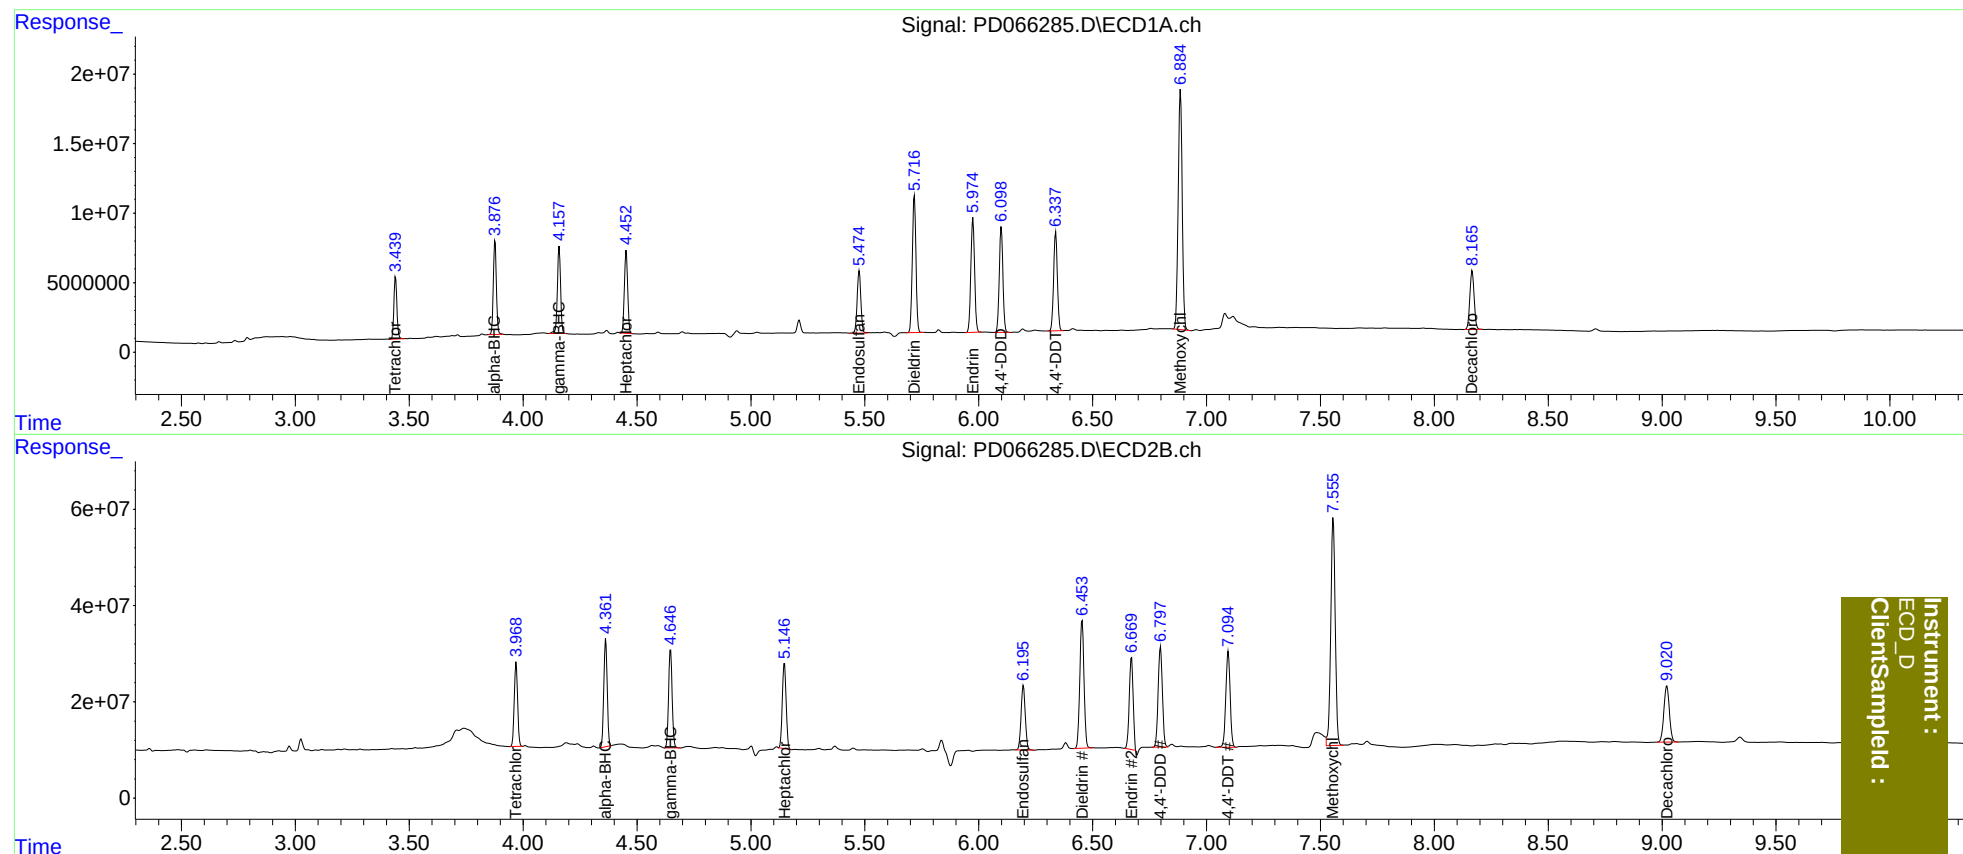


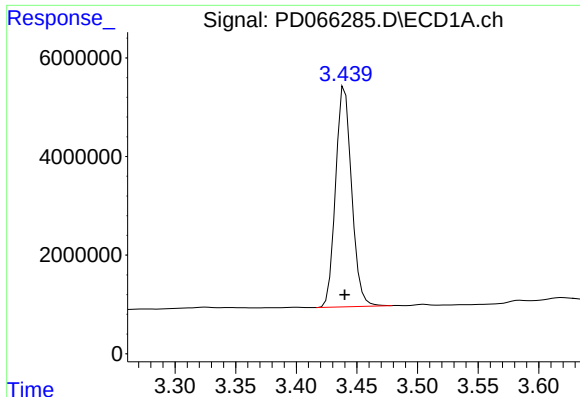

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 41067945
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

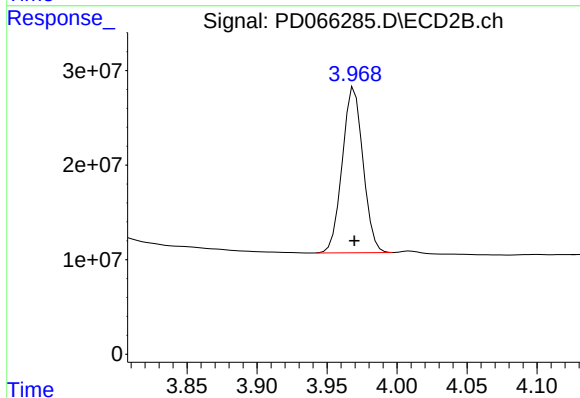


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 180487406
Conc: 20.00 ng/ml

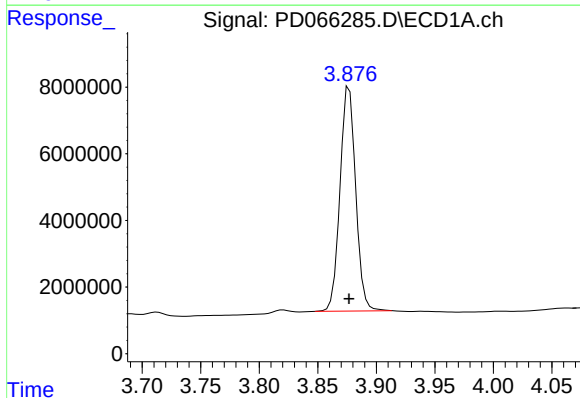


#2 alpha-BHC

R.T.: 3.877 min
Delta R.T.: 0.000 min
Response: 62802491
Conc: 20.00 ng/ml

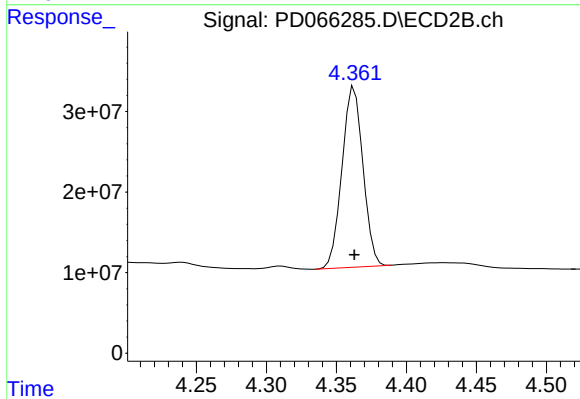

#2 alpha-BHC


R.T.: 4.363 min
Delta R.T.: 0.000 min
Response: 234467438
Conc: 20.00 ng/ml

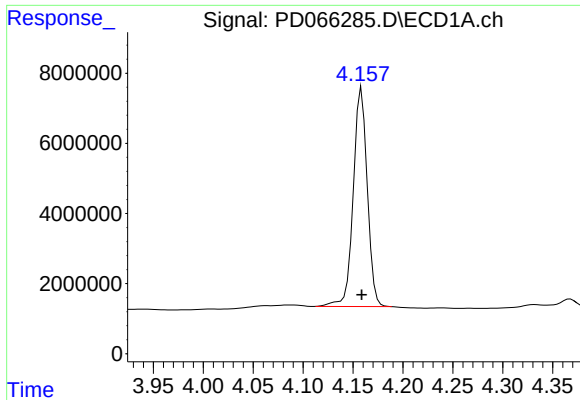

#3 gamma-BHC (Lindane)


R.T.: 4.159 min
Delta R.T.: 0.000 min
Response: 60991154
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

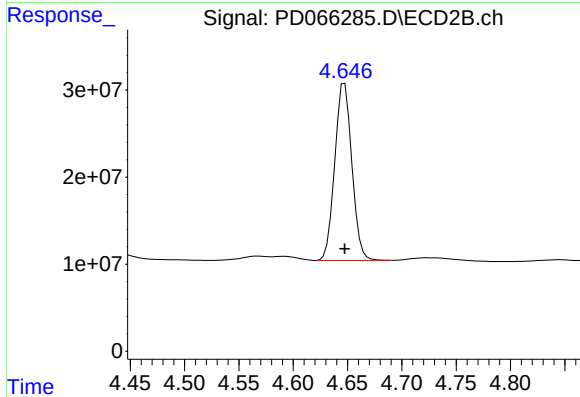


#3 gamma-BHC (Lindane)

R.T.: 4.647 min
Delta R.T.: 0.000 min
Response: 222831247
Conc: 20.00 ng/ml

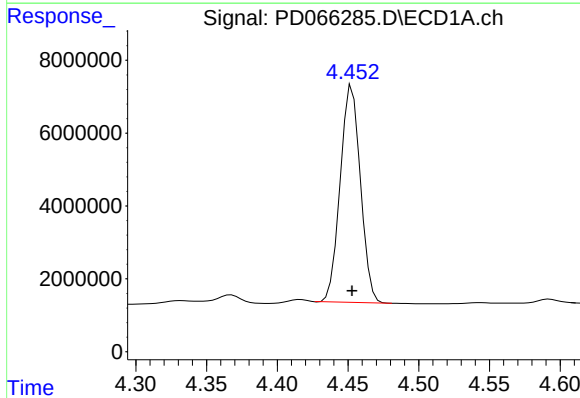


#4 Heptachlor

R.T.: 4.453 min
Delta R.T.: 0.000 min
Response: 59263052
Conc: 20.00 ng/ml

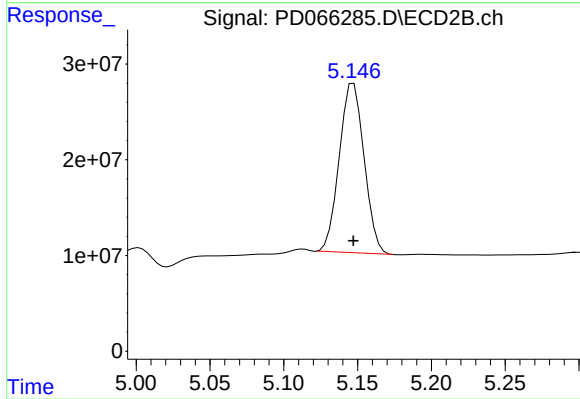

#4 Heptachlor


R.T.: 5.147 min
Delta R.T.: 0.000 min
Response: 206806081
Conc: 20.00 ng/ml

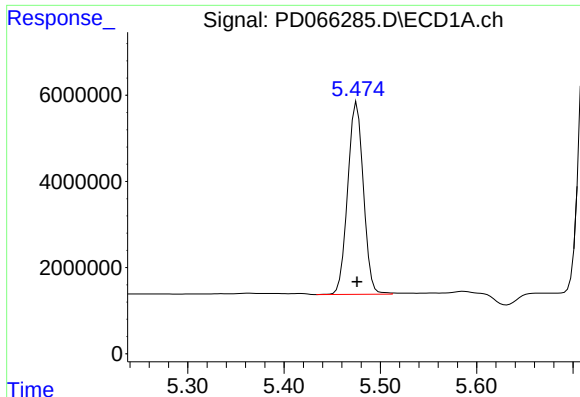

#9 Endosulfan I


R.T.: 5.476 min
Delta R.T.: 0.000 min
Response: 50338986
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

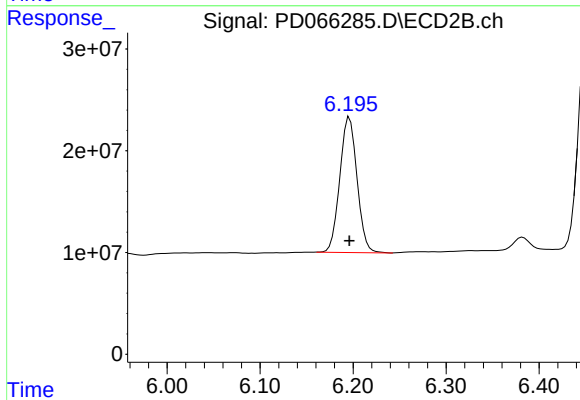


#9 Endosulfan I

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 171399662
Conc: 20.00 ng/ml

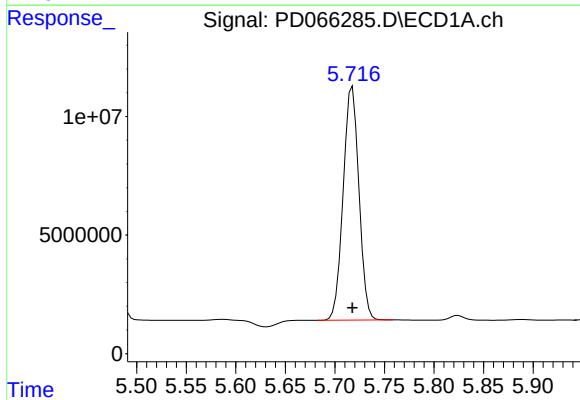


#13 Dieldrin

R.T.: 5.718 min
Delta R.T.: 0.000 min
Response: 108933566
Conc: 40.00 ng/ml

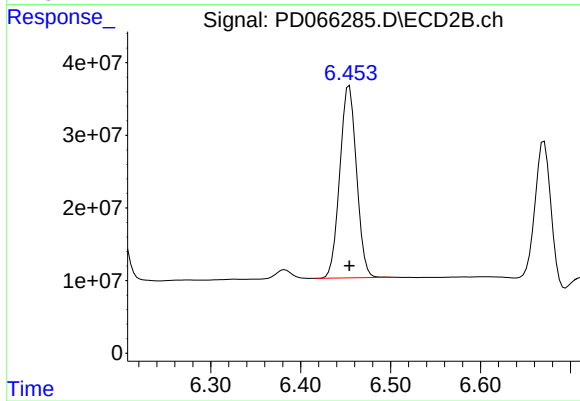

#13 Dieldrin


R.T.: 6.454 min
Delta R.T.: 0.000 min
Response: 341796757
Conc: 40.00 ng/ml

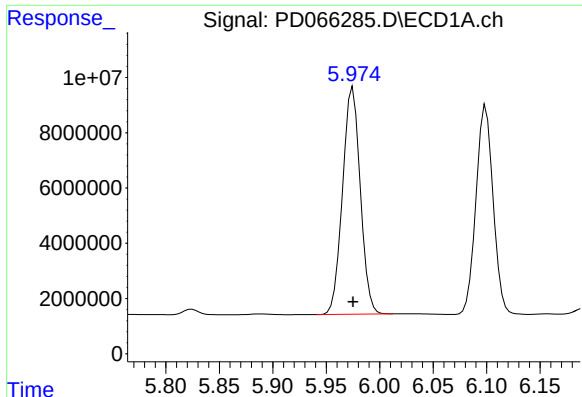

#14 Endrin


R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 95001732
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

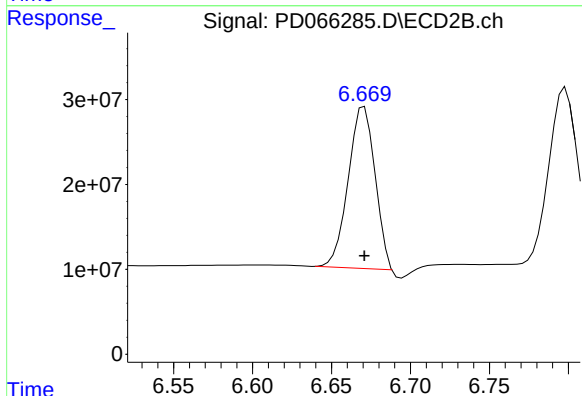


#14 Endrin

R.T.: 6.671 min
Delta R.T.: 0.000 min
Response: 224940042
Conc: 40.00 ng/ml

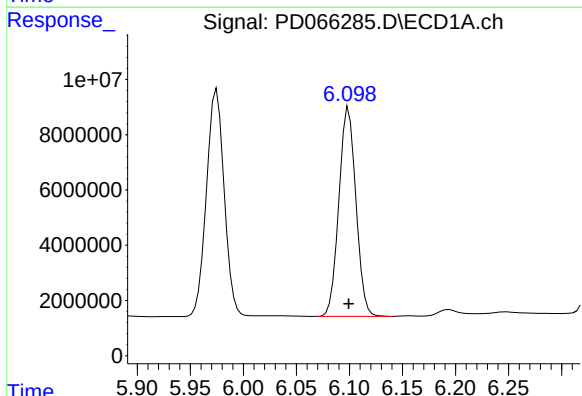


#16 4,4'-DDD

R.T.: 6.099 min
Delta R.T.: 0.000 min
Response: 84369586
Conc: 40.00 ng/ml

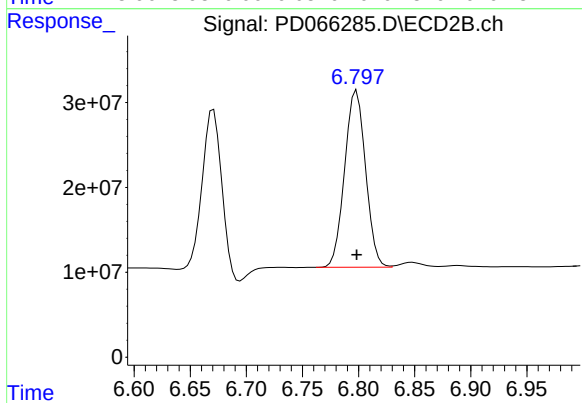

#16 4,4'-DDD


R.T.: 6.798 min
Delta R.T.: 0.000 min
Response: 270139291
Conc: 40.00 ng/ml

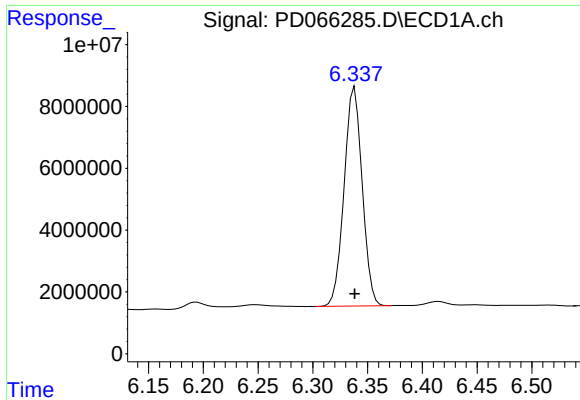

#17 4,4'-DDT


R.T.: 6.338 min
Delta R.T.: 0.000 min
Response: 81323984
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

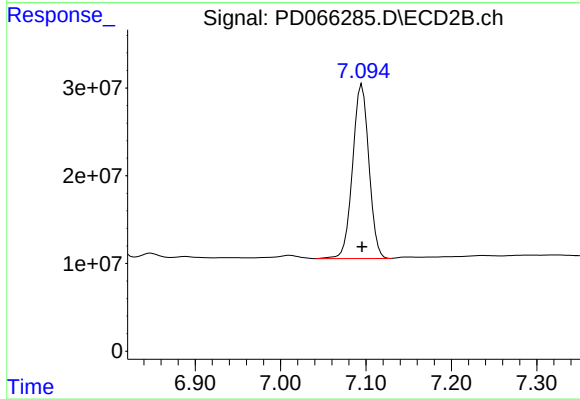


#17 4,4'-DDT

R.T.: 7.095 min
Delta R.T.: 0.000 min
Response: 263093618
Conc: 40.00 ng/ml

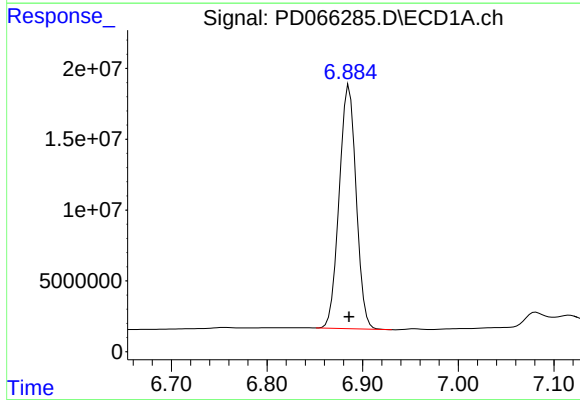


#20 Methoxychlor

R.T.: 6.886 min
Delta R.T.: 0.000 min
Response: 212045557
Conc: 200.00 ng/ml

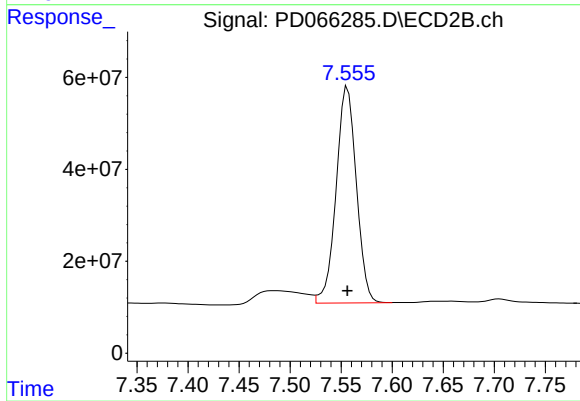

#20 Methoxychlor


R.T.: 7.556 min
Delta R.T.: 0.000 min
Response: 649710307
Conc: 200.00 ng/ml

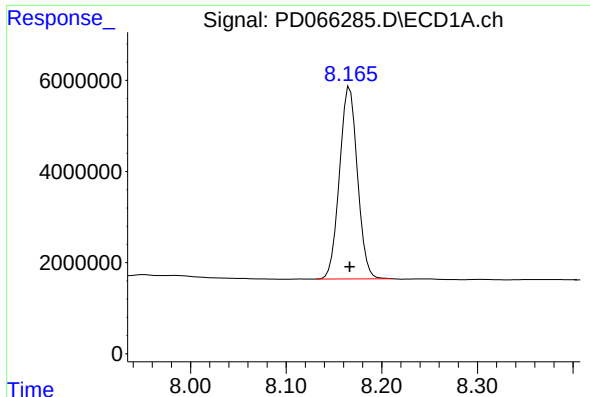

#27 Decachlorobiphenyl

R.T.: 8.166 min
Delta R.T.: 0.000 min
Response: 55111141
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

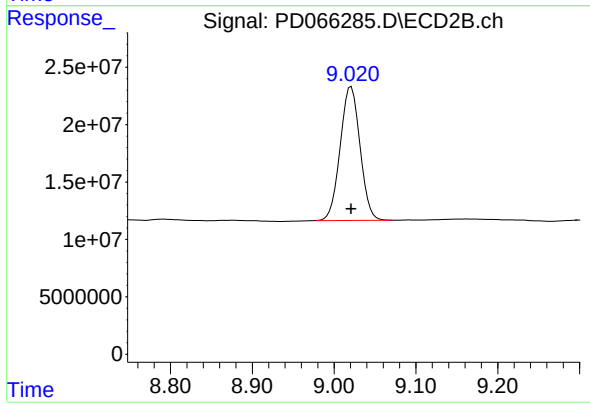

#27 Decachlorobiphenyl

R.T.: 9.021 min
Delta R.T.: 0.000 min
Response: 195710318
Conc: 40.00 ng/ml