

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
 Data File : PD066287.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2021 10:50
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 23:28:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 18 23:27:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	77999954	326.7E6	37.986	36.204
27)	SA Decachlor...	8.166	9.019	103.0E6	357.1E6	74.725	72.979
Target Compounds							
2)	A alpha-BHC	3.877	4.363	123.1E6	431.8E6	39.198	36.834
3)	MA gamma-BHC...	4.159	4.647	116.4E6	406.4E6	38.161	36.477
4)	MA Heptachlor	4.452	5.148	115.6E6	374.6E6	39.018	36.228
9)	A Endosulfan I	5.475	6.196	95868985	308.8E6	38.089	36.028
13)	MA Dieldrin	5.717	6.453	215.2E6	634.9E6	79.028	74.298
14)	MA Endrin	5.974	6.672	178.1E6	402.9E6	74.971	71.649
16)	A 4,4'-DDD	6.099	6.798	165.5E6	506.6E6	78.474	75.017
17)	MA 4,4'-DDT	6.338	7.095	162.9E6	487.1E6	80.147	74.051
20)	A Methoxychlor	6.885	7.555	402.7E6	1136.3E6	379.826	349.797


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
Data File : PD066287.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2021 10:50
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 23:28:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
Quant Title : GC Extractables
QLast Update : Mon Oct 18 23:27:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

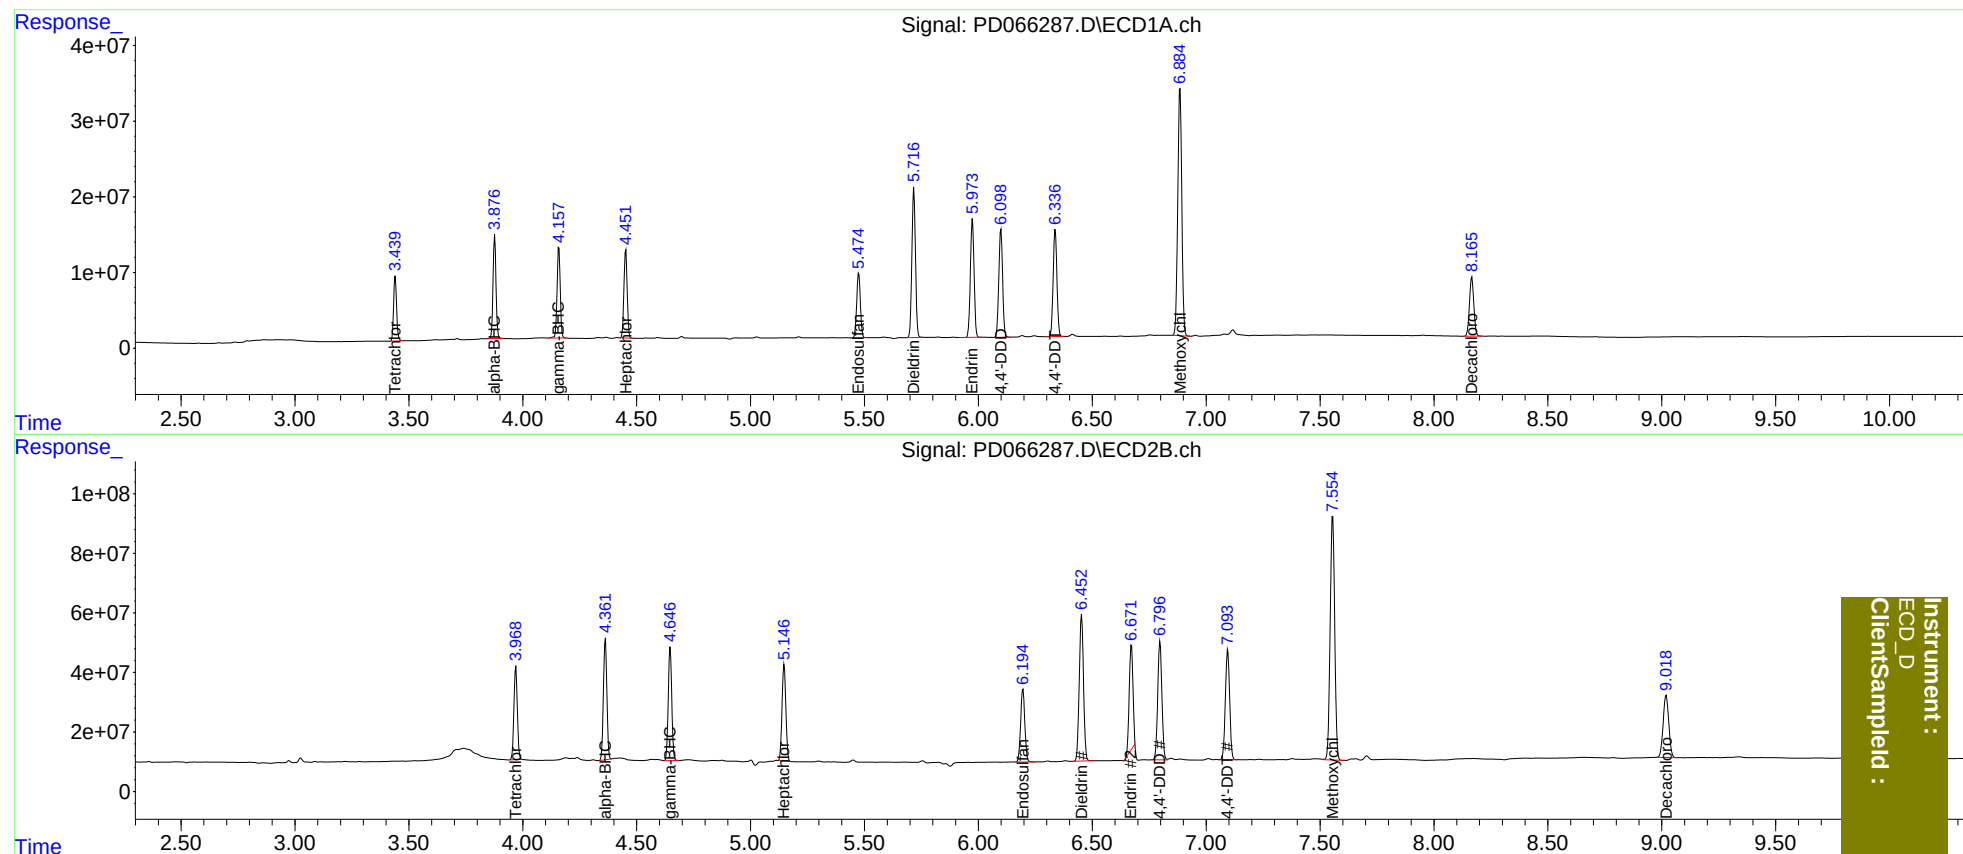


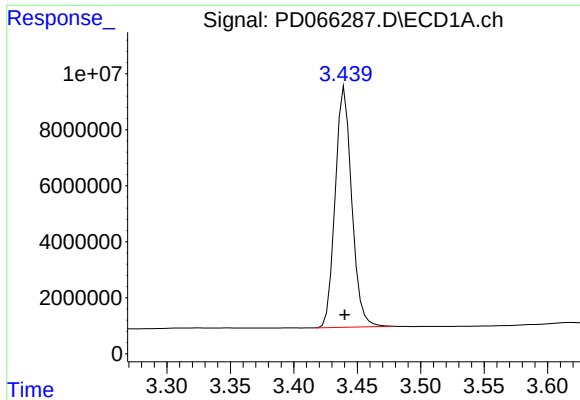

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 77999954
Conc: 37.99 ng/ml

Instrument :
ECD_D
ClientSampleId :

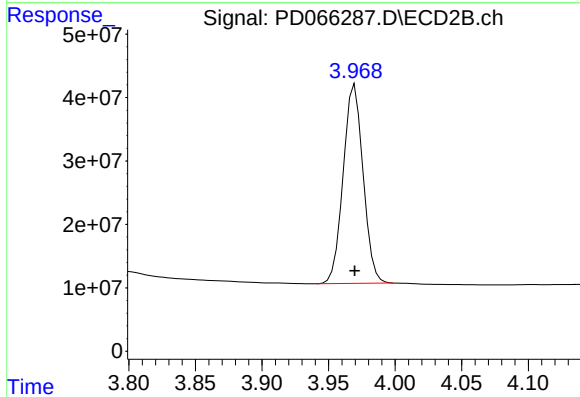


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 326720338
Conc: 36.20 ng/ml

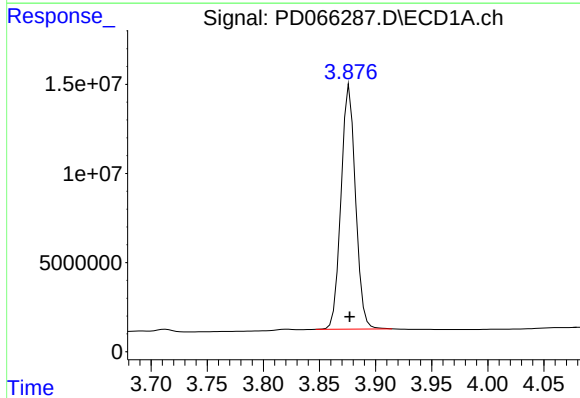


#2 alpha-BHC

R.T.: 3.877 min
Delta R.T.: 0.000 min
Response: 123085299
Conc: 39.20 ng/ml

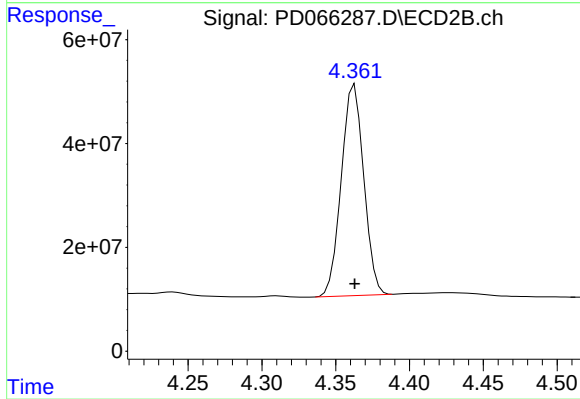

#2 alpha-BHC


R.T.: 4.363 min
Delta R.T.: 0.000 min
Response: 431818472
Conc: 36.83 ng/ml

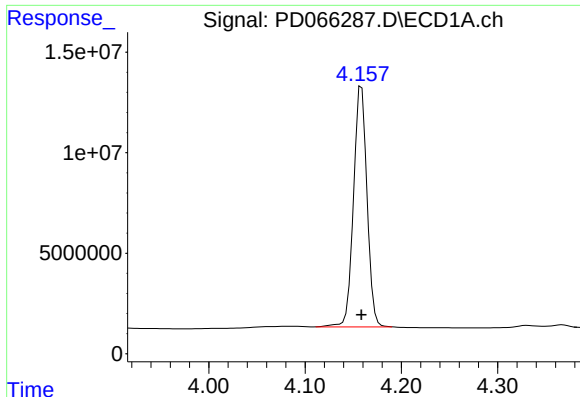

#3 gamma-BHC (Lindane)


R.T.: 4.159 min
Delta R.T.: 0.000 min
Response: 116374265
Conc: 38.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

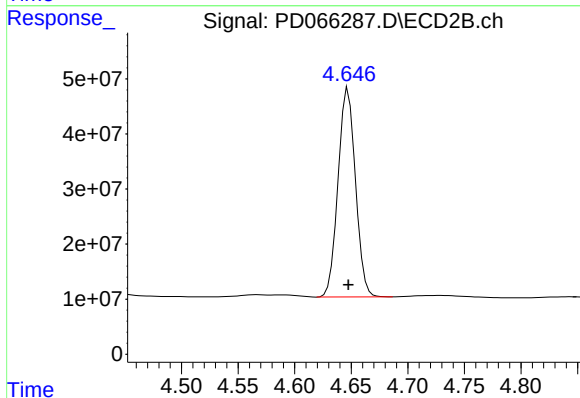


#3 gamma-BHC (Lindane)

R.T.: 4.647 min
Delta R.T.: 0.000 min
Response: 406410621
Conc: 36.48 ng/ml

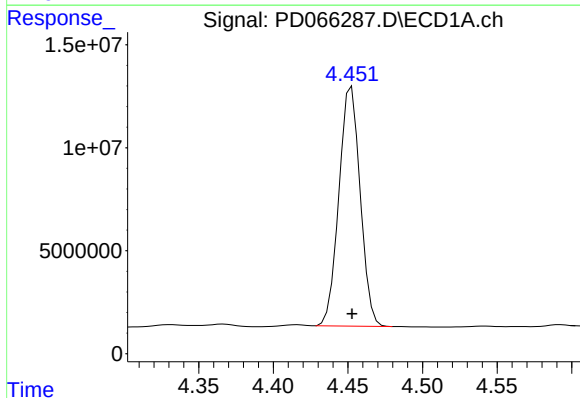


#4 Heptachlor

R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 115617231
Conc: 39.02 ng/ml

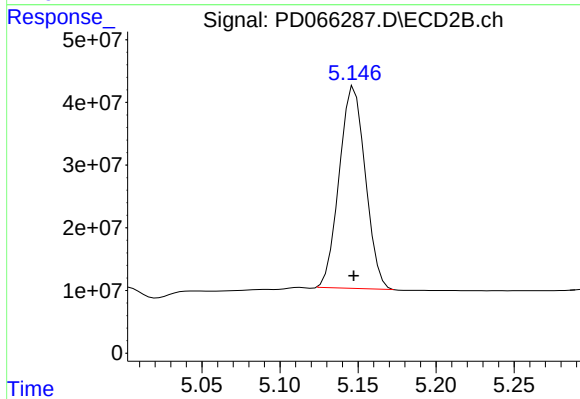

#4 Heptachlor


R.T.: 5.148 min
Delta R.T.: 0.000 min
Response: 374611863
Conc: 36.23 ng/ml

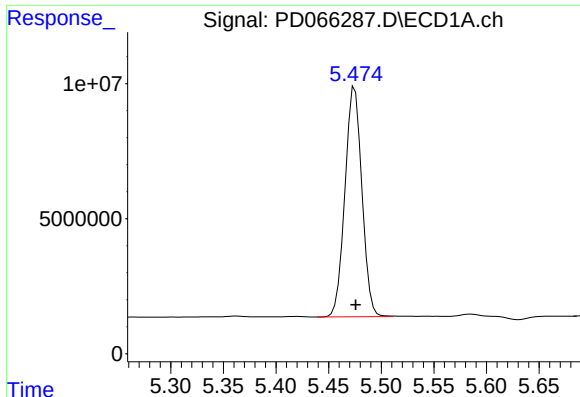

#9 Endosulfan I


R.T.: 5.475 min
Delta R.T.: 0.000 min
Response: 95868985
Conc: 38.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

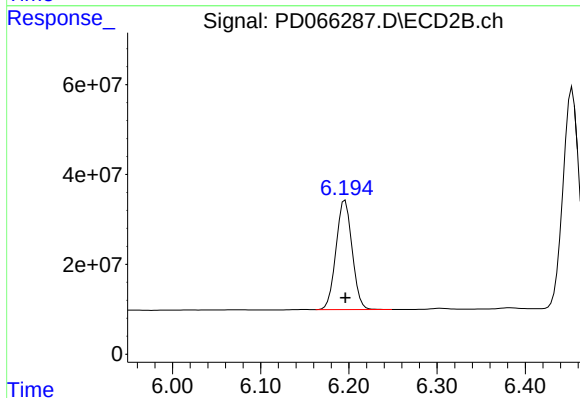


#9 Endosulfan I

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 308757764
Conc: 36.03 ng/ml

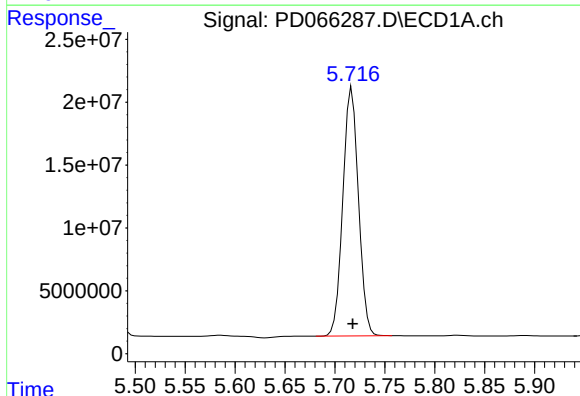


#13 Dieldrin

R.T.: 5.717 min
Delta R.T.: 0.000 min
Response: 215219273
Conc: 79.03 ng/ml

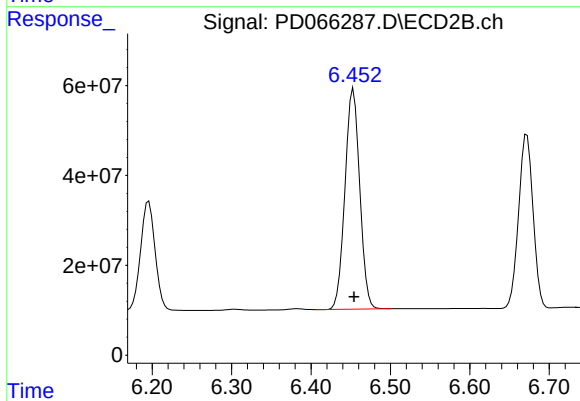

#13 Dieldrin


R.T.: 6.453 min
Delta R.T.: 0.000 min
Response: 634868394
Conc: 74.30 ng/ml

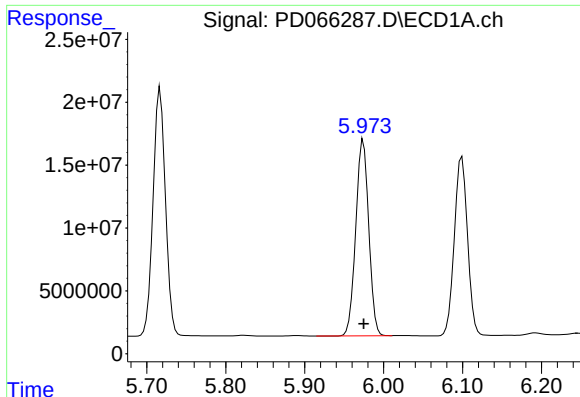

#14 Endrin


R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 178058589
Conc: 74.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

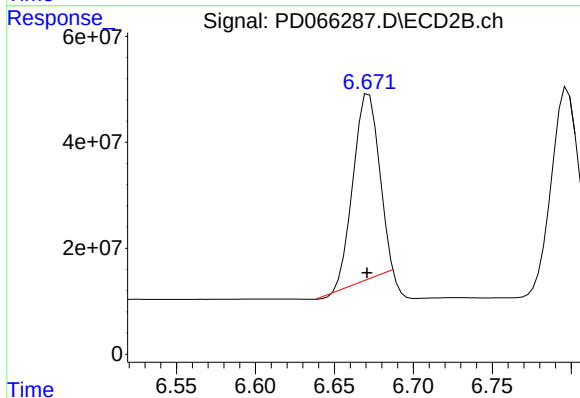


#14 Endrin

R.T.: 6.672 min
Delta R.T.: 0.001 min
Response: 402916119
Conc: 71.65 ng/ml

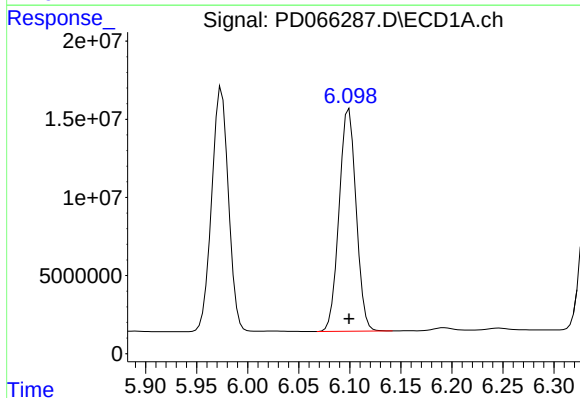


#16 4,4'-DDD

R.T.: 6.099 min
Delta R.T.: 0.000 min
Response: 165520808
Conc: 78.47 ng/ml

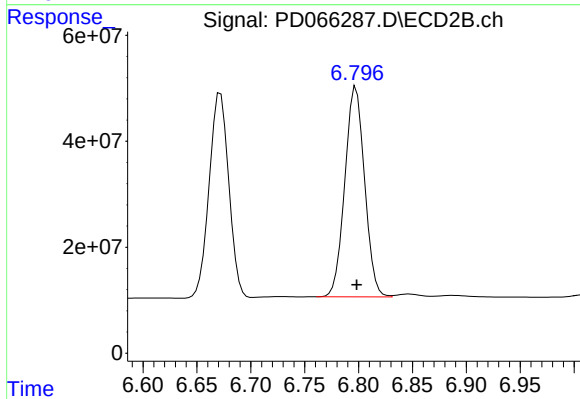

#16 4,4'-DDD


R.T.: 6.798 min
Delta R.T.: 0.000 min
Response: 506623405
Conc: 75.02 ng/ml

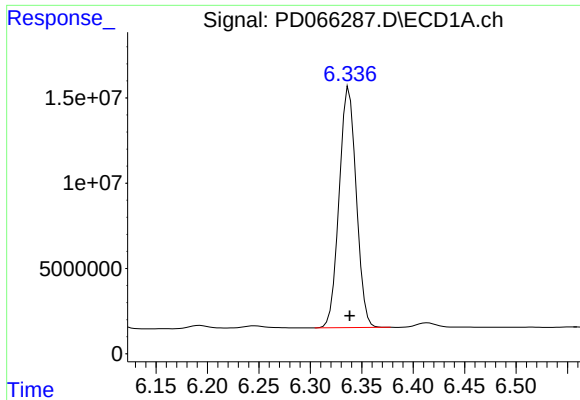

#17 4,4'-DDT


R.T.: 6.338 min
Delta R.T.: 0.000 min
Response: 162946782
Conc: 80.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

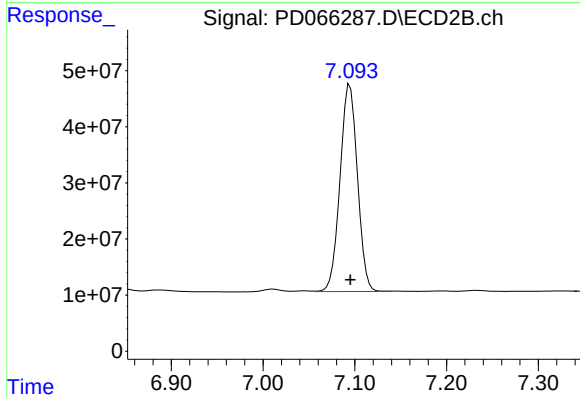


#17 4,4'-DDT

R.T.: 7.095 min
Delta R.T.: 0.000 min
Response: 487060292
Conc: 74.05 ng/ml

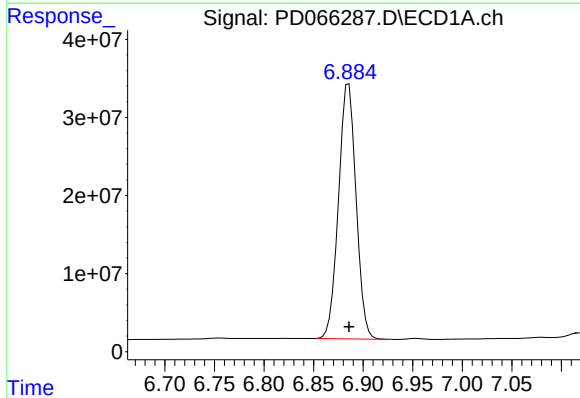


#20 Methoxychlor

R.T.: 6.885 min
Delta R.T.: 0.000 min
Response: 402702158
Conc: 379.83 ng/ml

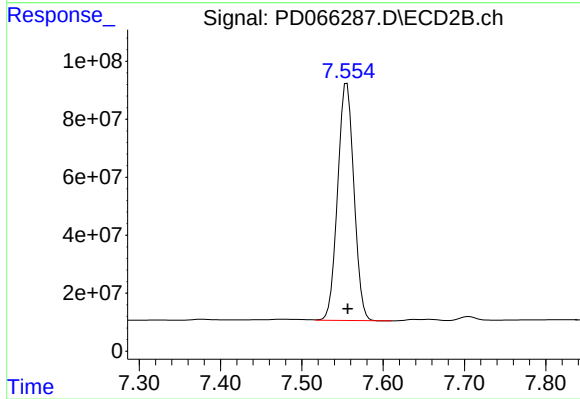

#20 Methoxychlor


R.T.: 7.555 min
Delta R.T.: 0.000 min
Response: 1136334972
Conc: 349.80 ng/ml

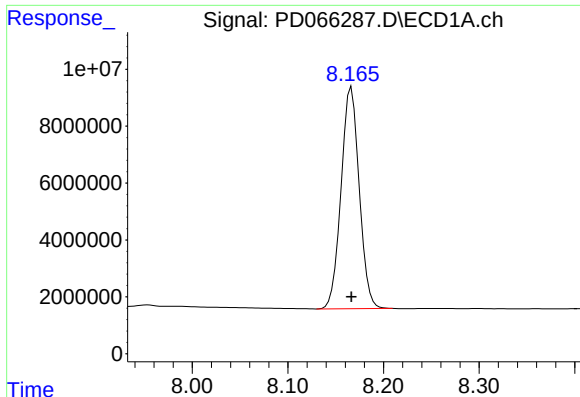

#27 Decachlorobiphenyl

R.T.: 8.166 min
Delta R.T.: 0.000 min
Response: 102953987
Conc: 74.72 ng/ml

Instrument :
ECD_D
ClientSampleId :

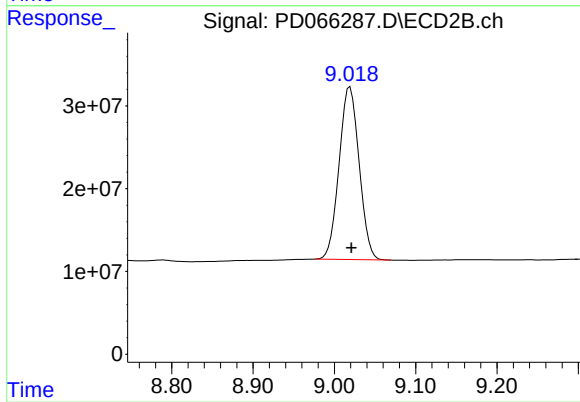

#27 Decachlorobiphenyl

R.T.: 9.019 min
Delta R.T.: -0.002 min
Response: 357066887
Conc: 72.98 ng/ml